


Data Path : Z:\HPCHEM1\BNA_M\Data\BM030415\
 Data File : BM000641.D
 Acq On : 04 Mar 2015 09:40
 Operator : TP/IZ
 Sample : DFTPP30
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-SIM-BM030315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 04 02:50:23 2015

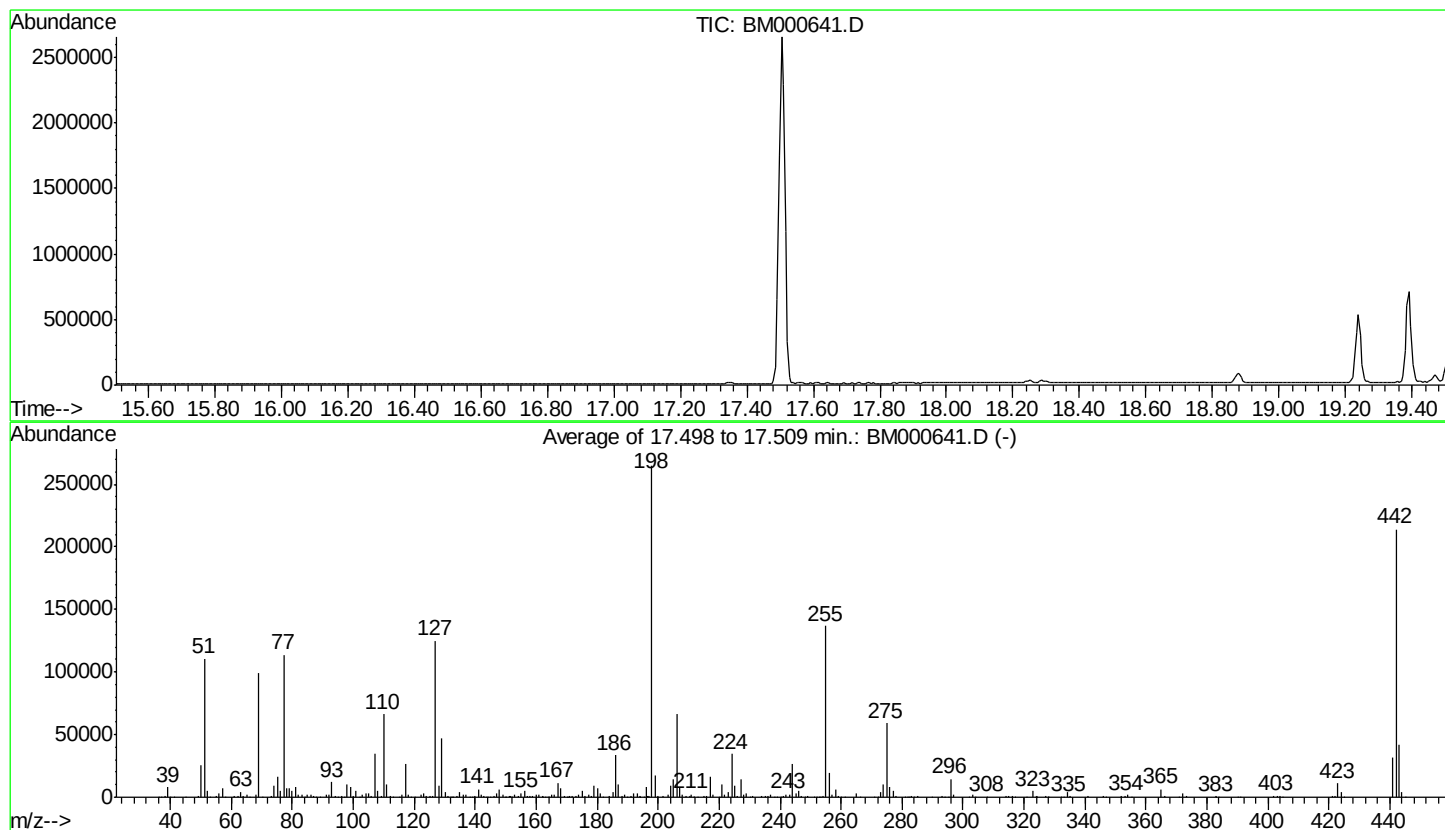

AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.9	110888	PASS
68	69	0.00	2	1.8	1757	PASS
69	198	0.00	100	37.5	99216	PASS
70	69	0.00	2	0.5	496	PASS
127	198	10	80	47.1	124829	PASS
197	198	0.00	1	0.3	899	PASS
198	198	100	100	100.0	264853	PASS
199	198	5	9	6.8	17890	PASS
275	198	10	60	22.3	59157	PASS
365	198	1	100	2.3	6186	PASS
441	443	0.01	100	76.6	32181	PASS
442	198	50	100	80.7	213813	PASS
443	442	15	24	19.6	41986	PASS