


Data Path : Z:\HPCHEM1\BNA\_M\Data\BM030415\  
Data File : BM000641.D  
Acq On : 04 Mar 2015 09:40  
Operator : TP/IZ  
Sample : DFTPP30  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM01.2-EPA-SIM-BM030315.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Wed Mar 04 02:50:23 2015

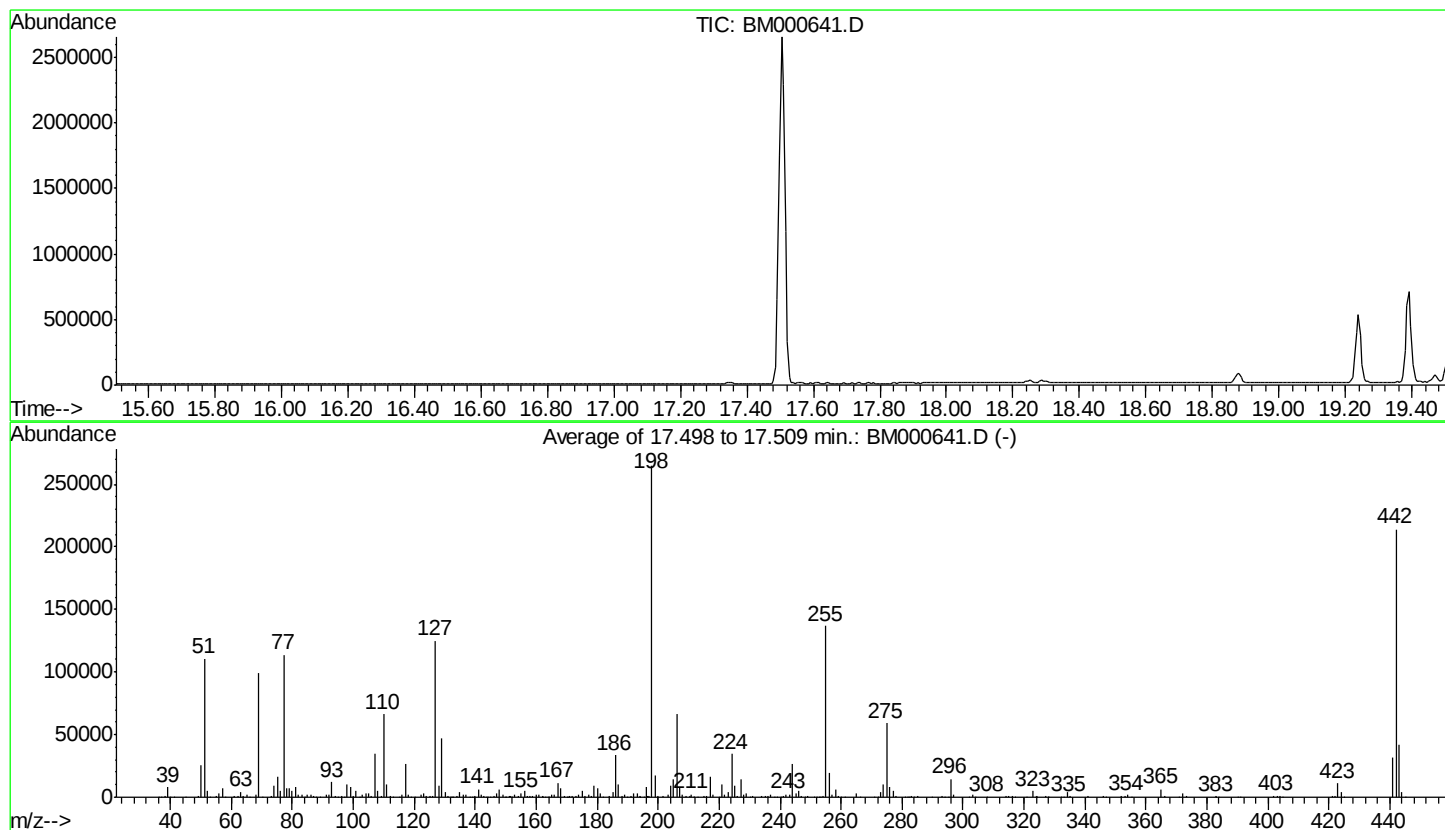

AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2512

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 41.9      | 110888  | PASS             |
| 68          | 69           | 0.00         | 2            | 1.8       | 1757    | PASS             |
| 69          | 198          | 0.00         | 100          | 37.5      | 99216   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.5       | 496     | PASS             |
| 127         | 198          | 10           | 80           | 47.1      | 124829  | PASS             |
| 197         | 198          | 0.00         | 1            | 0.3       | 899     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 264853  | PASS             |
| 199         | 198          | 5            | 9            | 6.8       | 17890   | PASS             |
| 275         | 198          | 10           | 60           | 22.3      | 59157   | PASS             |
| 365         | 198          | 1            | 100          | 2.3       | 6186    | PASS             |
| 441         | 443          | 0.01         | 100          | 76.6      | 32181   | PASS             |
| 442         | 198          | 50           | 100          | 80.7      | 213813  | PASS             |
| 443         | 442          | 15           | 24           | 19.6      | 41986   | PASS             |