

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030419\
 Data File : BM019029.D
 Acq On : 05 Mar 2019 03:29
 Operator : JU/SJ
 Sample : K1688-08
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Mar 05 04:54:06 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 05 03:36:13 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	213218	20.00	ng	0.00
21) Naphthalene-d8	10.46	136	834411	20.00	ng	0.00
39) Acenaphthene-d10	14.33	164	488114	20.00	ng	0.00
64) Phenanthrene-d10	17.09	188	1091765	20.00	ng	0.00
76) Chrysene-d12	21.28	240	885750	20.00	ng	0.00
87) Perylene-d12	23.53	264	891123	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.28	112	1959225	150.56	ng	0.00
7) Phenol-d6	6.86	99	2518460	137.38	ng	0.00
23) Nitrobenzene-d5	8.85	82	1887434	104.59	ng	0.00
42) 2,4,6-Tribromophenol	15.83	330	1153444	163.93	ng	0.00
45) 2-Fluorobiphenyl	12.95	172	3714026	101.01	ng	0.00
79) Terphenyl-d14	19.72	244	5684830	132.40	ng	0.00
Target Compounds						
9) Benzaldehyde	6.86	77	6134	Below Cal	Qvalue #	7


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030419\
Data File : BM019029.D
Acq On : 05 Mar 2019 03:29
Operator : JU/SJ
Sample : K1688-08
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Mar 05 04:54:06 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 05 03:36:13 2019
Response via : Initial Calibration

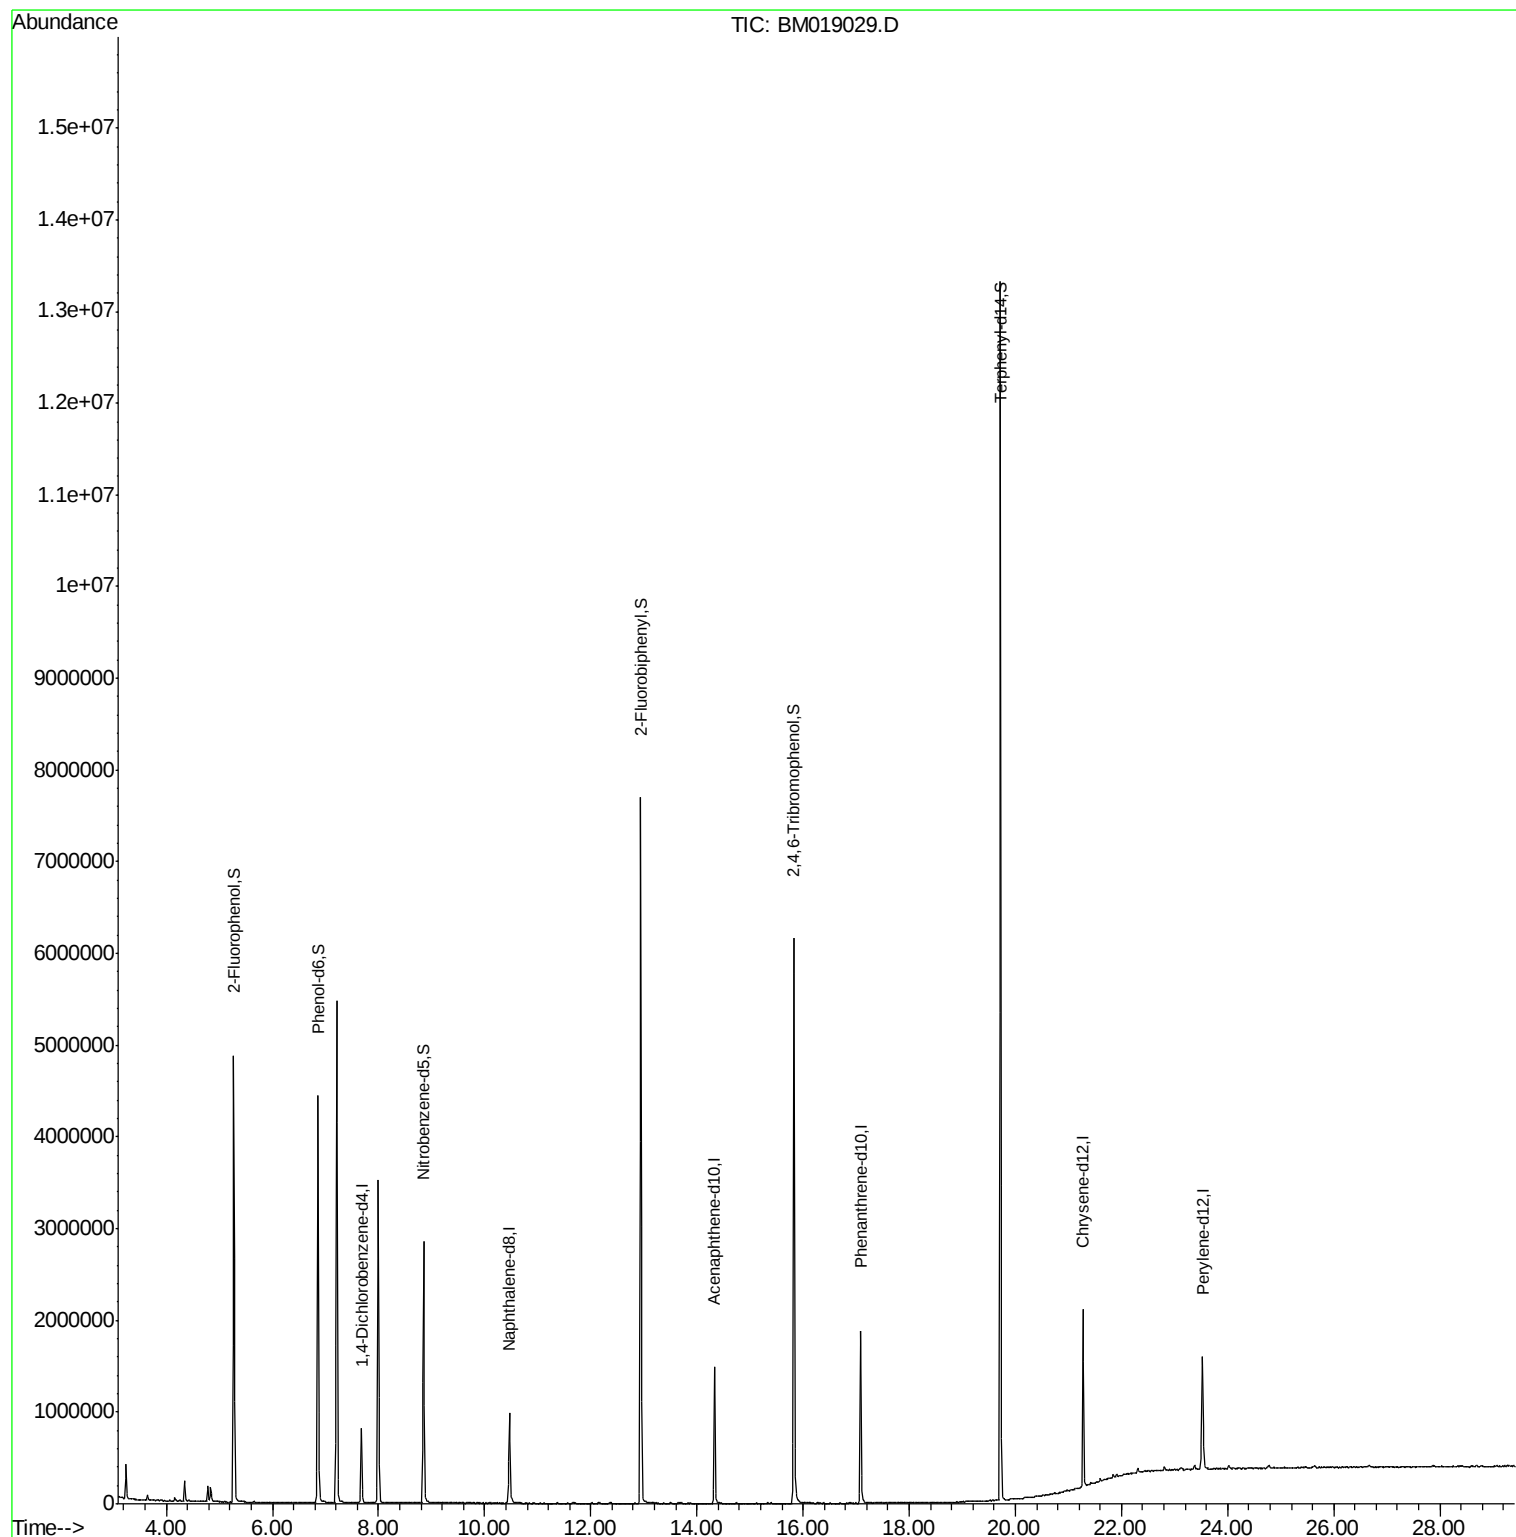




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.68 min Scan# 781
Delta R.T. 0.00 min
Lab File: BM019029.D
Acq: 05 Mar 2019 03:29

Instrument :
BNA_M
ClientSampled :

Tot Ion:152 Resp: 213218
Ion Ratio Lower Upper
152 100
150 156.5 127.3 190.9
115 62.4 50.8 76.2

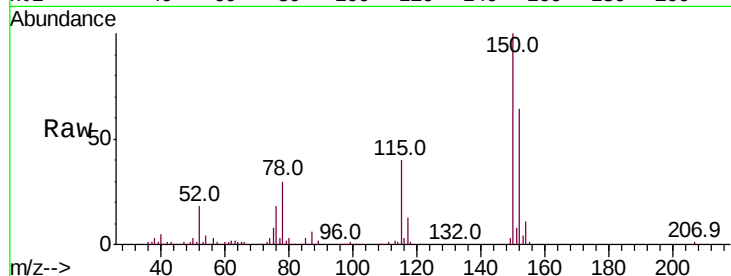


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

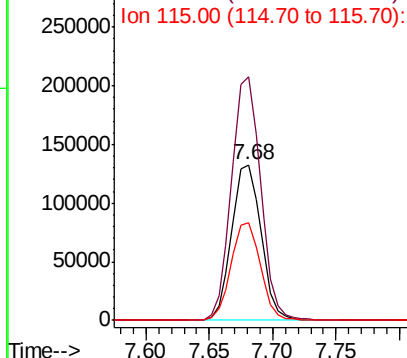



#5


2-Fluorophenol
Concen: 150.557 ng
RT: 5.28 min Scan# 372
Delta R.T. 0.00 min
Lab File: BM019029.D
Acq: 05 Mar 2019 03:29

Tgt Ion:112 Resp: 1959225
Ion Ratio Lower Upper
112 100
64 64.3 50.6 75.8
63 33.1 25.7 38.5



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

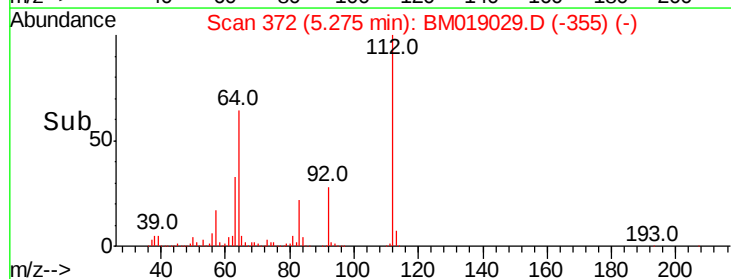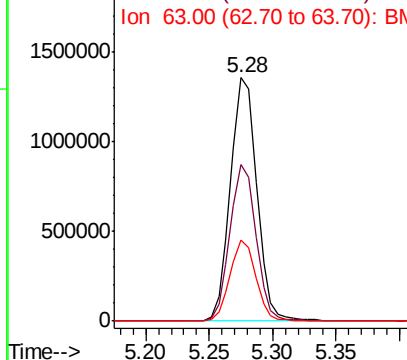



#7

Phenol-d6

Concen: 137.377 ng

RT: 6.86 min Scan# 641

Delta R.T. 0.00 min

Lab File: BM019029.D

Acq: 05 Mar 2019 03:29


Instrument :

BNA_M

ClientSampleId :

Tot Ion: 99 Resp: 2518460

Ion	Ratio	Lower	Upper
99	100		
42	14.3	11.0	16.6
71	37.9	31.3	46.9






Abundance

Ion 99.00 (98.70 to 99.70): BM018755.D (-637) (-)

Ion 42.00 (41.70 to 42.70): BM018755.D (-637) (-)

Ion 71.00 (70.70 to 71.70): BM018755.D (-637) (-)

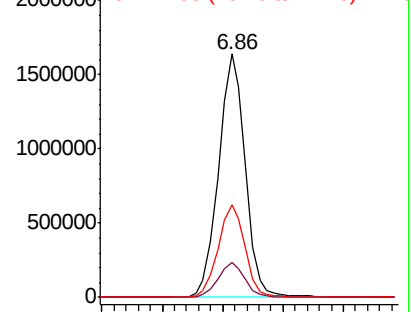

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.46 min Scan# 1254


Delta R.T. -0.01 min

Lab File: BM019029.D

Acq: 05 Mar 2019 03:29

Tgt Ion: 136 Resp: 834411

Ion	Ratio	Lower	Upper
136	100		
137	11.3	8.8	13.2
54	6.7	5.0	7.6
68	7.4	5.5	8.3





Abundance


Ion 136.00 (135.70 to 136.70): BM018755.D (-1252) (-)

Ion 137.00 (136.70 to 137.70): BM018755.D (-1252) (-)

Ion 54.00 (53.70 to 54.70): BM018755.D (-1252) (-)

Ion 68.00 (67.70 to 68.70): BM018755.D (-1252) (-)




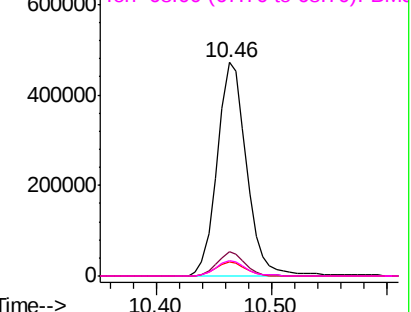




#23
Nitrobenzene-d5
Concen: 104.592 ng
RT: 8.85 min Scan# 979
Delta R.T. -0.01 min
Lab File: BM019029.D
Acq: 05 Mar 2019 03:29




Instrument :
BNA_M
ClientSampled :


Tot Ion: 82 Resp: 1887434
Ion Ratio Lower Upper
82 100
128 36.7 29.9 44.9
54 37.3 29.1 43.7

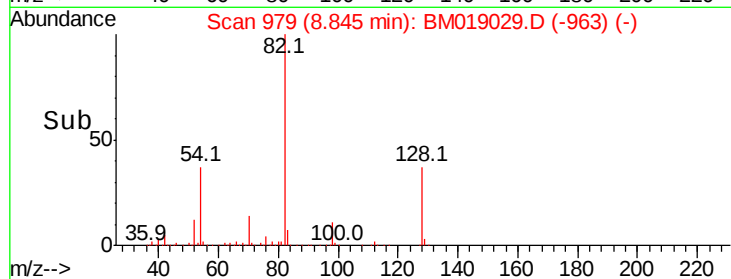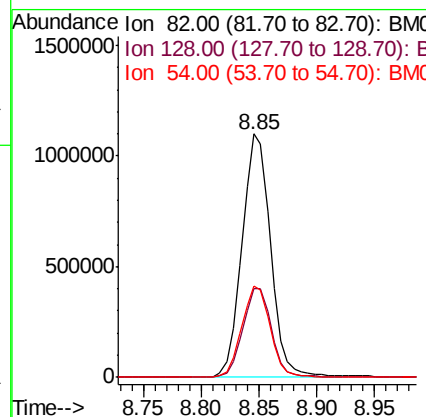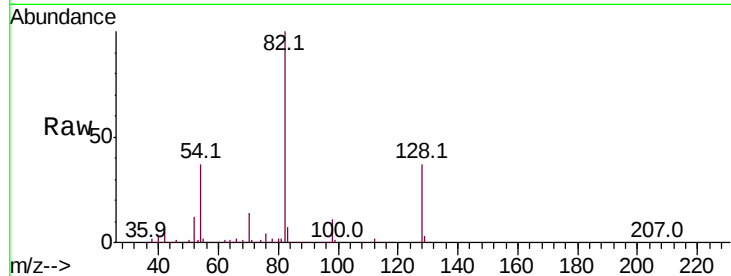

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.33 min Scan# 1911
Delta R.T. -0.01 min
Lab File: BM019029.D
Acq: 05 Mar 2019 03:29

Tgt Ion:164 Resp: 488114
Ion Ratio Lower Upper
164 100
162 105.4 83.4 125.0
160 44.6 36.6 55.0

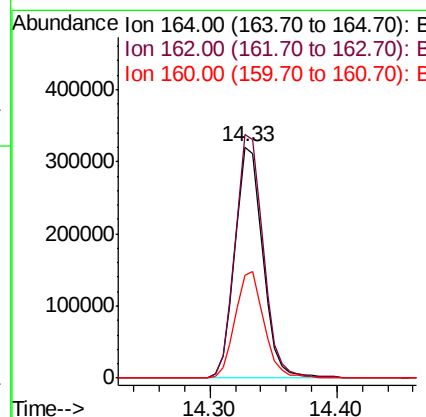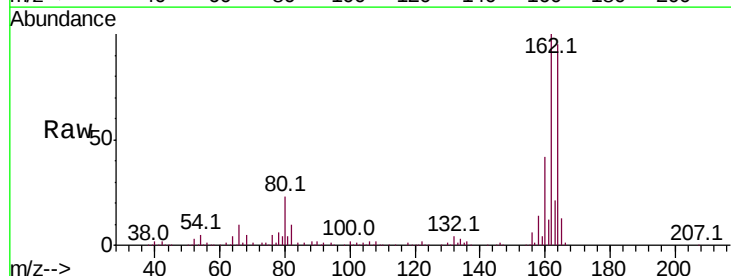


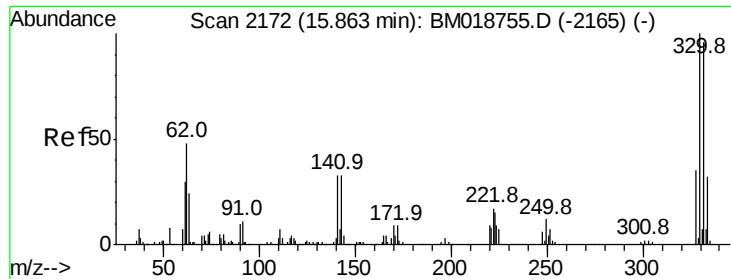




#42
 2,4,6-Tribromophenol
 Concen: 163.934 ng
 RT: 15.83 min Scan# 2167
 Delta R.T. 0.00 min
 Lab File: BM019029.D
 Acq: 05 Mar 2019 03:29

Instrument :
 BNA_M
 ClientSampled :

Tot Ion:330 Resp: 1153444
 Ion Ratio Lower Upper
 330 100
 332 96.4 76.9 115.3
 141 34.1 28.7 43.1

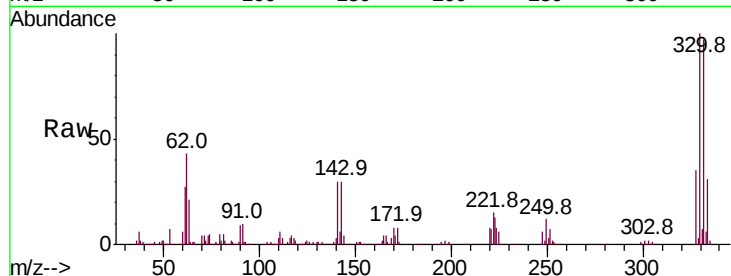


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


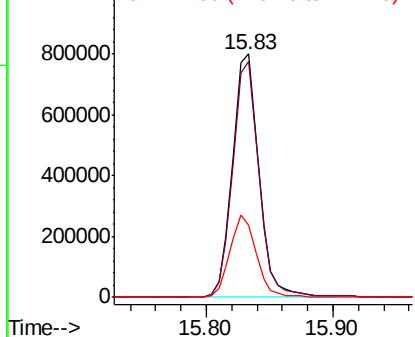



#45
 2-Fluorobiphenyl
 Concen: 101.007 ng
 RT: 12.95 min Scan# 1676
 Delta R.T. -0.01 min
 Lab File: BM019029.D
 Acq: 05 Mar 2019 03:29

Tgt Ion:172 Resp: 3714026
 Ion Ratio Lower Upper
 172 100
 171 36.4 29.0 43.6
 170 23.4 18.6 28.0



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E




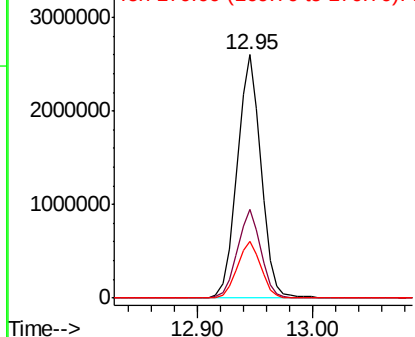


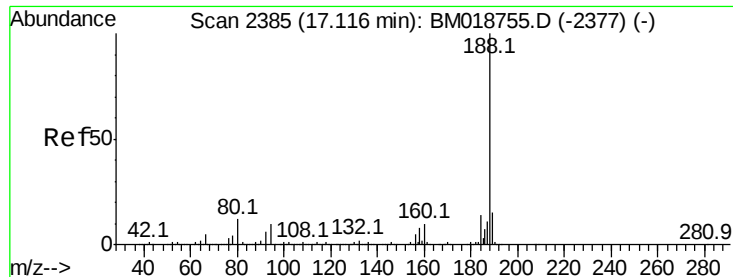

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.09 min Scan# 2380
Delta R.T. 0.00 min
Lab File: BM019029.D
Acq: 05 Mar 2019 03:29




Instrument :
BNA_M
ClientSampleId :


Tot Ion:188 Resp: 1091765
Ion Ratio Lower Upper
188 100
94 10.1 8.2 12.2
80 11.9 9.7 14.5

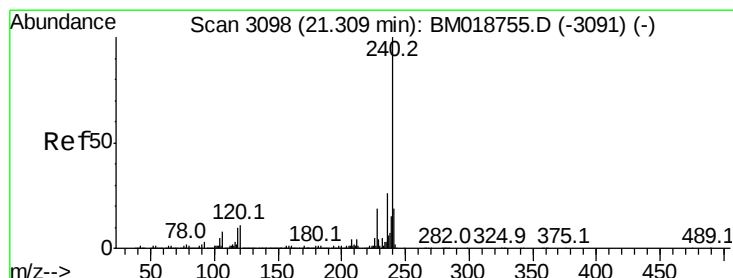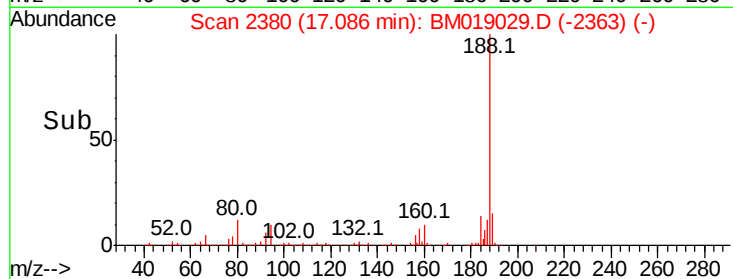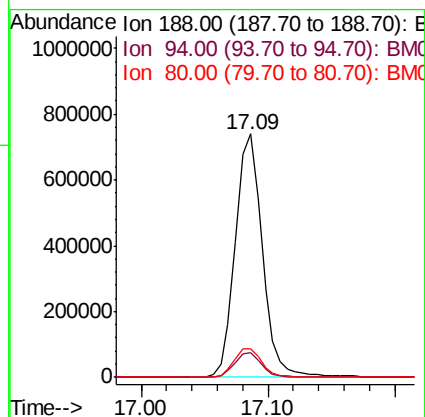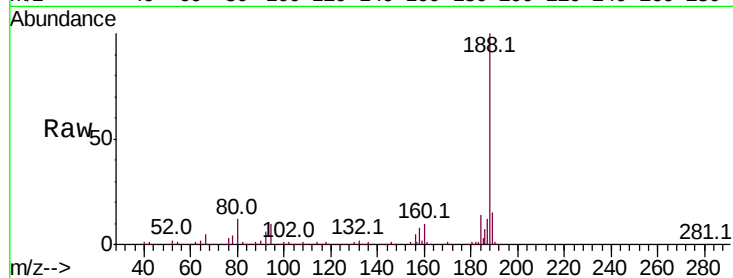

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.28 min Scan# 3093
Delta R.T. -0.01 min
Lab File: BM019029.D
Acq: 05 Mar 2019 03:29

Tgt Ion:240 Resp: 885750
Ion Ratio Lower Upper
240 100
120 10.7 8.9 13.3
236 26.1 20.9 31.3

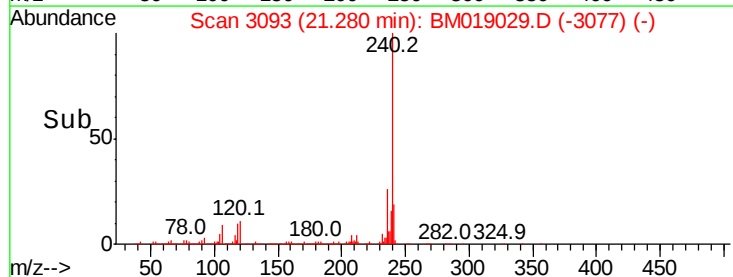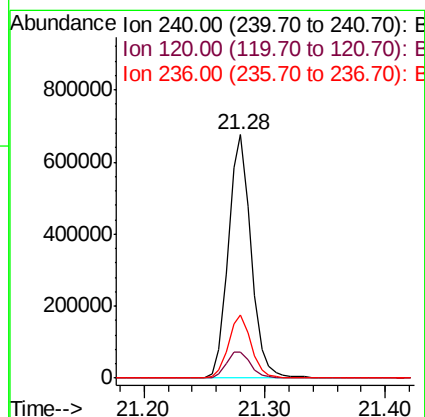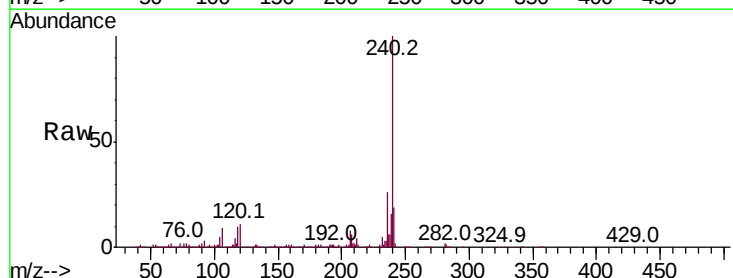



#79

Terphenyl-d14

Concen: 132.399 ng

RT: 19.72 min Scan# 2828

Delta R.T. -0.01 min

Lab File: BM019029.D

Acq: 05 Mar 2019 03:29

Instrument :

BNA_M

ClientSampleId :


Tot Ion:244 Resp: 5684830

Ion Ratio Lower Upper




244 100

212 6.9 5.6 8.4

122 11.3 9.3 13.9

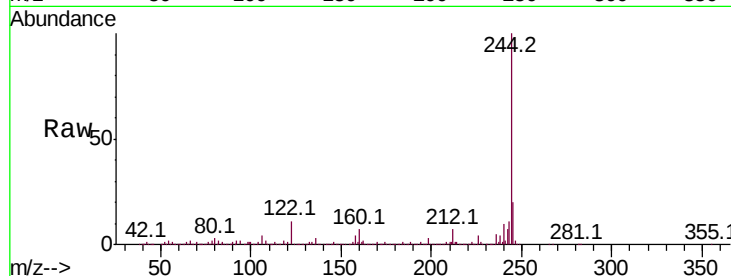

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

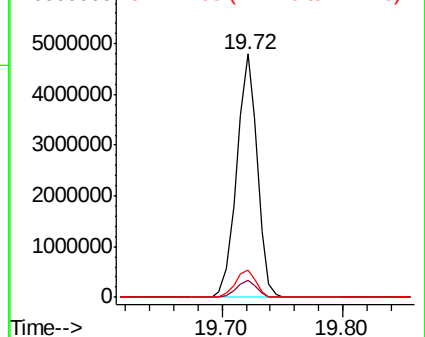

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.53 min Scan# 3475

Delta R.T. -0.01 min

Lab File: BM019029.D

Acq: 05 Mar 2019 03:29


Tgt Ion:264 Resp: 891123

Ion Ratio Lower Upper

264 100

260 23.6 18.9 28.3

265 21.6 17.3 25.9



Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

