
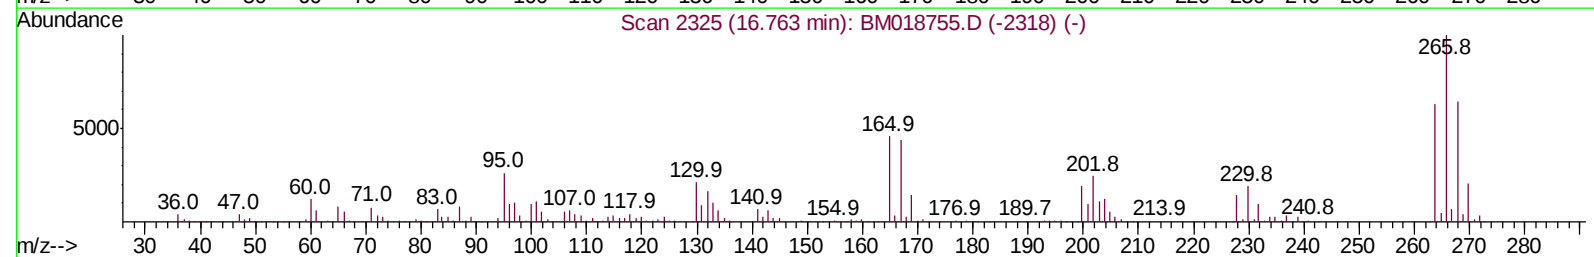
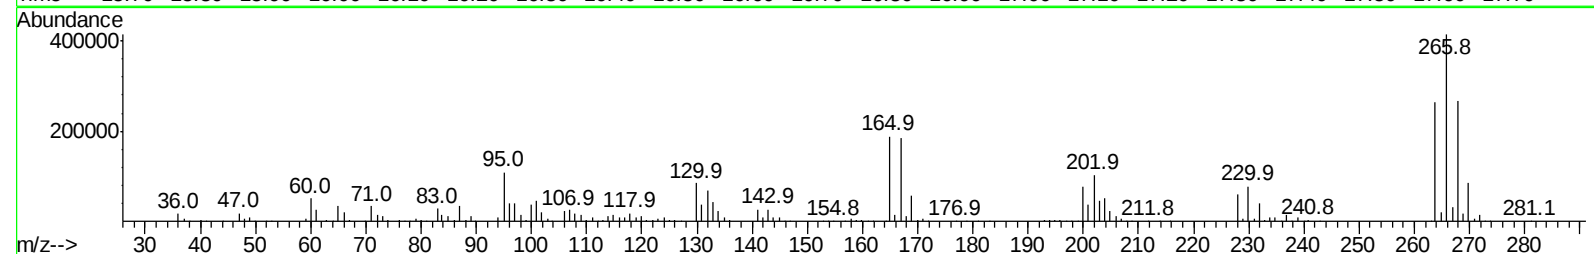


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030419\
 Data File : BM019002.D
 Acq On : 04 Mar 2019 10:40
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 05 07:24:19 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 05 03:36:13 2019
 Response via : Initial Calibration

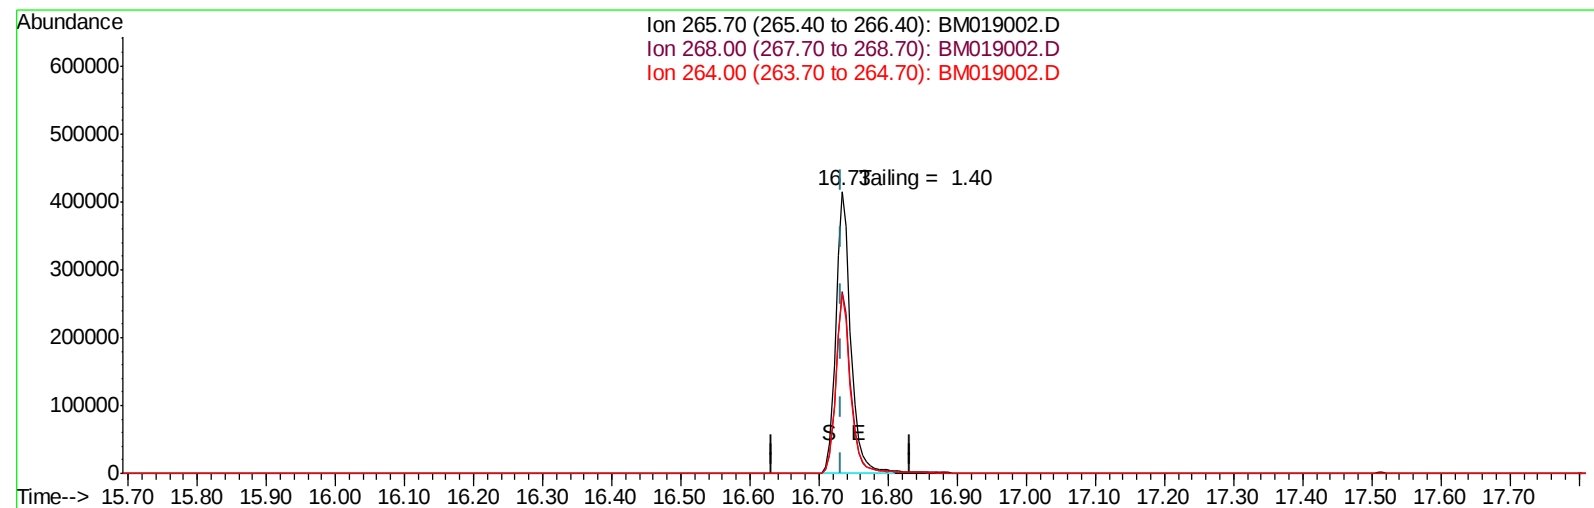

TIC: BM019002.D

(70) Pentachlorophenol (C)




16.733min (+0.000) 160196.07ng

response 620000

Ion	Exp%	Act%
265.70	100	100
268.00	64.10	64.49
264.00	63.20	63.61
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030419\
Data File : BM019002.D
Acq On : 04 Mar 2019 10:40
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 05 07:24:19 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 05 03:36:13 2019
Response via : Initial Calibration

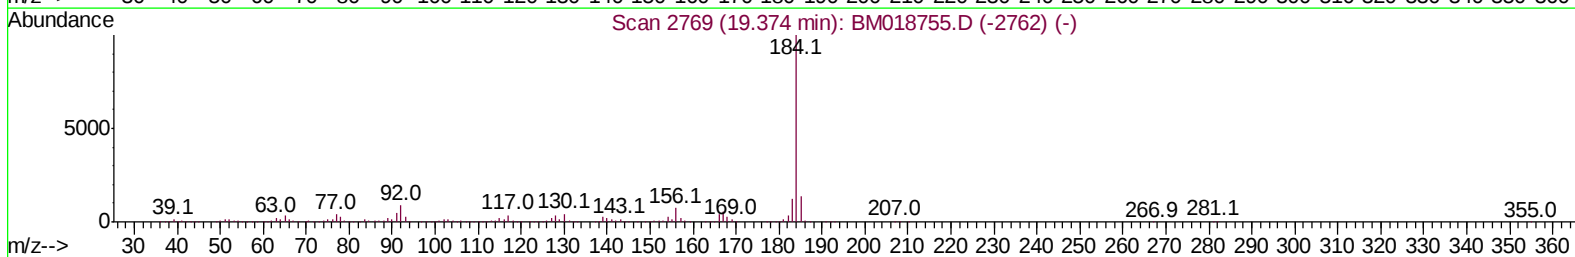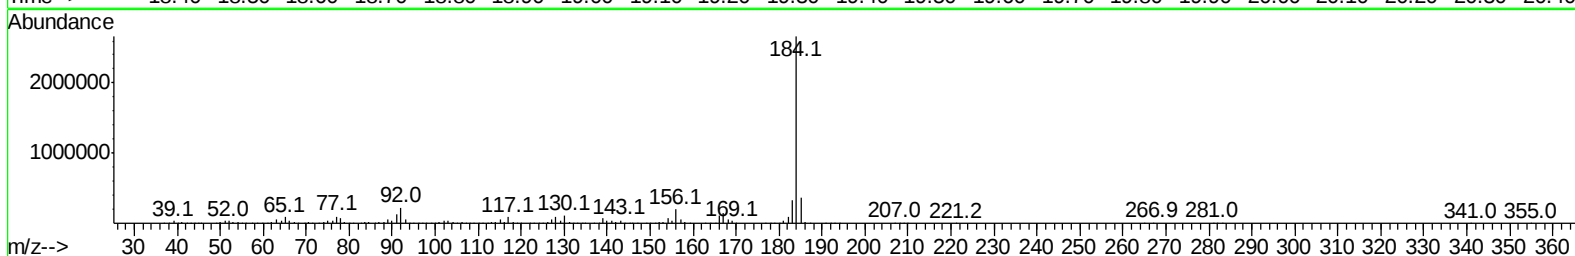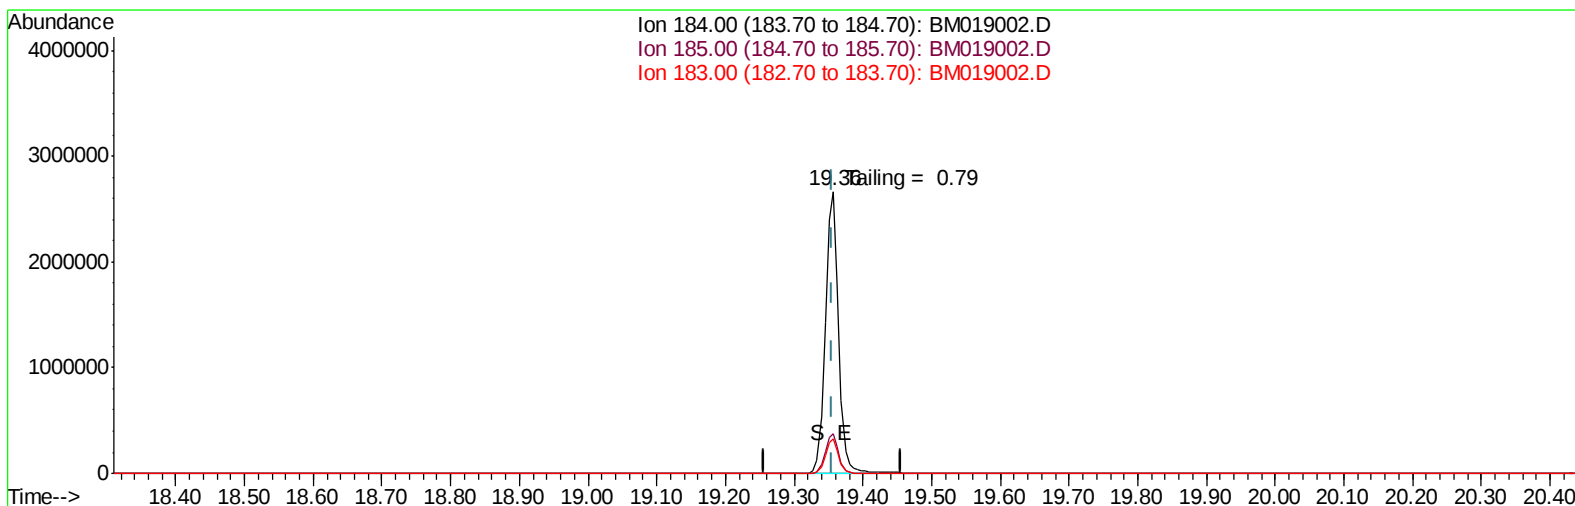

TIC: BM019002.D

(77) Benzidine

19.357min (+0.000) 44233.24ng

response 3573353

Ion	Exp%	Act%
184.00	100	100
185.00	14.00	14.03
183.00	12.10	12.39
0.00	0.00	0.00