
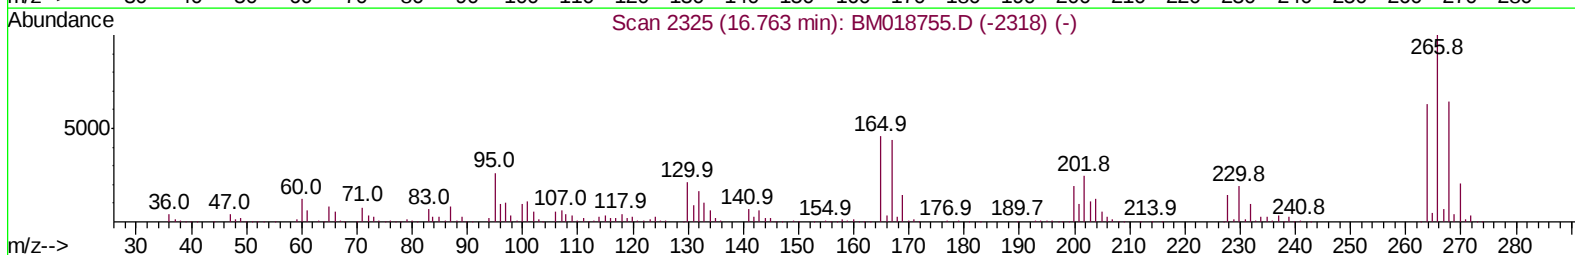
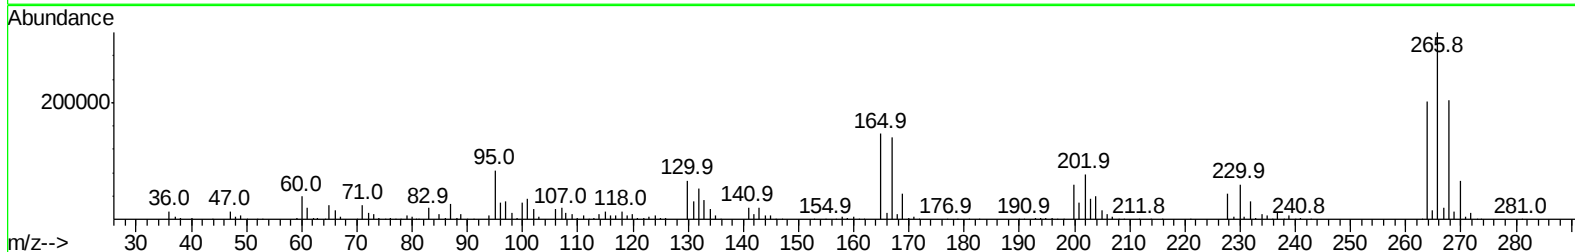


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030419\
Data File : BM019022.D
Acq On : 04 Mar 2019 23:17
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 05 07:26:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 05 03:36:13 2019
Response via : Initial Calibration

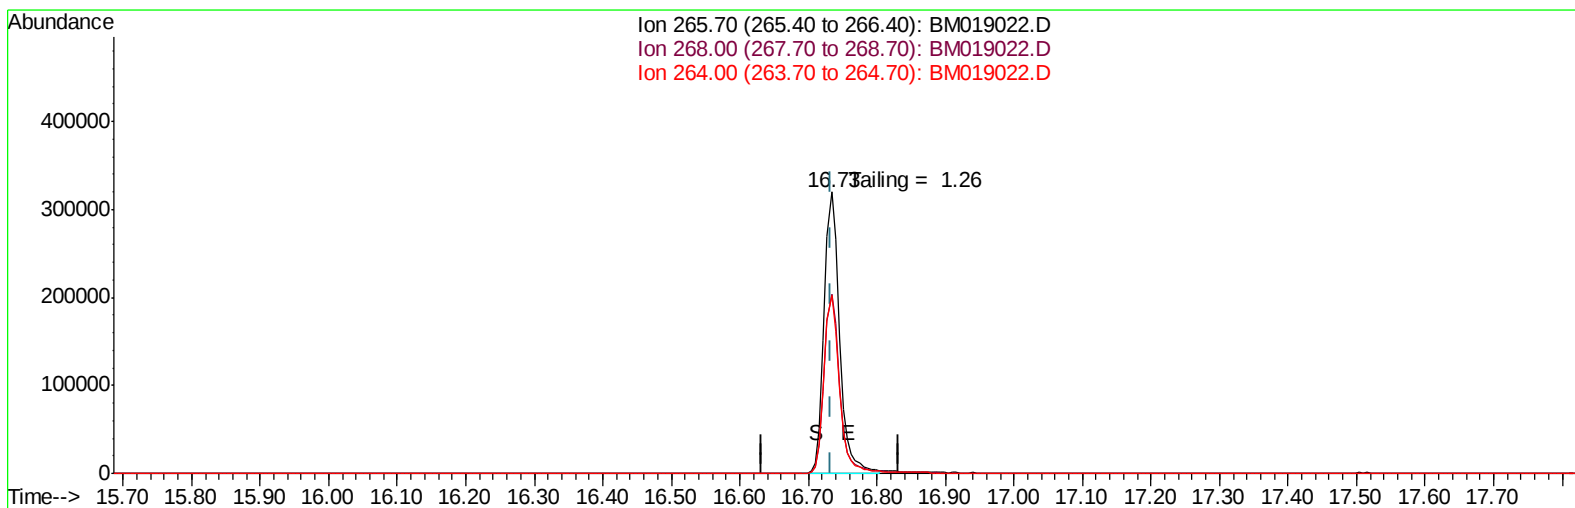

TIC: BM019022.D

(70) Pentachlorophenol (C)




16.733min (+0.000) 79427.82ng

response 501032

Ion	Exp%	Act%
265.70	100	100
268.00	64.10	63.74
264.00	63.20	63.02
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030419\
 Data File : BM019022.D
 Acq On : 04 Mar 2019 23:17
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 05 07:26:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 05 03:36:13 2019
 Response via : Initial Calibration

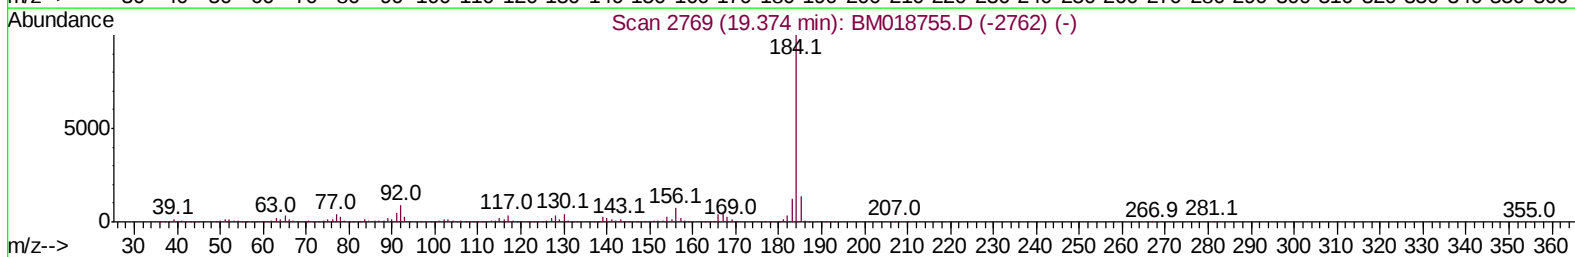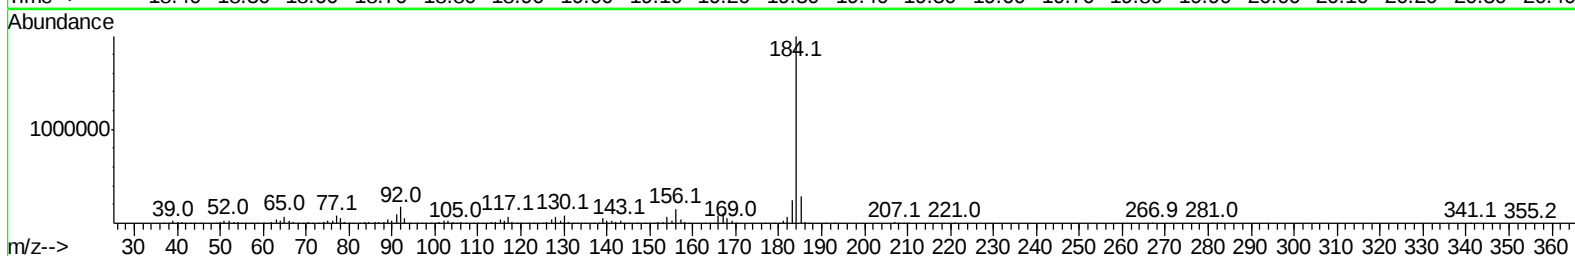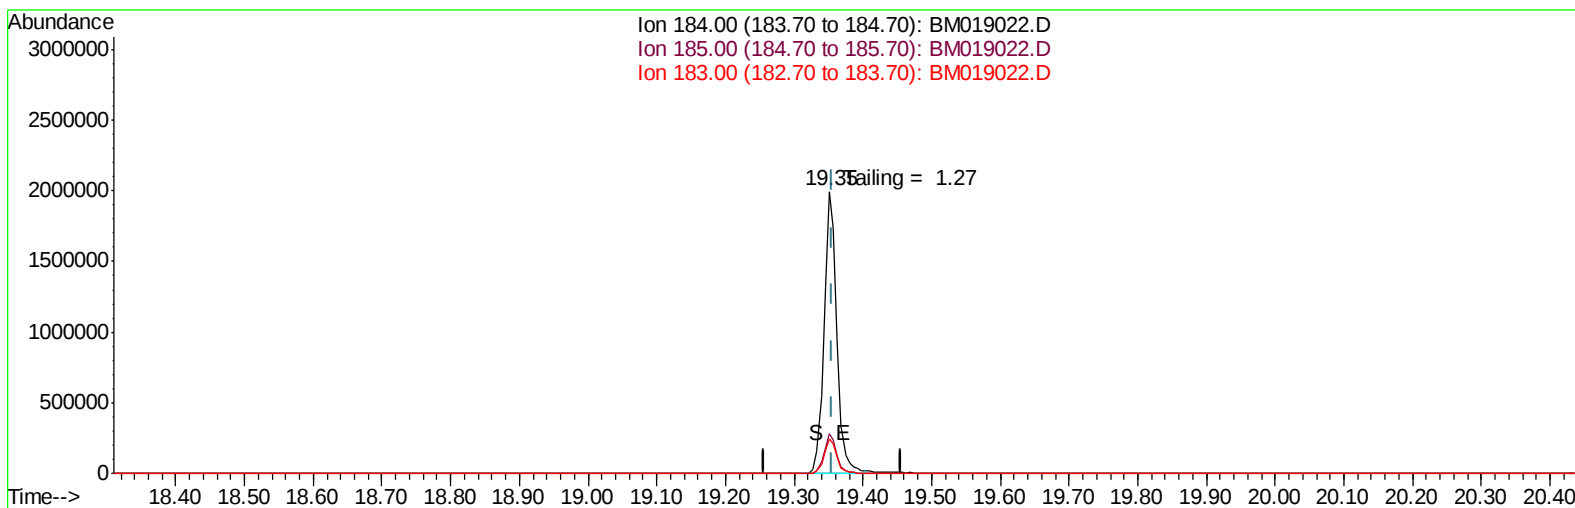

TIC: BM019022.D

(77) Benzidine

19.351min (-0.006) 44979.76ng

response 2625717

Ion	Exp%	Act%
184.00	100	100
185.00	14.00	14.29
183.00	12.10	12.37
0.00	0.00	0.00