

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030419\
 Data File : BM019013.D
 Acq On : 04 Mar 2019 17:17
 Operator : JU/SJ
 Sample : K1655-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 FB-022719

Quant Time: Mar 05 04:02:57 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 05 03:36:13 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	293312	20.00	ng	0.00
21) Naphthalene-d8	10.47	136	1172423	20.00	ng	0.00
39) Acenaphthene-d10	14.33	164	675470	20.00	ng	0.00
64) Phenanthrene-d10	17.09	188	1458264	20.00	ng	0.00
76) Chrysene-d12	21.28	240	1144173	20.00	ng	0.00
87) Perylene-d12	23.53	264	1070940	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.27	112	1081234	60.40	ng	0.00
7) Phenol-d6	6.86	99	900085	35.69	ng	0.00
23) Nitrobenzene-d5	8.85	82	2403878	94.81	ng	0.00
42) 2,4,6-Tribromophenol	15.83	330	1466287	150.59	ng	0.00
45) 2-Fluorobiphenyl	12.95	172	4931376	96.91	ng	0.00
79) Terphenyl-d14	19.72	244	6998951	126.19	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030419\
Data File : BM019013.D
Acq On : 04 Mar 2019 17:17
Operator : JU/SJ
Sample : K1655-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FB-022719

Quant Time: Mar 05 04:02:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 05 03:36:13 2019
Response via : Initial Calibration

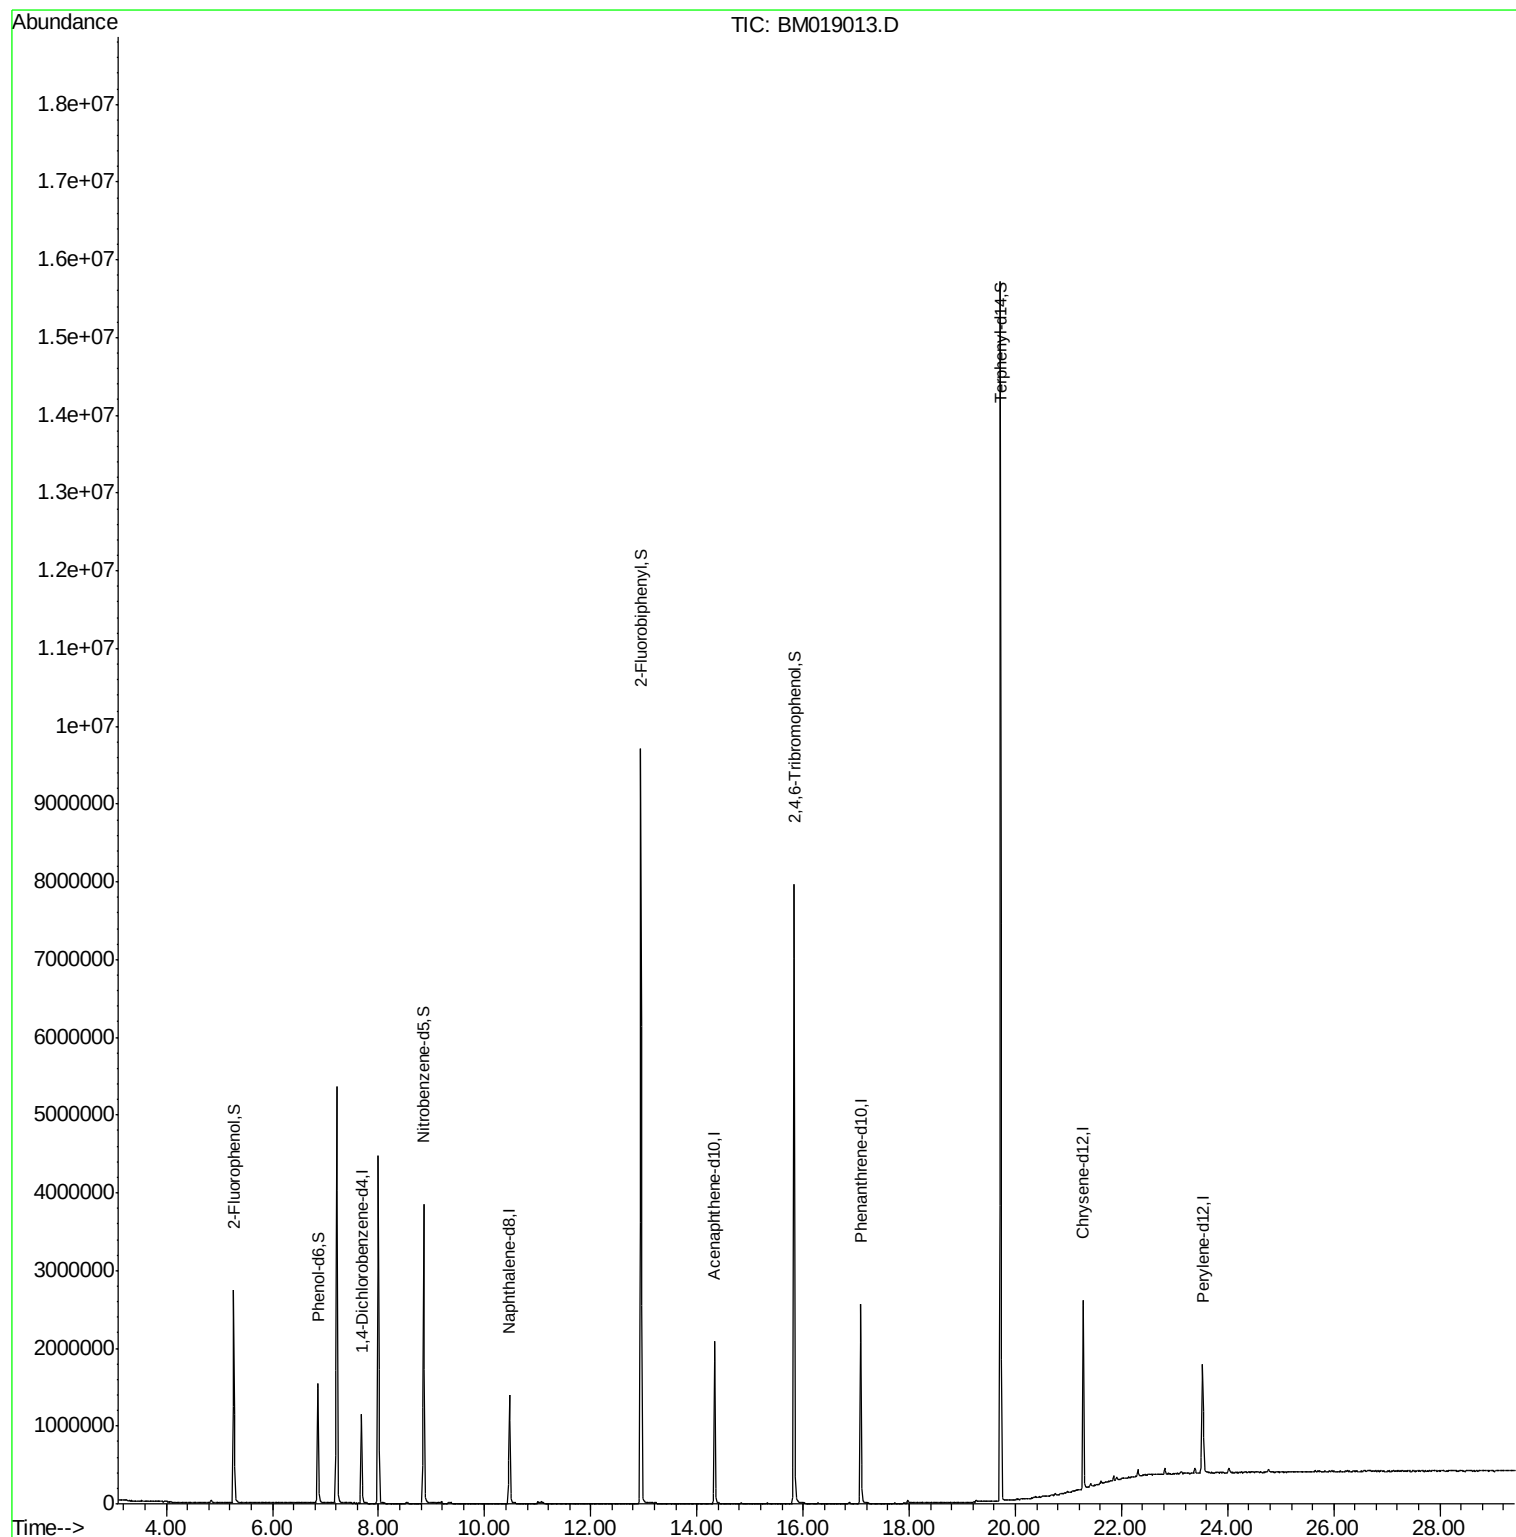

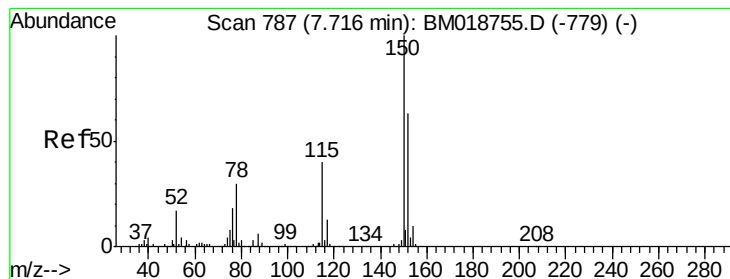


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.68 min Scan# 781
Delta R.T. -0.00 min
Lab File: BM019013.D
Acq: 04 Mar 2019 17:17

Instrument :
BNA_M
ClientSampleId :
FB-022719

Tot Ion	Ratio	Lower	Upper
152	100		
150	157.3	127.3	190.9
115	63.7	50.8	76.2



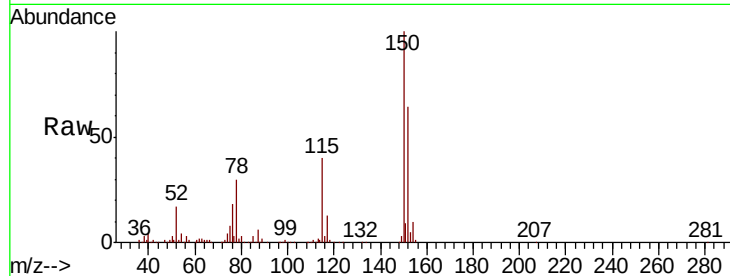


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

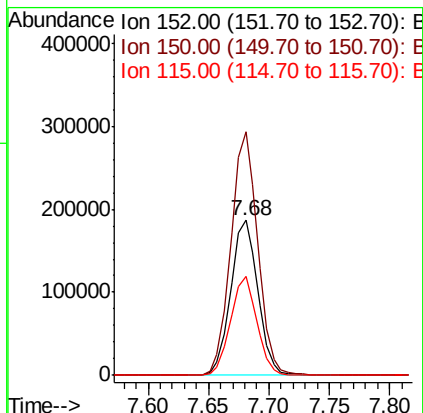

#5

2-Fluorophenol
Concen: 60.399 ng
RT: 5.27 min Scan# 372
Delta R.T. -0.00 min
Lab File: BM019013.D
Acq: 04 Mar 2019 17:17

Tgt Ion	Ratio	Lower	Upper
112	100		
64	63.2	50.6	75.8
63	32.0	25.7	38.5


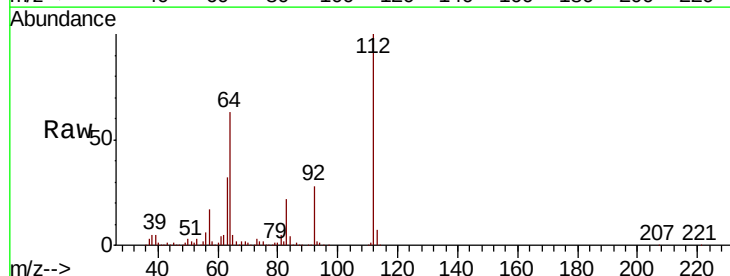



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 63.00 (62.70 to 63.70): BM0

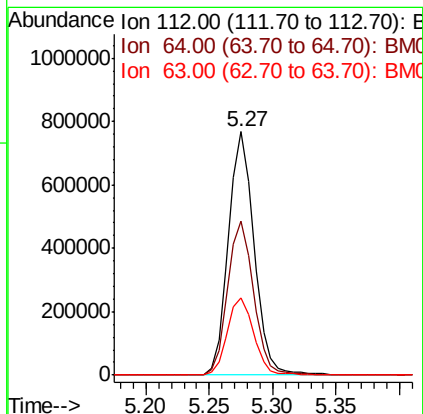



#7

Phenol-d6

Concen: 35.691 ng

RT: 6.86 min Scan# 641

Delta R.T. -0.00 min

Lab File: BM019013.D

Acq: 04 Mar 2019 17:17

Instrument :

BNA_M

ClientSampleId :

FB-022719


Tot Ion: 99 Resp: 900085

Ion Ratio Lower Upper

99 100

42 14.1 11.0 16.6




71 38.2 31.3 46.9



Abundance Ion 99.00 (98.70 to 99.70): BM018755.D (-637) (-)

Ion 42.00 (41.70 to 42.70): BM018755.D (-637) (-)

Ion 71.00 (70.70 to 71.70): BM018755.D (-637) (-)

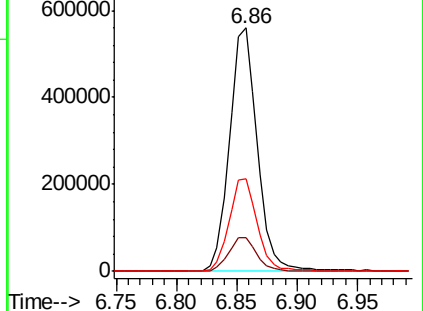

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.47 min Scan# 1255

Delta R.T. -0.00 min

Lab File: BM019013.D

Acq: 04 Mar 2019 17:17

Tgt Ion: 136 Resp: 1172423


Ion Ratio Lower Upper

136 100

137 10.9 8.8 13.2

54 6.8 5.0 7.6

68 7.5 5.5 8.3






Abundance Ion 136.00 (135.70 to 136.70): BM018755.D (-1252) (-)

Ion 137.00 (136.70 to 137.70): BM018755.D (-1252) (-)

Ion 54.00 (53.70 to 54.70): BM018755.D (-1252) (-)

Ion 68.00 (67.70 to 68.70): BM018755.D (-1252) (-)

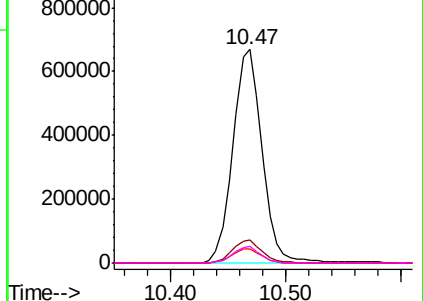







#23
Nitrobenzene-d5
Concen: 94.805 ng
RT: 8.85 min Scan# 980
Delta R.T. -0.00 min
Lab File: BM019013.D
Acq: 04 Mar 2019 17:17

Instrument :
BNA_M
ClientSampleId :
FB-022719

Tot Ion: 82 Resp: 2403878
Ion Ratio Lower Upper
82 100
128 37.7 29.9 44.9
54 37.0 29.1 43.7

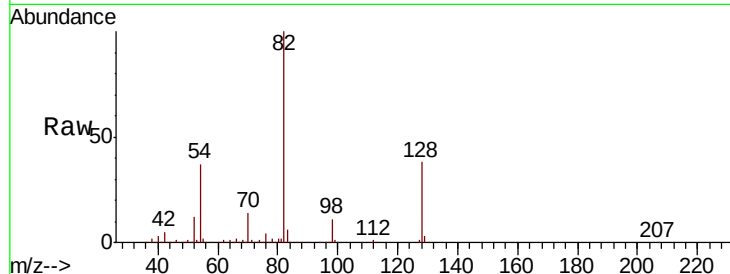


Abundance Ion 82.00 (81.70 to 82.70): BM018755.D (-976) (-)
Ion 128.00 (127.70 to 128.70): BM018755.D (-976) (-)
Ion 54.00 (53.70 to 54.70): BM018755.D (-976) (-)

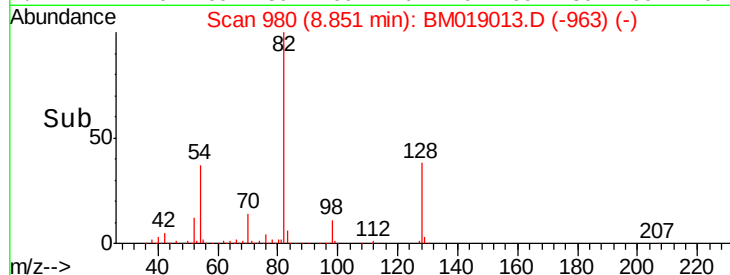
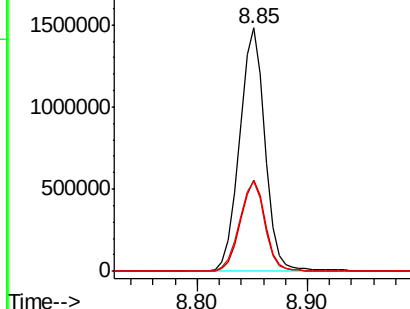



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.33 min Scan# 1912
Delta R.T. -0.00 min
Lab File: BM019013.D
Acq: 04 Mar 2019 17:17

Tgt Ion:164 Resp: 675470
Ion Ratio Lower Upper
164 100
162 105.1 83.4 125.0
160 46.3 36.6 55.0

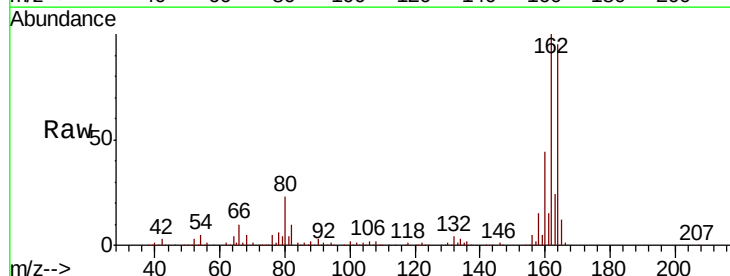

Abundance Ion 164.00 (163.70 to 164.70): BM018755.D (-1910) (-)
Ion 162.00 (161.70 to 162.70): BM018755.D (-1910) (-)
Ion 160.00 (159.70 to 160.70): BM018755.D (-1910) (-)

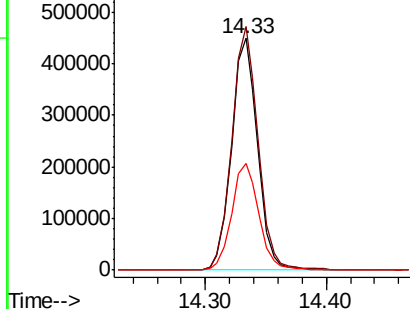







#42
 2,4,6-Tribromophenol
 Concen: 150.594 ng
 RT: 15.83 min Scan# 2167
 Delta R.T. -0.00 min
 Lab File: BM019013.D
 Acq: 04 Mar 2019 17:17

Instrument :
 BNA_M
 ClientSampled :
 FB-022719

Tot Ion:330 Resp: 1466287
 Ion Ratio Lower Upper
 330 100
 332 96.2 76.9 115.3
 141 33.1 28.7 43.1

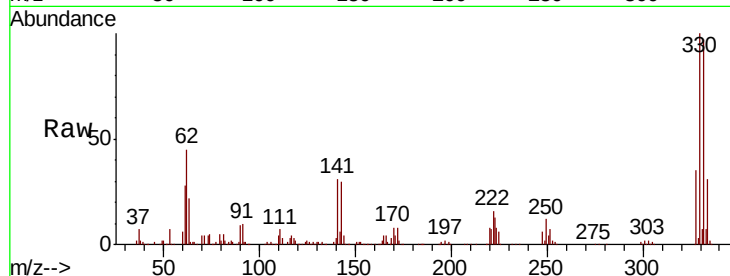


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


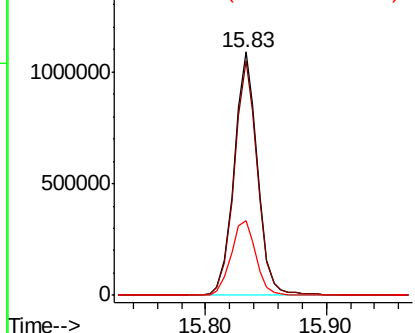



#45
 2-Fluorobiphenyl
 Concen: 96.914 ng
 RT: 12.95 min Scan# 1676
 Delta R.T. -0.01 min
 Lab File: BM019013.D
 Acq: 04 Mar 2019 17:17

Tgt Ion:172 Resp: 4931376
 Ion Ratio Lower Upper
 172 100
 171 36.0 29.0 43.6
 170 23.3 18.6 28.0



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

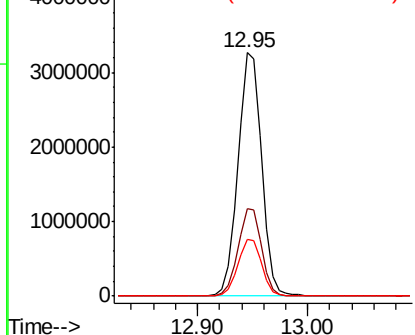



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.09 min Scan# 2380

Delta R.T. -0.00 min

Lab File: BM019013.D

Acq: 04 Mar 2019 17:17

Instrument :

BNA_M

ClientSampleId :

FB-022719


Tot Ion:188 Resp: 1458264

Ion Ratio Lower Upper

188 100

94 10.3 8.2 12.2




80 12.7 9.7 14.5



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM

Ion 80.00 (79.70 to 80.70): BM

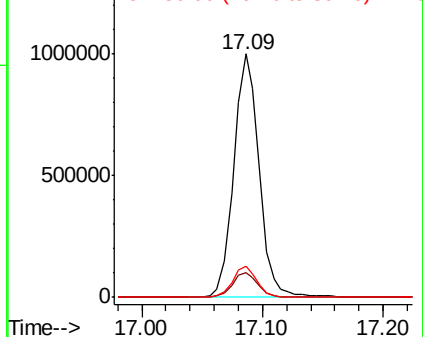

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.28 min Scan# 3093

Delta R.T. -0.01 min

Lab File: BM019013.D

Acq: 04 Mar 2019 17:17


Tgt Ion:240 Resp: 1144173

Ion Ratio Lower Upper

240 100

120 11.9 8.9 13.3



236 25.7 20.9 31.3




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

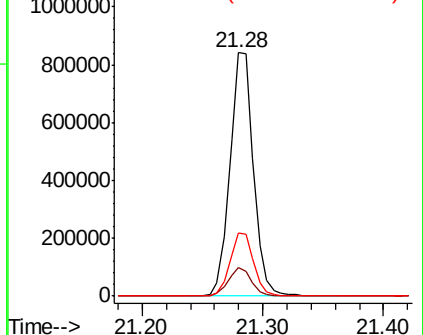

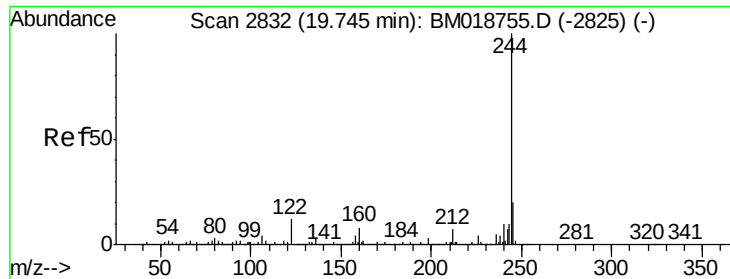

#79

Terphenyl-d14

Concen: 126.188 ng

RT: 19.72 min Scan# 2828

Delta R.T. -0.01 min

Lab File: BM019013.D

Acq: 04 Mar 2019 17:17

Instrument :

BNA_M

ClientSampleId :

FB-022719


Tot Ion:244 Resp: 6998951

Ion Ratio Lower Upper

244 100

212 7.0 5.6 8.4




122 12.0 9.3 13.9



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

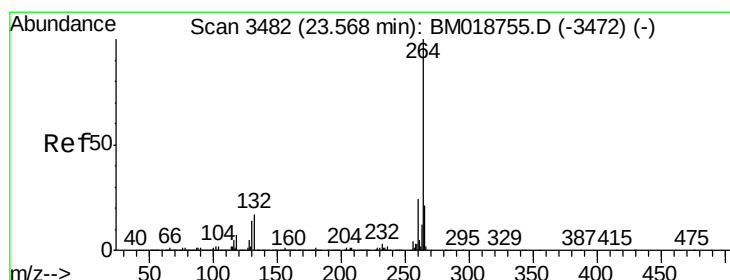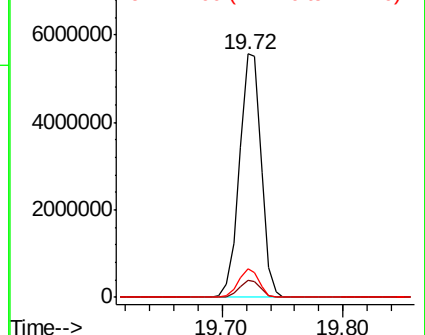

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.53 min Scan# 3475

Delta R.T. -0.01 min

Lab File: BM019013.D

Acq: 04 Mar 2019 17:17


Tgt Ion:264 Resp: 1070940

Ion Ratio Lower Upper

264 100

260 23.4 18.9 28.3

265 22.0 17.3 25.9



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

