

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030419\
Data File : BM019005.D
Acq On : 04 Mar 2019 12:28
Operator : JU/SJ
Sample : PB117506BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB117506BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.275	366	372	394	rBV	4973975	7125547	63.52%	9.410%
2	6.858	634	641	661	rBV	4717695	7669136	68.36%	10.128%
3	7.216	694	702	714	rBV	5179345	7937076	70.75%	10.481%
4	7.681	774	781	791	rBV	981687	1487581	13.26%	1.964%
5	7.999	827	835	843	rBV	3612936	5647024	50.34%	7.457%
6	8.852	972	980	993	rBV	2647319	4514554	40.24%	5.962%
7	10.469	1247	1255	1276	rBV	1151333	2022345	18.03%	2.671%
8	12.945	1669	1676	1693	rBV	7216190	10674519	95.15%	14.096%
9	14.334	1905	1912	1928	rBV2	1694278	2657564	23.69%	3.509%
10	15.833	2160	2167	2188	rBV	4901890	7455446	66.46%	9.845%
11	17.086	2374	2380	2395	rBV	1844716	2825345	25.18%	3.731%
12	19.721	2822	2828	2838	rBV	8994762	11218551	100.00%	14.815%
13	21.286	3089	3094	3101	rBV	1705882	2265317	20.19%	2.991%
14	23.533	3470	3476	3487	rVB2	1092188	2225845	19.84%	2.939%


Sum of corrected areas: 75725850

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030419\
Data File : BM019005.D
Acq On : 04 Mar 2019 12:28
Operator : JU/SJ
Sample : PB117506BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB117506BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

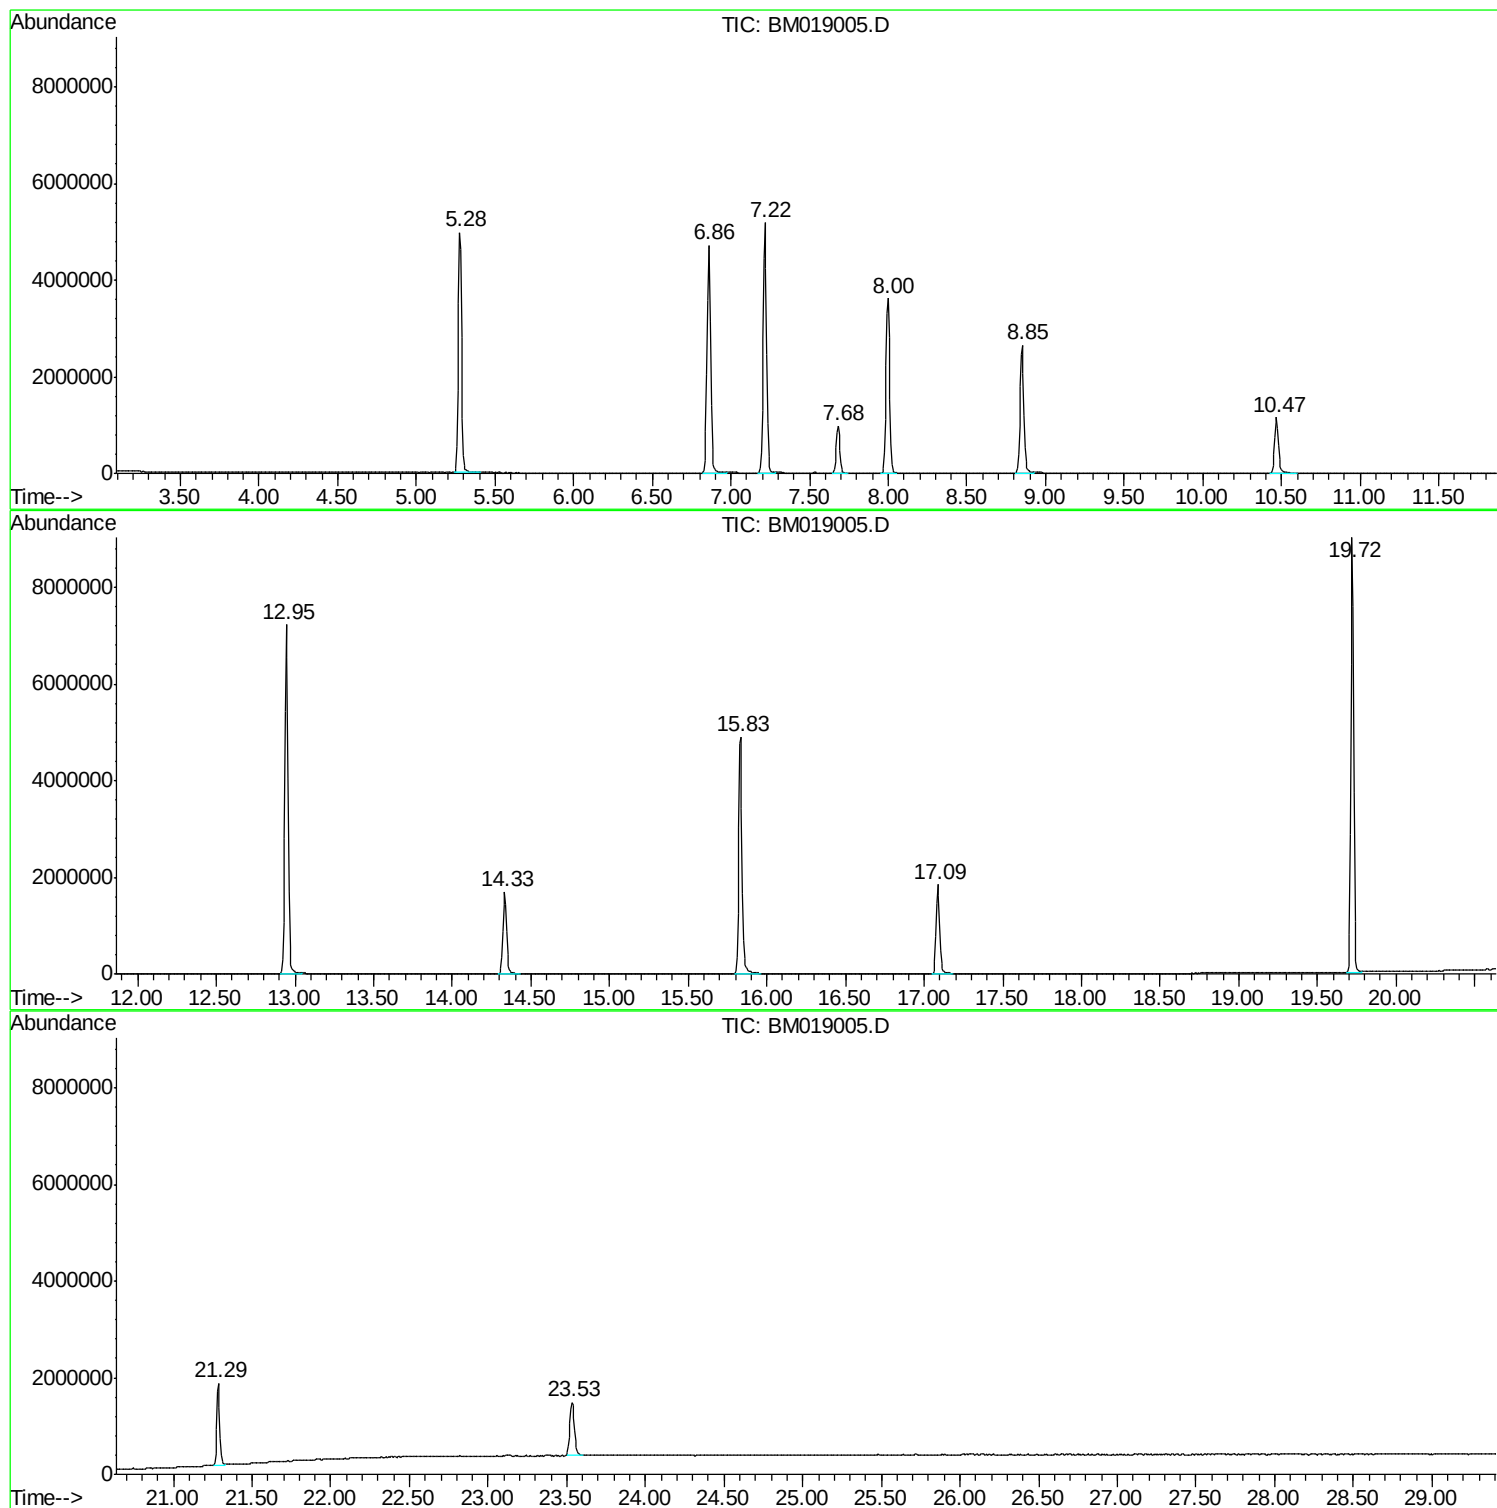

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030419\
Data File : BM019005.D
Acq On : 04 Mar 2019 12:28
Operator : JU/SJ
Sample : PB117506BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB117506BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.22 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.22	106.71 ng	7937080	1,4-Dichlorobenzene-d4	7.68

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
3		Tranvlcyproline-propionyl	189	C12H15NO	1000123-86-3	12
4		2-Cyclohexen-1-one	96	C6H8O	000930-68-7	11
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

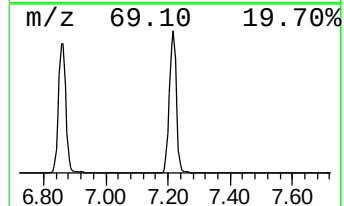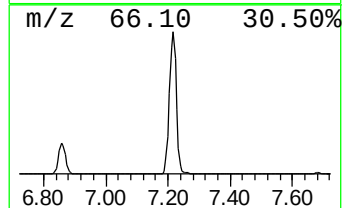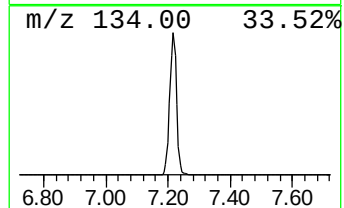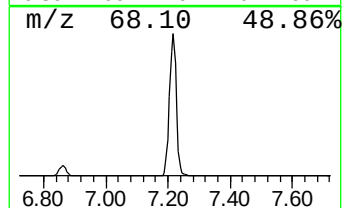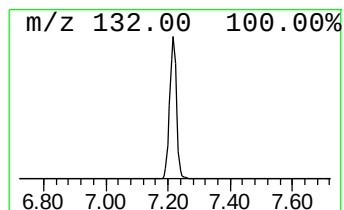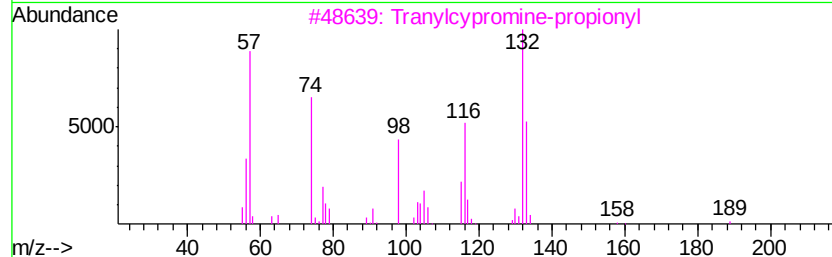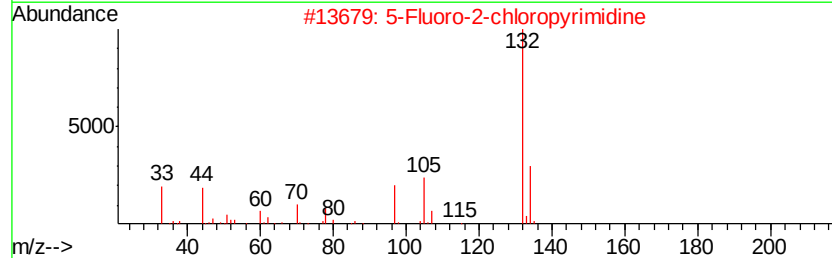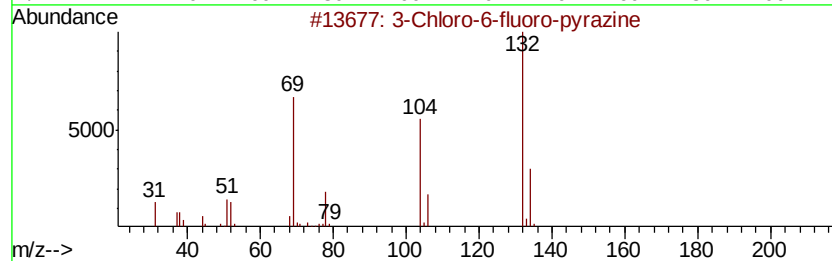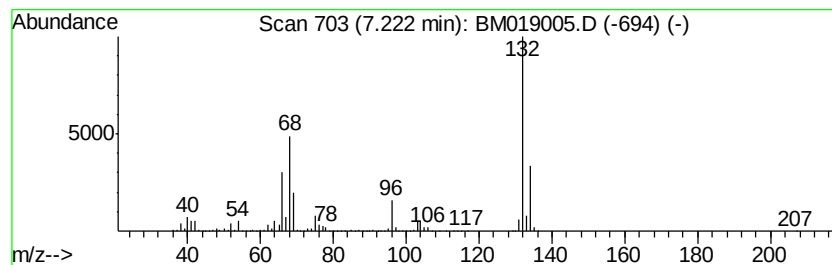

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM030419\
Data File : BM019005.D
Acq On : 04 Mar 2019 12:28
Operator : JU/SJ
Sample : PB117506BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB117506BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown7.22	7.22	106.7	ng	7937080	1	7.68	1487580	20.0