

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030419\
 Data File : BM019011.D
 Acq On : 04 Mar 2019 16:05
 Operator : JU/SJ
 Sample : K1650-18
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 TWP-1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.275	366	372	389	rBV	2532910	3670333	22.29%	4.696%
2	6.857	634	641	653	rBV	1498309	2434472	14.79%	3.115%
3	7.216	694	702	718	rBV	4640122	7390406	44.89%	9.456%
4	7.681	774	781	789	rBV	945449	1461326	8.88%	1.870%
5	7.998	827	835	848	rBV	3810454	6150983	37.36%	7.870%
6	8.851	972	980	997	rBV	3184538	5352610	32.51%	6.849%
7	10.469	1247	1255	1268	rBV	1111508	1994327	12.11%	2.552%
8	12.945	1669	1676	1701	rBV	8333114	12207325	74.14%	15.619%
9	14.333	1903	1912	1932	rBV2	1696825	2701535	16.41%	3.457%
10	15.833	2160	2167	2185	rBV	6769651	9741284	59.17%	12.464%
11	17.086	2372	2380	2393	rBV	2187157	3145231	19.10%	4.024%
12	19.721	2822	2828	2837	rBV	13000512	16464577	100.00%	21.066%
13	21.286	3088	3094	3101	rBV	2066852	2898850	17.61%	3.709%
14	23.533	3469	3476	3488	rBV	1264314	2542417	15.44%	3.253%


Sum of corrected areas: 78155676

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030419\
Data File : BM019011.D
Acq On : 04 Mar 2019 16:05
Operator : JU/SJ
Sample : K1650-18
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TWP-1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

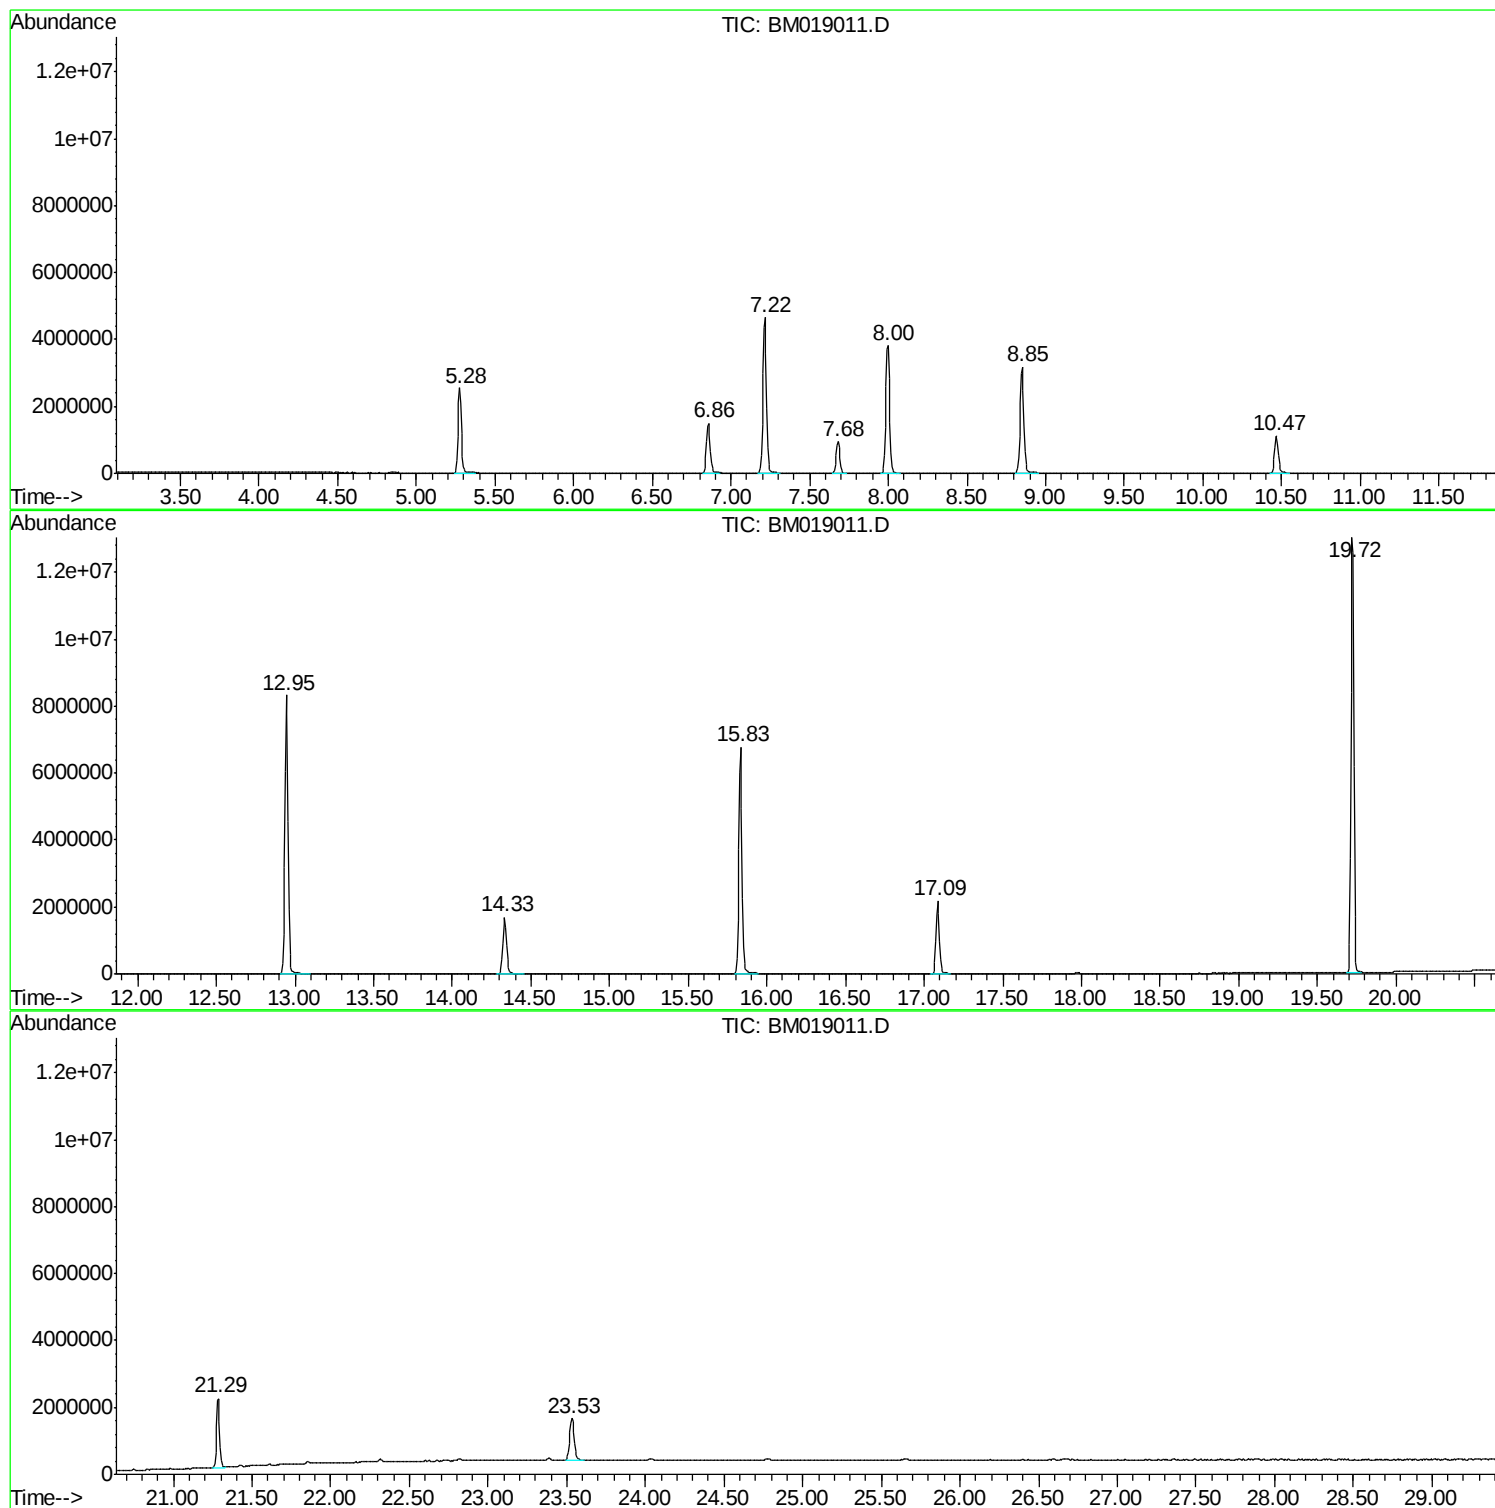

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030419\
Data File : BM019011.D
Acq On : 04 Mar 2019 16:05
Operator : JU/SJ
Sample : K1650-18
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TWP-1










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.22 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.22	101.15 ng	7390410	1,4-Dichlorobenzene-d4	7.68

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	12
4		2-Cyclohexen-1-one	96	C6H8O	000930-68-7	11
5		4-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-60-2	9

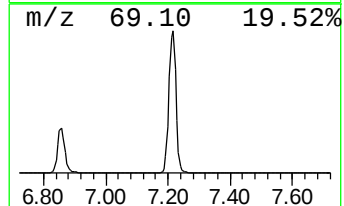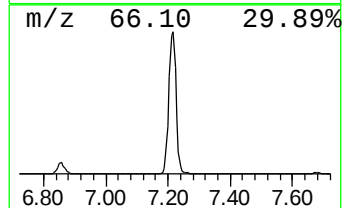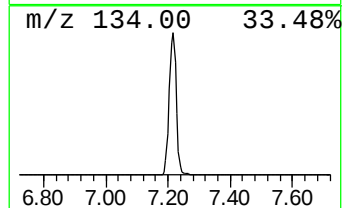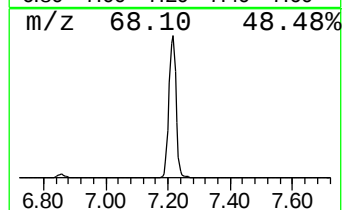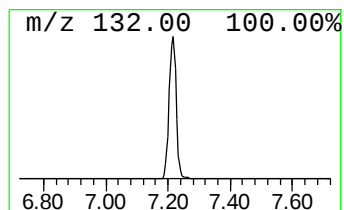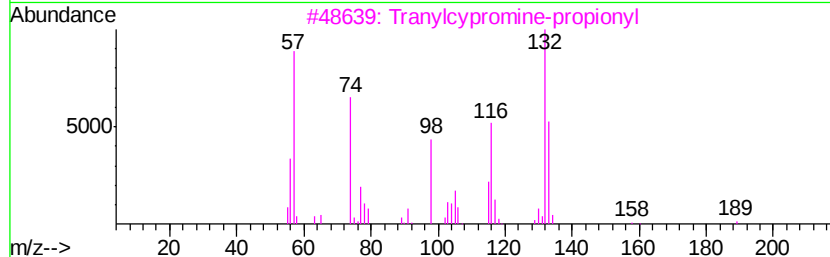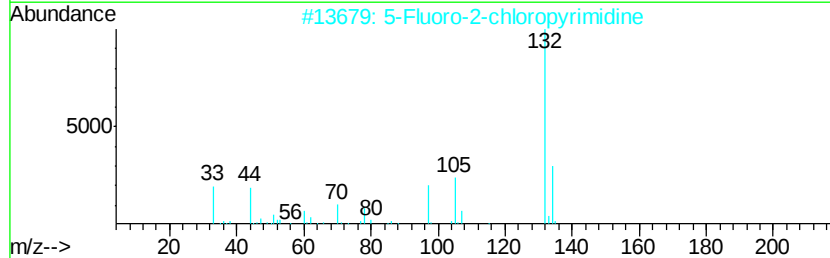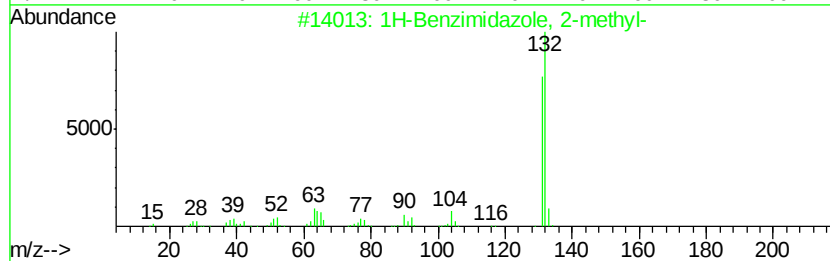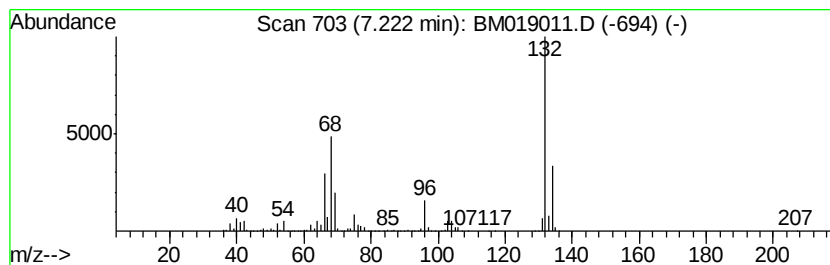

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030419\
Data File : BM019011.D
Acq On : 04 Mar 2019 16:05
Operator : JU/SJ
Sample : K1650-18
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TWP-1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.22	7.22	101.2	ng	7390410	1	7.68	1461330	20.0