


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030419\
 Data File : BM019002.D
 Acq On : 04 Mar 2019 10:40
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 05 03:36:13 2019

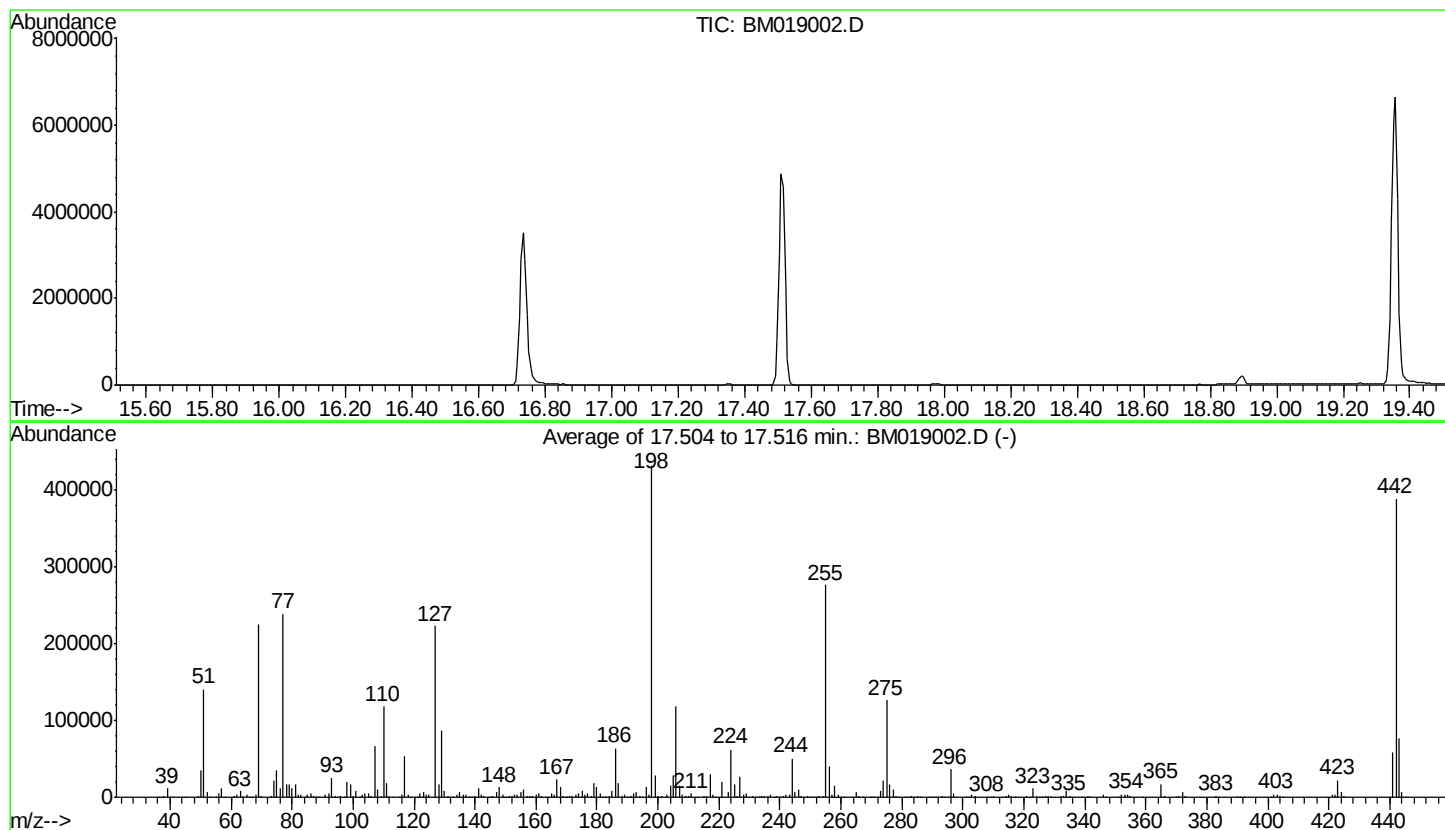

AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.5	140450	PASS
68	69	0.00	2	1.8	4130	PASS
69	198	0.00	100	52.2	225365	PASS
70	69	0.00	2	0.6	1273	PASS
127	198	10	80	51.7	222997	PASS
197	198	0.00	2	0.7	3206	PASS
198	198	100	100	100.0	431552	PASS
199	198	5	9	6.8	29173	PASS
275	198	10	60	29.3	126362	PASS
365	198	1	100	4.0	17448	PASS
441	198	0.01	100	13.6	58728	PASS
442	198	50	100	90.0	388309	PASS
443	442	15	24	19.5	75898	PASS