


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030419\
Data File : BM019022.D
Acq On : 04 Mar 2019 23:17
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Mar 05 03:36:13 2019

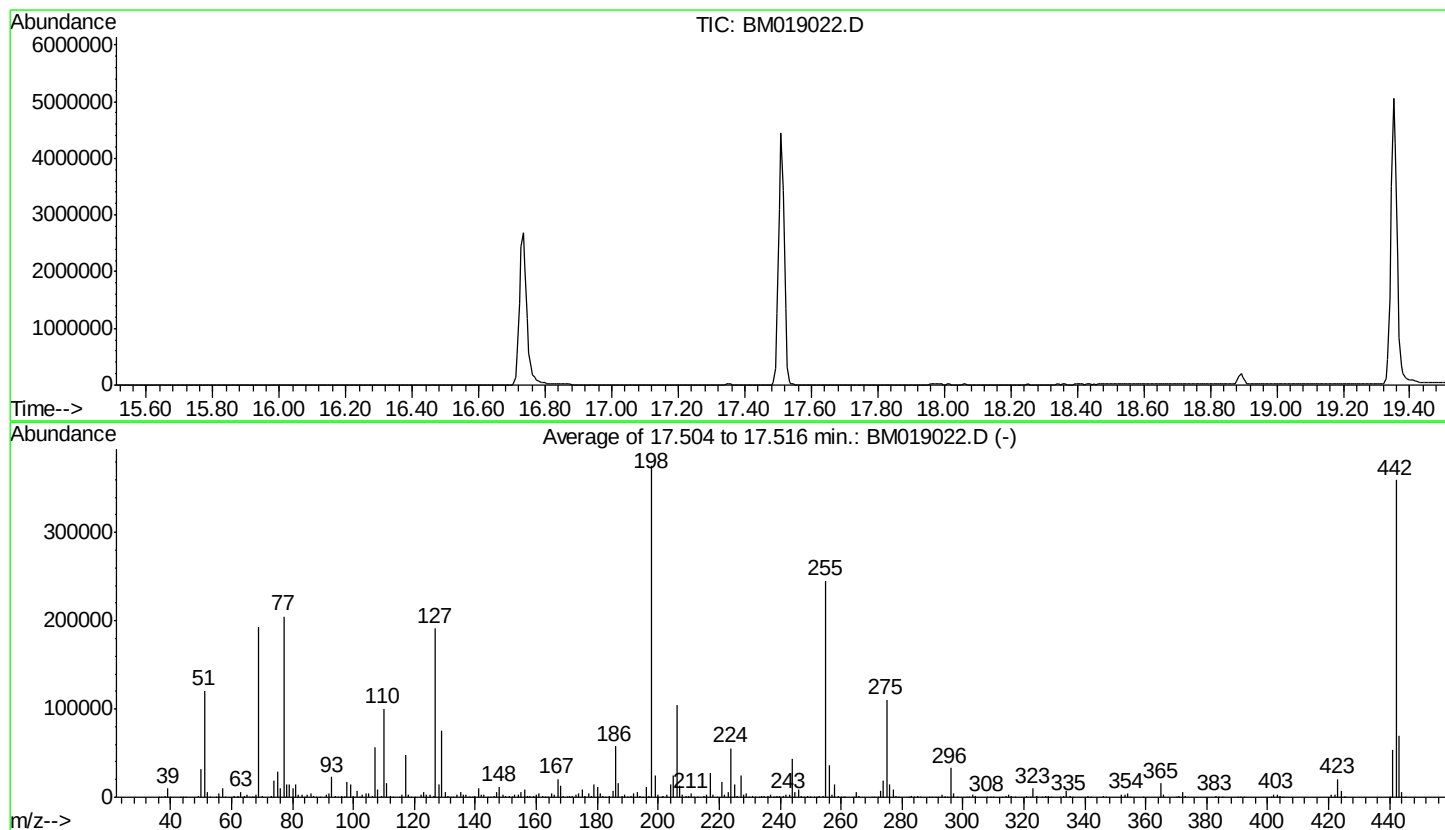

AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.1	120618	PASS
68	69	0.00	2	1.8	3397	PASS
69	198	0.00	100	51.5	193621	PASS
70	69	0.00	2	0.5	1007	PASS
127	198	10	80	50.8	190912	PASS
197	198	0.00	2	0.5	1824	PASS
198	198	100	100	100.0	375744	PASS
199	198	5	9	6.6	24826	PASS
275	198	10	60	29.5	110893	PASS
365	198	1	100	4.2	15813	PASS
441	198	0.01	100	14.4	54226	PASS
442	198	50	100	95.7	359466	PASS
443	442	15	24	19.4	69610	PASS