

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030425\
 Data File : BM049692.D
 Acq On : 04 Mar 2025 12:28
 Operator : RC/JU
 Sample : SSTD3.2059
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD3.2046

Quant Time: Mar 04 12:59:21 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM030425.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 04 11:57:36 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.805	152	7931	0.400	ng/ul	0.00
4) Naphthalene-d8	10.601	136	20879	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.442	164	11320	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.183	188	21315	0.400	ng/ul	0.00
17) Chrysene-d12	21.365	240	16801	0.400	ng/ul	0.00
23) Perylene-d12	23.650	264	17509	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.248	96	28149	3.149	ng/ul	0.00
6) 2-Methylnaphthalene-d10	0.000	152	0d	0.000	ng/ul	
18) Fluoranthene-d10	0.000	212	0d	0.000	ng/ul	
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.286	88	29954	3.137	ng/ul#	83
14) Pentachlorophenol	16.841	266	16626	3.860	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030425\
Data File : BM049692.D
Acq On : 04 Mar 2025 12:28
Operator : RC/JU
Sample : SST3.2059
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTD3.2046

Quant Time: Mar 04 12:59:21 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM030425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 04 11:57:36 2025
Response via : Initial Calibration




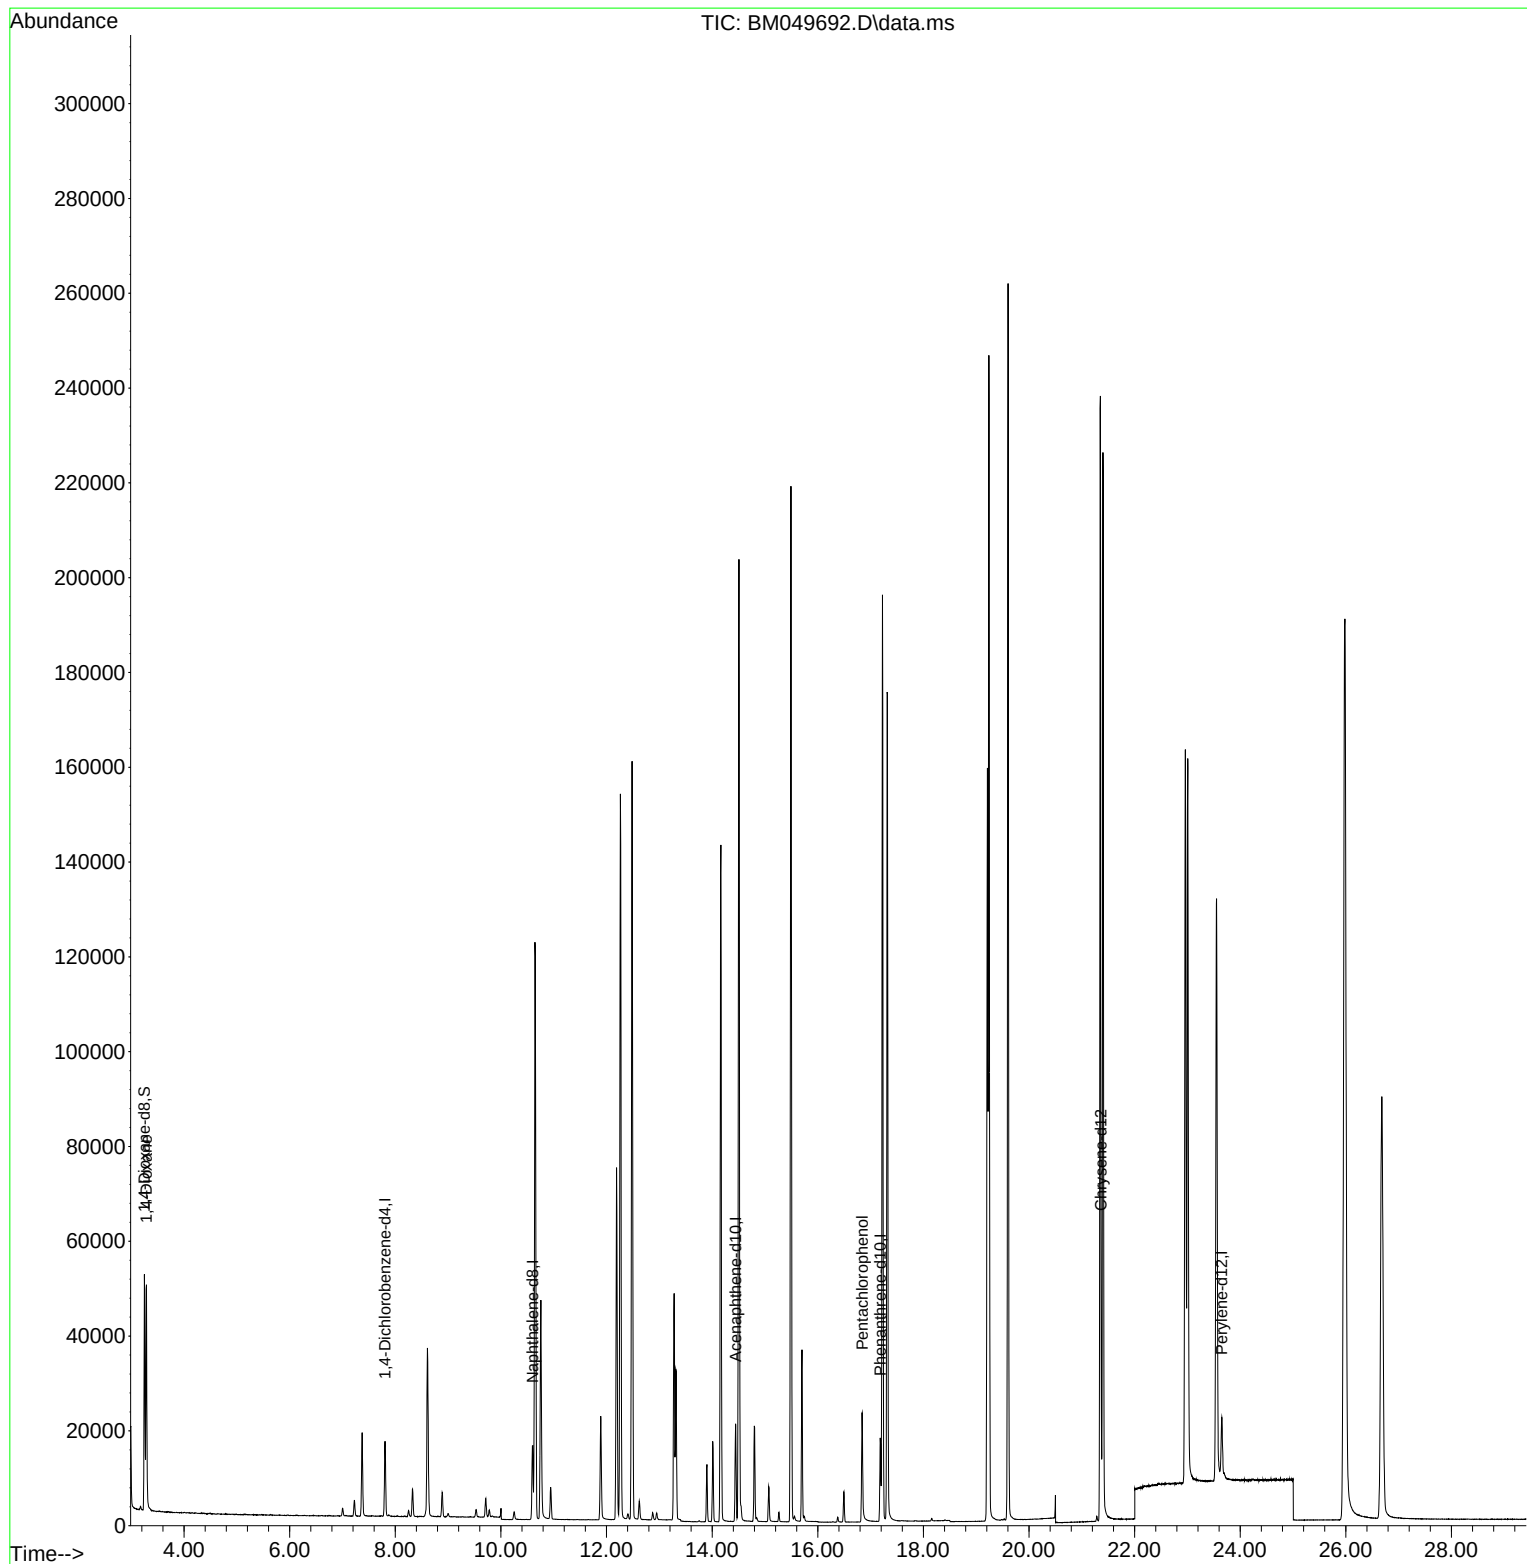


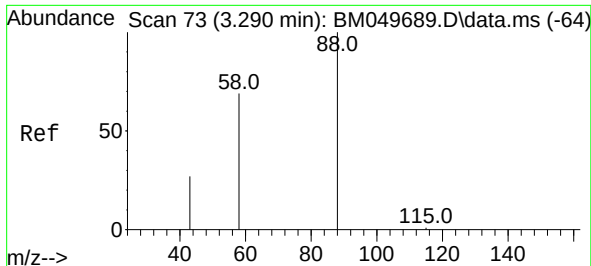

#2
1,4-Dioxane
Concen: 3.137 ng/ul
RT: 3.286 min Scan# 71
Delta R.T. -0.004 min
Lab File: BM049692.D
Acq: 04 Mar 2025 12:28

Instrument :
BNA_M
ClientSampleId :
SSTD3.2046

Tgt Ion: 88 Resp: 29954
Ion Ratio Lower Upper
88 100
43 28.7 32.6 49.0#
58 68.4 45.9 68.9

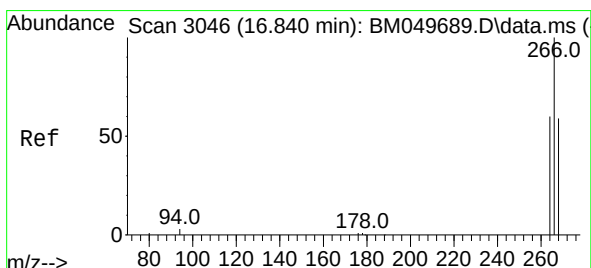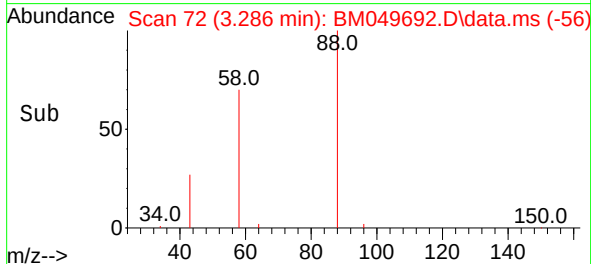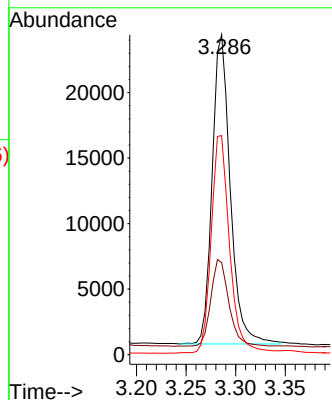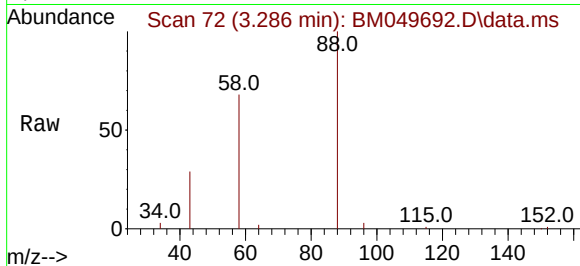

#14
Pentachlorophenol
Concen: 3.860 ng/ul
RT: 16.841 min Scan# 3046
Delta R.T. 0.001 min
Lab File: BM049692.D
Acq: 04 Mar 2025 12:28

Tgt Ion: 266 Resp: 16626
Ion Ratio Lower Upper
266 100
264 62.7 50.2 75.4
268 63.7 49.9 74.9

