


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030425\
Data File : BM049686.D
Acq On : 04 Mar 2025 08:50
Operator : RC/JU
Sample : DFTPP088
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP088

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM030425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Mar 04 13:03:01 2025

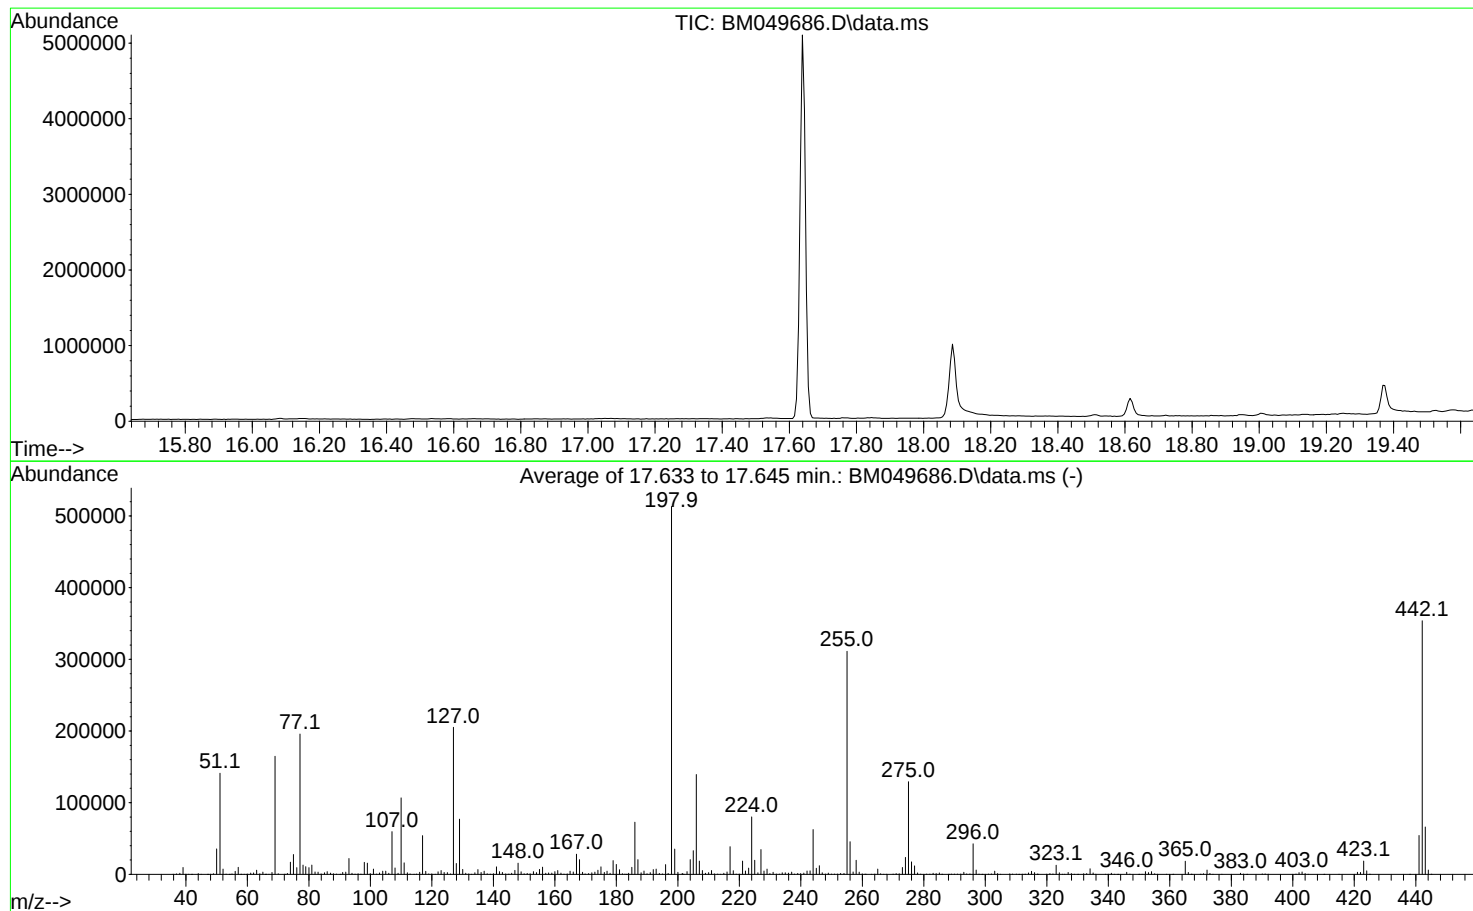

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	27.5	141187	PASS
68	69	0.00	2	1.6	2610	PASS
69	198	0.00	100	32.1	164760	PASS
70	69	0.00	2	0.5	813	PASS
127	198	10	80	40.0	205099	PASS
197	198	0.00	2	0.3	1300	PASS
198	198	100	100	100.0	513237	PASS
199	198	5	9	6.9	35259	PASS
275	198	10	60	25.2	129219	PASS
365	198	1	100	3.6	18372	PASS
441	198	0.01	100	10.6	54275	PASS
442	198	50	100	68.9	353749	PASS
443	442	15	24	18.7	66037	PASS