

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030516\
 Data File : BM004558.D
 Acq On : 05 Mar 2016 16:19
 Operator : SJ/UM
 Sample : SSTDICC0.1
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC0.1

Manual Integrations
 APPROVED

UMANGI
 3/7/2016 12:36:06 PM

Quant Time: Mar 07 07:36:01 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM030516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 07 07:21:48 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.29	152	24274	5.00	ng	0.00
7) Naphthalene-d8	10.06	136	94554	5.00	ng	0.00
13) Acenaphthene-d10	13.98	164	50435	5.00	ng	0.00
19) Phenanthrene-d10	16.74	188	129884	5.00	ng	0.00
25) Chrysene-d12	20.97	240	110637	5.00	ng	-0.01
34) Perylene-d12	23.09	264	109410	5.00	ng	0.01

System Monitoring Compounds

4) 2-Fluorophenol	5.01	112	600	0.12	ng	0.00
5) Phenol-d6	6.64	99	676	0.11	ng	0.02
8) Nitrobenzene-d5	8.49	82	504	0.12	ng	0.02
14) 2,4,6-Tribromophenol	15.51	330	230	0.15	ng	0.00
15) 2-Fluorobiphenyl	12.59	172	1724	0.11	ng	0.00
28) Terphenyl-d14	19.42	244	2027	0.10	ng	0.00

Target Compounds

						Qvalue
2) 1,4-Dioxane	2.87	88	486	0.18	ng	# 100
3) n-Nitrosodimethylamine	3.20	42	217	0.13	ng	# 100
6) bis(2-Chloroethyl)ether	6.75	93	586	0.10	ng	# 20
9) Nitrobenzene	8.53	77	557	0.12	ng	# 100
10) Naphthalene	10.11	128	3372	0.15	ng	# 91
11) Hexachlorobutadiene	10.39	225	415	0.11	ng	# 100
12) 2-Methylnaphthalene	11.76	142	1511	0.11	ng	# 93
16) Acenaphthylene	13.69	152	2709	0.11	ng	# 42
17) Acenaphthene	14.02	154	1822	0.12	ng	# 55
18) Fluorene	15.04	166	2379	0.13	ng	# 83
20) Hexachlorobenzene	16.07	284	1130	0.20	ng	# 100
21) Pentachlorophenol	16.48	266	120	0.15	ng	# 86
22) Phenanthrene	16.79	178	3696	0.12	ng	# 100
23) Anthracene	16.89	178	3030	0.11	ng	# 100
24) Fluoranthene	18.84	202	4460	0.11	ng	# 97
26) Benzidine	19.08	184	381	0.04	ng	# 1
27) Pyrene	19.20	202	4619	0.11	ng	# 84
29) Benzo(a)anthracene	20.97	228	4124	0.11	ng	# 92
30) 3,3'-Dichlorobenzidine	20.93	252	685m	0.06	ng	
31) Chrysene	21.01	228	4575m	0.10	ng	
32) Bis(2-ethylhexyl)phthalate	20.89	149	3286	0.14	ng	# 52
33) Indeno(1,2,3-cd)pyrene	25.18	276	3735	0.12	ng	# 83
35) Benzo(a)pyrene	22.99	252	3392	0.10	ng	# 62
36) Dibenzo(a,h)anthracene	25.18	278	2940	0.11	ng	# 69
37) Benzo(g,h,i)perylene	25.82	276	3289	0.11	ng	# 82

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030516\
Data File : BM004558.D
Acq On : 05 Mar 2016 16:19
Operator : SJ/UM
Sample : SSTDIC0.1
Misc :
ALS Vial : 3 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
SSTDIC0.1

Manual Integrations
APPROVED

UMANGI
3/7/2016 12:36:06 PM

Quant Time: Mar 07 07:36:01 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM030516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 07 07:21:48 2016
Response via : Initial Calibration






#1

1,4-Dichlorobenzene-d4
Concen: 5.00 ng
RT: 7.29 min Scan# 291
Delta R.T. -0.00 min
Lab File: BM004558.D
Acq: 05 Mar 2016 16:19




Instrument :
BNA_M
ClientSampleId :
SSTDIC0.1



Tgt Ion: 152 Resp: 24274
Ion Ratio Lower Upper
152 100
150 173.8 140.1 210.1
115 69.1 56.1 84.1

Manual Integrations
APPROVED




UMANGI
3/7/2016 12:36:06 PM




#2

1,4-Dioxane
Concen: 0.18 ng
RT: 2.87 min Scan# 13
Delta R.T. -0.00 min
Lab File: BM004558.D
Acq: 05 Mar 2016 16:19

Tgt Ion: 88 Resp: 486
Ion Ratio Lower Upper
88 100
58 36.0 0.0 0.0#
43 0.0 0.0 0.0





#3

n-Nitrosodimethylamine

Concen: 0.13 ng

RT: 3.20 min Scan# 34

Delta R.T. -0.00 min

Lab File: BM004558.D

Acq: 05 Mar 2016 16:19

Instrument :

BNA_M





ClientSampleId :

SSTDICC0.1

Tgt Ion:	42	Resp:	217
Ion	Ratio	Lower	Upper
42	100		
74	144.2	0.0	0.0#
44	34.6	0.0	0.0#

Manual Integrations
APPROVED

UMANGI
3/7/2016 12:36:06 PM



#4

2-Fluorophenol

Concen: 0.12 ng




RT: 5.01 min Scan# 151




Delta R.T. -0.00 min

Lab File: BM004558.D

Acq: 05 Mar 2016 16:19

Tgt Ion:	112	Resp:	600
Ion	Ratio	Lower	Upper
112	100		
64	48.8	0.0	0.0#
63	26.0	0.0	0.0#





#5

Phenol-d6

Concen: 0.11 ng

RT: 6.64 min Scan# 253

Delta R.T. 0.02 min

Lab File: BM004558.D

Acq: 05 Mar 2016 16:19

Tgt Ion:	99	Resp:	676
Ion	Ratio	Lower	Upper
99	100		
42	22.6	0.0	0.0#
71	29.4	0.2	0.2#

Instrument :





BNA_M

ClientSampleId :

SSTDICC0.1

Manual Integrations
APPROVED

UMANGI
3/7/2016 12:36:06 PM



#6

bis(2-Chloroethyl)ether

Concen: 0.10 ng


RT: 6.75 min Scan# 259


Delta R.T. -0.00 min

Lab File: BM004558.D

Acq: 05 Mar 2016 16:19

Tgt Ion:	93	Resp:	586
Ion	Ratio	Lower	Upper
93	100		
63	62.6	18.7	28.1#
95	30.5	0.0	0.0#





#7

Naphthalene-d8

Concen: 5.00 ng

RT: 10.06 min Scan# 527

Delta R.T. -0.00 min

Lab File: BM004558.D


Acq: 05 Mar 2016 16:19

Instrument :

BNA_M

ClientSampleId :

SSTDIC0.1



Tgt Ion: 136 Resp: 94554

Ion Ratio Lower Upper

136 100




137 11.1 9.2 13.8

54 4.6 3.0 4.4#

68 4.3 2.9 4.3#

Manual Integrations
APPROVED

UMANGI
3/7/2016 12:36:06 PM



#8

Nitrobenzene-d5

Concen: 0.12 ng

RT: 8.49 min Scan# 378

Delta R.T. 0.02 min

Lab File: BM004558.D

Acq: 05 Mar 2016 16:19




Tgt Ion: 82 Resp: 504


Ion Ratio Lower Upper

82 100

128 63.3 38.6 58.0#

54 74.2 38.5 57.7#





#9

Nitrobenzene

Concen: 0.12 ng

RT: 8.53 min Scan# 382

Delta R.T. 0.02 min

Lab File: BM004558.D

Acq: 05 Mar 2016 16:19

Instrument :

BNA_M





ClientSampleId :

SSTDIC0.1

Tgt Ion:	77	Resp:	557
Ion	Ratio	Lower	Upper
77	100		
123	56.0	0.0	0.0#
65	10.6	0.0	0.0#

Manual Integrations
APPROVED

UMANGI
3/7/2016 12:36:06 PM

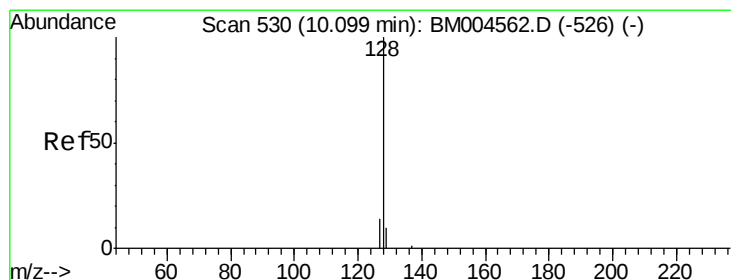

#10

Naphthalene

Concen: 0.15 ng




RT: 10.11 min Scan# 530


Delta R.T. 0.01 min

Lab File: BM004558.D

Acq: 05 Mar 2016 16:19

Tgt Ion:	128	Resp:	3372
Ion	Ratio	Lower	Upper
128	100		
129	16.4	8.7	13.1#
127	15.8	11.3	16.9









#11
Hexachlorobutadiene
Concen: 0.11 ng
RT: 10.39 min Scan# 546
Delta R.T. -0.00 min
Lab File: BM004558.D
Acq: 05 Mar 2016 16:19

Instrument :
BNA_M
ClientSampleId :
SSTDICC0.1

Tgt Ion	Ratio	Resp Lower	Resp Upper
225	100		415
223	63.4	0.0	0.0#
227	62.2	0.0	0.0#




Manual Integrations
APPROVED


UMANGI
3/7/2016 12:36:06 PM



#12
2-Methylnaphthalene
Concen: 0.11 ng
RT: 11.76 min Scan# 655
Delta R.T. 0.02 min
Lab File: BM004558.D
Acq: 05 Mar 2016 16:19

Tgt Ion	Ratio	Resp Lower	Resp Upper
142	100		1511
141	85.1	72.3	108.5
115	38.8	25.4	38.2#









#13
Acenaphthene-d10
Concen: 5.00 ng
RT: 13.98 min Scan# 844
Delta R.T. 0.01 min
Lab File: BM004558.D
Acq: 05 Mar 2016 16:19

Instrument :
BNA_M
ClientSampleId :
SSTDIC0.1

Tgt Ion	Ratio	Lower	Upper
164	100		
162	93.0	78.2	117.2
160	37.1	31.9	47.9




Manual Integrations
APPROVED


UMANGI
3/7/2016 12:36:06 PM



#14
2,4,6-Tribromophenol
Concen: 0.15 ng
RT: 15.51 min Scan# 913
Delta R.T. 0.01 min
Lab File: BM004558.D
Acq: 05 Mar 2016 16:19

Tgt Ion	Ratio	Lower	Upper
330	100		
332	0.0	0.0	0.0
141	58.7	0.0	0.0#



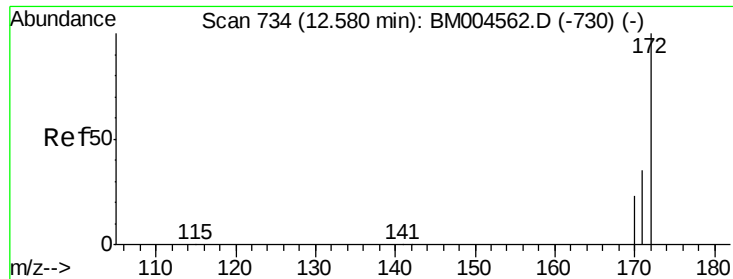





#15
2-Fluorobiphenyl
Concen: 0.11 ng
RT: 12.59 min Scan# 734
Delta R.T. 0.01 min
Lab File: BM004558.D
Acq: 05 Mar 2016 16:19

Instrument :
BNA_M
ClientSampleId :
SSTDIC0.1

Tgt Ion	Ratio	Lower	Upper
172	100		
171	39.1	28.6	42.8
170	28.0	19.1	28.7




Manual Integrations
APPROVED


UMANGI
3/7/2016 12:36:06 PM



#16
Acenaphthylene
Concen: 0.11 ng
RT: 13.69 min Scan# 831
Delta R.T. 0.01 min
Lab File: BM004558.D
Acq: 05 Mar 2016 16:19

Tgt Ion	Ratio	Lower	Upper
152	100		
151	18.6	9.2	13.8#
153	12.8	51.4	77.0#









#17
Acenaphthene
Concen: 0.12 ng
RT: 14.02 min Scan# 846
Delta R.T. -0.02 min
Lab File: BM004558.D
Acq: 05 Mar 2016 16:19

Instrument :
BNA_M
ClientSampleId :
SSTDICC0.1

Tgt Ion	Ratio	Lower	Upper
154	100		
153	104.7	0.0	0.0#
152	57.7	0.2	0.2#




Manual Integrations
APPROVED


UMANGI
3/7/2016 12:36:06 PM

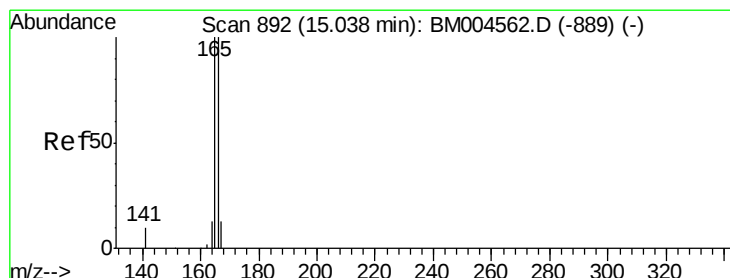

#18
Fluorene
Concen: 0.13 ng
RT: 15.04 min Scan# 892
Delta R.T. 0.01 min
Lab File: BM004558.D
Acq: 05 Mar 2016 16:19

Tgt Ion	Ratio	Lower	Upper
166	100		
165	94.8	0.0	0.0#
167	16.2	20.0	30.0#





#19

Phenanthrene-d10

Concen: 5.00 ng

RT: 16.74 min Scan# 964

Delta R.T. 0.01 min

Lab File: BM004558.D

Acq: 05 Mar 2016 16:19

Instrument :

BNA_M


ClientSampleId :

SSTDICC0.1

Tgt Ion:	188	Resp:	129884
Ion Ratio	Lower	Upper	
188	100		
94	5.4	6.0	9.0#
80	4.5	5.3	7.9#

Manual Integrations
APPROVED

UMANGI
3/7/2016 12:36:06 PM






Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM0

Ion 80.00 (79.70 to 80.70): BM0

Time-->



#20

Hexachlorobenzene

Concen: 0.20 ng


RT: 16.07 min Scan# 938

Delta R.T. 0.01 min

Lab File: BM004558.D

Acq: 05 Mar 2016 16:19

Tgt Ion:	284	Resp:	1130
Ion Ratio	Lower	Upper	
284	100		
142	0.0	0.0	0.0
249	0.0	0.0	0.0






Abundance Ion 283.80 (283.50 to 284.50): E

Ion 142.00 (141.70 to 142.70): E

Ion 249.00 (248.70 to 249.70): E

Time-->









#21
 Pentachlorophenol
 Concen: 0.15 ng
 RT: 16.48 min Scan# 954
 Delta R.T. 0.01 min
 Lab File: BM004558.D
 Acq: 05 Mar 2016 16:19

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC0.1

Tgt Ion	Ratio	Lower	Upper
266	100		
268	92.0	62.6	94.0
264	81.6	57.4	86.0




Manual Integrations
 APPROVED


UMANGI
 3/7/2016 12:36:06 PM



#22
 Phenanthrene
 Concen: 0.12 ng
 RT: 16.79 min Scan# 966
 Delta R.T. 0.01 min
 Lab File: BM004558.D
 Acq: 05 Mar 2016 16:19

Tgt Ion	Ratio	Lower	Upper
178	100		
176	0.0	0.0	0.0
179	21.0	0.0	0.0#









#23
 Anthracene
 Concen: 0.11 ng
 RT: 16.89 min Scan# 970
 Delta R.T. 0.01 min
 Lab File: BM004558.D
 Acq: 05 Mar 2016 16:19

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC0.1

Tgt Ion	Ratio	Lower	Upper
178	100		
176	18.8	0.0	0.0#
179	15.7	0.0	0.0#




Manual Integrations
 APPROVED


UMANGI
 3/7/2016 12:36:06 PM



#24
 Fluoranthene
 Concen: 0.11 ng
 RT: 18.84 min Scan# 1062
 Delta R.T. 0.01 min
 Lab File: BM004558.D
 Acq: 05 Mar 2016 16:19

Tgt Ion	Ratio	Lower	Upper
202	100		
101	12.9	12.2	18.4
203	17.7	14.6	21.8





#25

Chrysene-d12

Concen: 5.00 ng

RT: 20.97 min Scan# 1182

Delta R.T. -0.01 min

Lab File: BM004558.D

Acq: 05 Mar 2016 16:19

Instrument :

BNA_M

ClientSampleId :

SSTDICC0.1

Tgt Ion:240 Resp: 110637
Ion Ratio Lower Upper

240 100


120 35.1 3.5 5.3#

236 34.7 20.3 30.5#




Manual Integrations
APPROVED

UMANGI

3/7/2016 12:36:06 PM



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



#26

Benzidine

Concen: 0.04 ng

RT: 19.08 min Scan# 1076

Delta R.T. 0.01 min

Lab File: BM004558.D


Acq: 05 Mar 2016 16:19

Tgt Ion:184 Resp: 381
Ion Ratio Lower Upper



184 100


185 103.7 19.4 29.0#

183 76.3 16.5 24.7#



Abundance Ion 184.00 (183.70 to 184.70): E
Ion 185.00 (184.70 to 185.70): E
Ion 183.00 (182.70 to 183.70): E









#27
 Pyrene
 Concen: 0.11 ng
 RT: 19.20 min Scan# 1083
 Delta R.T. 0.01 min
 Lab File: BM004558.D
 Acq: 05 Mar 2016 16:19

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC0.1

Tgt Ion	Ratio	Resp Lower	Upper
202	100		
200	20.6	0.2	0.2#
203	18.9	0.0	0.0#




Manual Integrations
 APPROVED


UMANGI
 3/7/2016 12:36:06 PM



#28
 Terphenyl-d14
 Concen: 0.10 ng
 RT: 19.42 min Scan# 1096
 Delta R.T. 0.01 min
 Lab File: BM004558.D
 Acq: 05 Mar 2016 16:19

Tgt Ion	Ratio	Resp Lower	Upper
244	100		
212	13.5	7.0	10.4#
122	19.5	4.2	6.4#









#29
Benzo(a)anthracene
Concen: 0.11 ng
RT: 20.97 min Scan# 1182
Delta R.T. 0.01 min
Lab File: BM004558.D
Acq: 05 Mar 2016 16:19

Instrument :
BNA_M
ClientSampleId :
SSTDICC0.1

Tgt Ion	Ratio	Lower	Upper
228	100		
226	24.2	20.3	30.5
229	26.9	16.3	24.5




Manual Integrations
APPROVED


UMANGI
3/7/2016 12:36:06 PM



#30
3,3'-Dichlorobenzidine
Concen: 0.06 ng m
RT: 20.93 min Scan# 1180
Delta R.T. 0.01 min
Lab File: BM004558.D
Acq: 05 Mar 2016 16:19

Tgt Ion	Ratio	Lower	Upper
252	100		
254	69.6	53.9	80.9
126	49.6	6.9	10.3





#31

Chrysene

Concen: 0.10 ng m

RT: 21.01 min Scan# 1184

Delta R.T. -0.01 min

Lab File: BM004558.D

Acq: 05 Mar 2016 16:19

Instrument :

BNA_M





ClientSampleId :

SSTDICC0.1

Tgt Ion:	228	Resp:	4575
Ion Ratio	Lower	Upper	
228	100		
226	33.1	20.3	30.5#
229	21.3	17.8	26.6

Manual Integrations
APPROVED

UMANGI
3/7/2016 12:36:06 PM



#32

Bis(2-ethylhexyl)phthalate

Concen: 0.14 ng




RT: 20.89 min Scan# 1178


Delta R.T. -0.01 min

Lab File: BM004558.D

Acq: 05 Mar 2016 16:19

Tgt Ion:	149	Resp:	3286
Ion Ratio	Lower	Upper	
149	100		
167	26.4	0.6	0.8#
279	0.0	0.0	0.0






#33
 Indeno(1,2,3-cd)pyrene
 Concen: 0.12 ng
 RT: 25.18 min Scan# 1504
 Delta R.T. 0.02 min
 Lab File: BM004558.D
 Acq: 05 Mar 2016 16:19

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC0.1




Tgt Ion	Ratio	Lower	Upper
276	100		
138	39.3	22.8	34.2#
277	24.3	15.2	22.8#

Manual Integrations
 APPROVED

UMANGI
 3/7/2016 12:36:06 PM






Abundance Ion 276.00 (275.70 to 276.70): E
 Ion 138.00 (137.70 to 138.70): E
 Ion 277.00 (276.70 to 277.70): E




#34
 Perylene-d12
 Concen: 5.00 ng
 RT: 23.09 min Scan# 1303
 Delta R.T. 0.01 min
 Lab File: BM004558.D
 Acq: 05 Mar 2016 16:19

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.9	21.4	32.2
265	23.5	17.8	26.8

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E



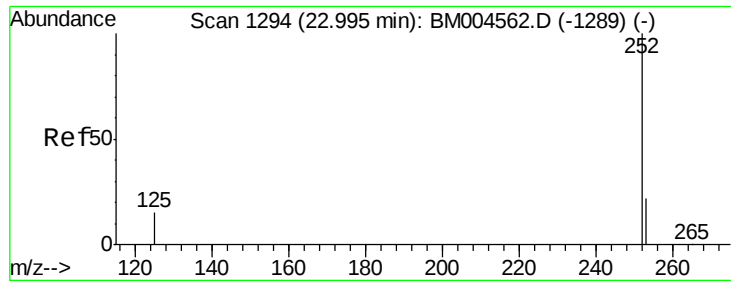





#35
Benzo(a)pyrene
Concen: 0.10 ng
RT: 22.99 min Scan# 1294
Delta R.T. -0.00 min
Lab File: BM004558.D
Acq: 05 Mar 2016 16:19

Instrument :
BNA_M
ClientSampleId :
SSTDIC0.1

Tgt Ion	Ratio	Lower	Upper
252	100		
253	38.6	19.0	28.6#
125	39.2	14.4	21.6#




Manual Integrations
APPROVED


UMANGI
3/7/2016 12:36:06 PM



#36
Dibenzo(a,h)anthracene
Concen: 0.11 ng
RT: 25.18 min Scan# 1504
Delta R.T. 0.02 min
Lab File: BM004558.D
Acq: 05 Mar 2016 16:19

Tgt Ion	Ratio	Lower	Upper
278	100		
139	44.4	21.7	32.5#
279	39.8	20.2	30.4#



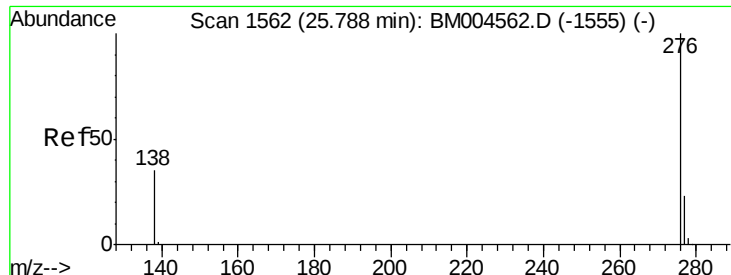

#37
 Benzo(g,h,i)perylene
 Concen: 0.11 ng
 RT: 25.82 min Scan# 1565
 Delta R.T. 0.03 min
 Lab File: BM004558.D
 Acq: 05 Mar 2016 16:19

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC0.1

Tgt Ion	Ratio	Lower	Upper
276	100		
277	30.9	19.1	28.7#
138	48.9	29.3	43.9#

Manual Integrations
 APPROVED

UMANGI
 3/7/2016 12:36:06 PM

