

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030516\
 Data File : BM004562.D
 Acq On : 05 Mar 2016 18:44
 Operator : SJ/UM
 Sample : SSTDICCC001
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICCC001

Manual Integrations
 APPROVED

UMANGI
 3/7/2016 12:36:42 PM

Quant Time: Mar 07 07:31:40 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM030516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 07 07:21:48 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.29	152	25679	5.00	ng	0.00
7) Naphthalene-d8	10.06	136	100811	5.00	ng	0.00
13) Acenaphthene-d10	13.97	164	56139	5.00	ng	0.00
19) Phenanthrene-d10	16.73	188	142828	5.00	ng	0.00
25) Chrysene-d12	20.98	240	119900	5.00	ng	0.00
34) Perylene-d12	23.08	264	109152	5.00	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.01	112	5472	1.00	ng	0.00
5) Phenol-d6	6.63	99	6593	1.05	ng	0.00
8) Nitrobenzene-d5	8.47	82	4833	1.05	ng	0.00
14) 2,4,6-Tribromophenol	15.50	330	1761	1.01	ng	0.00
15) 2-Fluorobiphenyl	12.58	172	16310	0.92	ng	0.00
28) Terphenyl-d14	19.41	244	15834	0.69	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	2.87	88	2509	0.89	ng	# 100
3) n-Nitrosodimethylamine	3.20	42	1770	0.98	ng	# 100
6) bis(2-Chloroethyl)ether	6.75	93	5721	0.97	ng	# 23
9) Nitrobenzene	8.51	77	5290	1.04	ng	# 100
10) Naphthalene	10.10	128	20627	0.86	ng	# 100
11) Hexachlorobutadiene	10.39	225	3938	0.96	ng	# 100
12) 2-Methylnaphthalene	11.75	142	14398	0.99	ng	# 100
16) Acenaphthylene	13.68	152	25279	0.96	ng	# 42
17) Acenaphthene	14.04	154	14645	0.88	ng	# 100
18) Fluorene	15.04	166	20490	1.01	ng	# 76
20) Hexachlorobenzene	16.07	284	5873	0.93	ng	# 100
21) Pentachlorophenol	16.47	266	463	0.52	ng	# 100
22) Phenanthrene	16.78	178	27850	0.80	ng	# 100
23) Anthracene	16.88	178	26286	0.83	ng	# 100
24) Fluoranthene	18.83	202	35927	0.79	ng	# 97
26) Benzidine	19.07	184	4097	0.43	ng	# 100
27) Pyrene	19.19	202	38055	0.82	ng	# 84
29) Benzo(a)anthracene	20.96	228	33838m	0.84	ng	# 100
30) 3,3'-Dichlorobenzidine	20.92	252	11477	1.00	ng	# 100
31) Chrysene	21.02	228	34497m	0.70	ng	# 100
32) Bis(2-ethylhexyl)phthalate	20.90	149	23648	0.94	ng	# 44
33) Indeno(1,2,3-cd)pyrene	25.16	276	31642	0.90	ng	# 81
35) Benzo(a)pyrene	22.99	252	30551	0.94	ng	# 100
36) Dibenzo(a,h)anthracene	25.16	278	24528	0.91	ng	# 100
37) Benzo(g,h,i)perylene	25.79	276	27257	0.90	ng	# 100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030516\
Data File : BM004562.D
Acq On : 05 Mar 2016 18:44
Operator : SJ/UM
Sample : SSTDICCC001
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
SSTDICCC001

Manual Integrations
APPROVED

UMANGI
3/7/2016 12:36:42 PM

Quant Time: Mar 07 07:31:40 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM030516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 07 07:21:48 2016
Response via : Initial Calibration

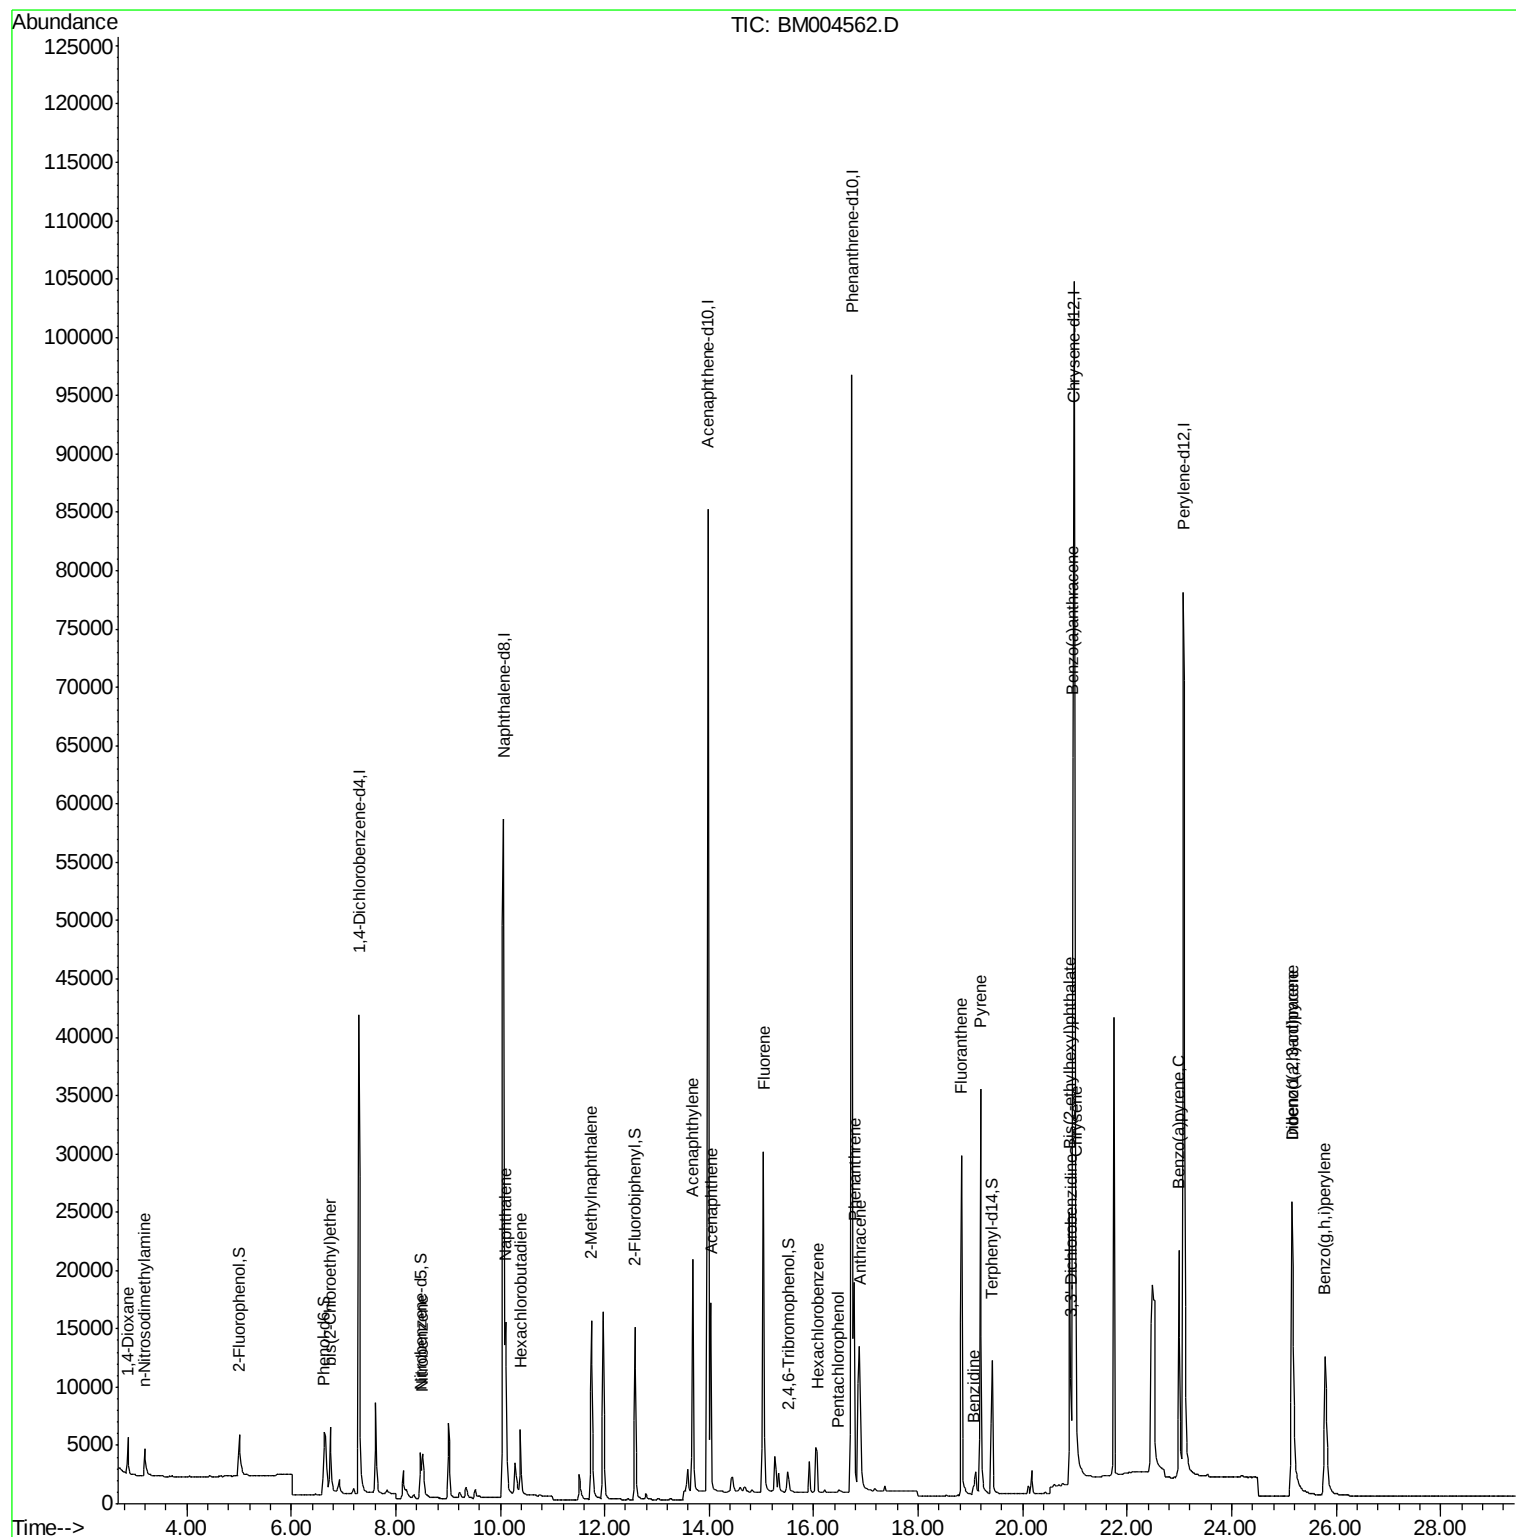



#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 7.29 min Scan# 291

Delta R.T. 0.00 min

Lab File: BM004562.D


Acq: 05 Mar 2016 18:44

Instrument :

BNA_M

ClientSampled :

SSTDICCC001

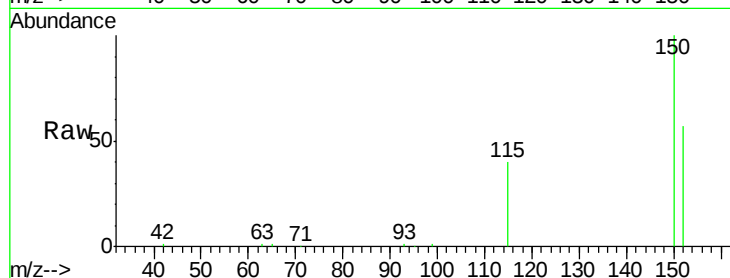

Tgt Ion: 152 Resp: 25679

Ion Ratio Lower Upper

152 100




150 175.1 140.1 210.1

115 70.1 56.1 84.1

Manual Integrations
APPROVED

UMANGI

3/7/2016 12:36:42 PM

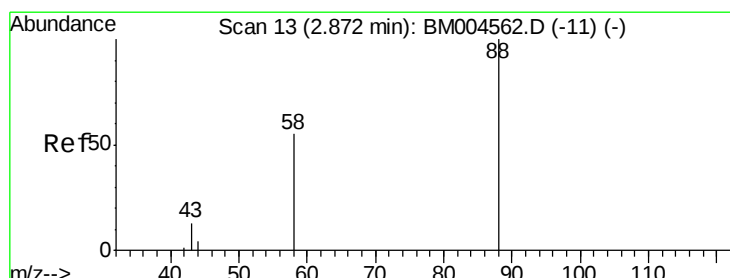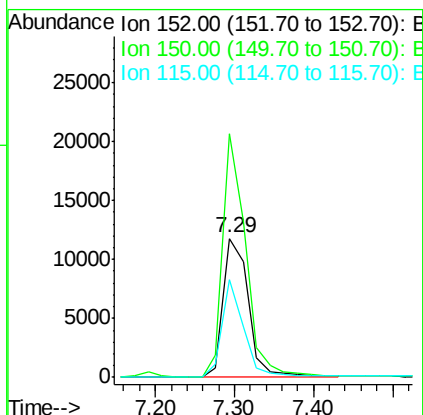

#2

1,4-Dioxane

Concen: 0.89 ng

RT: 2.87 min Scan# 13

Delta R.T. 0.00 min

Lab File: BM004562.D

Acq: 05 Mar 2016 18:44




Tgt Ion: 88 Resp: 2509


Ion Ratio Lower Upper

88 100

58 58.3 0.0 0.0#

43 27.7 0.0 0.0#

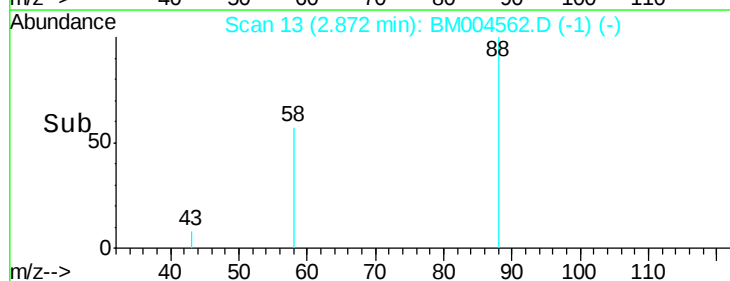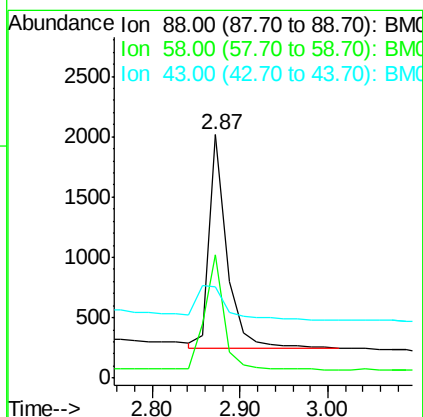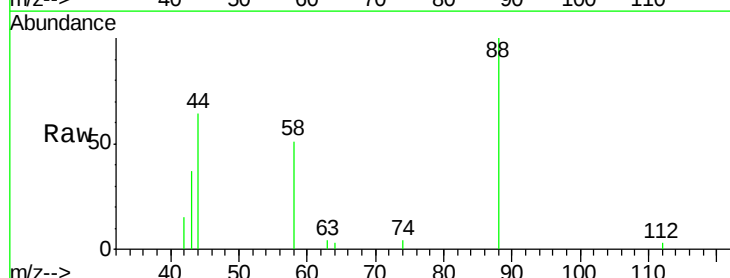



#3





n-Nitrosodimethylamine
 Concen: 0.98 ng
 RT: 3.20 min Scan# 34
 Delta R.T. 0.00 min
 Lab File: BM004562.D
 Acq: 05 Mar 2016 18:44

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC001

Tgt Ion	Ratio	Lower	Upper
42	100		
74	165.5	0.0	0.0#
44	9.7	0.0	0.0#

Manual Integrations
 APPROVED




UMANGI
 3/7/2016 12:36:42 PM

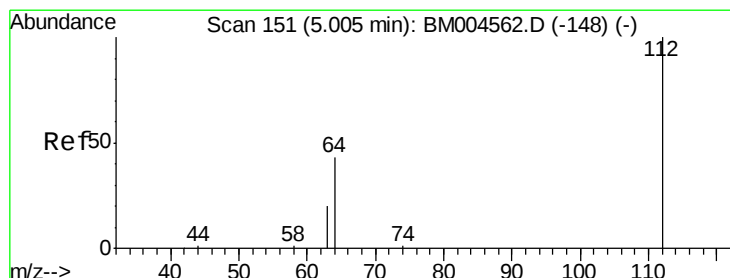

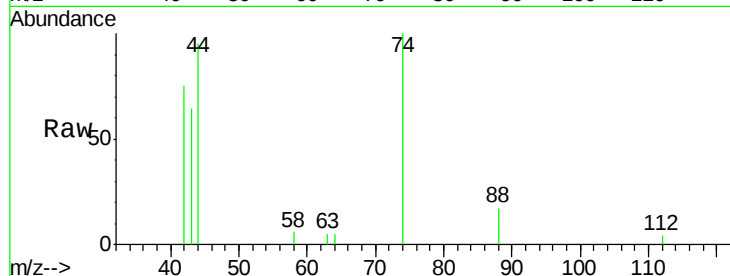


#4

2-Fluorophenol
 Concen: 1.00 ng
 RT: 5.01 min Scan# 151
 Delta R.T. 0.00 min
 Lab File: BM004562.D
 Acq: 05 Mar 2016 18:44

Tgt Ion	Ratio	Lower	Upper
112	100		
64	47.6	0.0	0.0#
63	23.1	0.0	0.0#

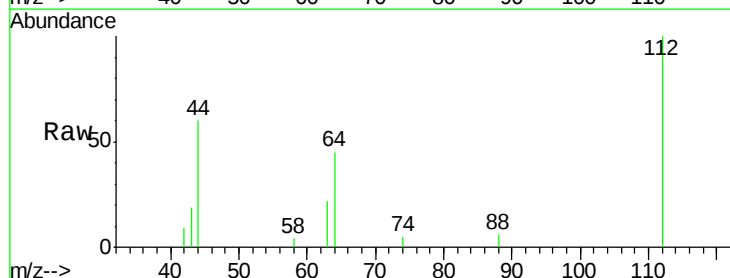



#5

Phenol-d6

Concen: 1.05 ng

RT: 6.63 min Scan# 252

Delta R.T. 0.00 min

Lab File: BM004562.D

Acq: 05 Mar 2016 18:44

Tgt Ion	Ratio	Resp	Lower	Upper
99	100	6593		
42	15.4	0.0	0.0#	
71	27.3	0.2	0.2#	

Instrument :





BNA_M

ClientSampleId :

SSTDICCC001

Manual Integrations
APPROVED

UMANGI
3/7/2016 12:36:42 PM



#6

bis(2-Chloroethyl)ether

Concen: 0.97 ng


RT: 6.75 min Scan# 259


Delta R.T. 0.00 min

Lab File: BM004562.D

Acq: 05 Mar 2016 18:44

Tgt Ion	Ratio	Resp	Lower	Upper
93	100	5721		
63	60.9	18.7	28.1#	
95	29.8	0.0	0.0#	



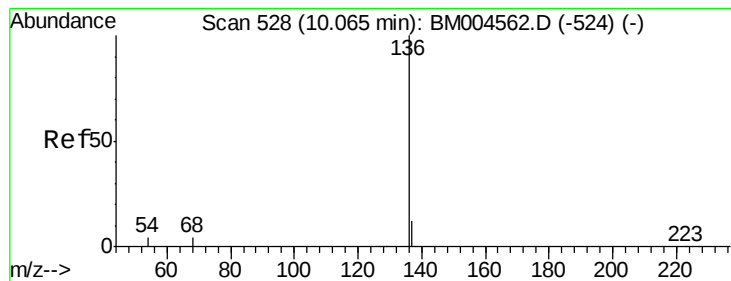

#7

Naphthalene-d8

Concen: 5.00 ng

RT: 10.06 min Scan# 528

Delta R.T. 0.00 min

Lab File: BM004562.D


Acq: 05 Mar 2016 18:44

Instrument :

BNA_M

ClientSampleId :

SSTDICCC001



Tgt Ion: 136 Resp: 100811

Ion Ratio Lower Upper

136 100


137 11.5 9.2 13.8

54 3.7 3.0 4.4

68 3.6 2.9 4.3

Manual Integrations
APPROVED

UMANGI
3/7/2016 12:36:42 PM





Abundance Ion 136.00 (135.70 to 136.70): B

Ion 137.00 (136.70 to 137.70): B

Ion 54.00 (53.70 to 54.70): B

Ion 68.00 (67.70 to 68.70): B

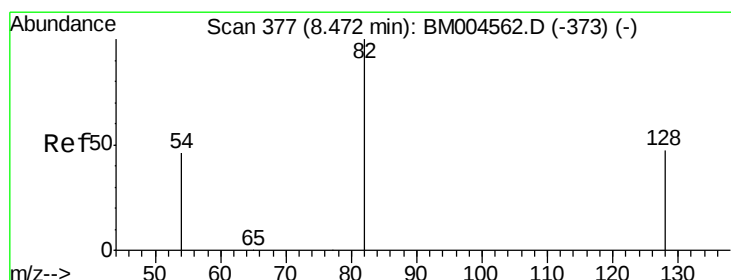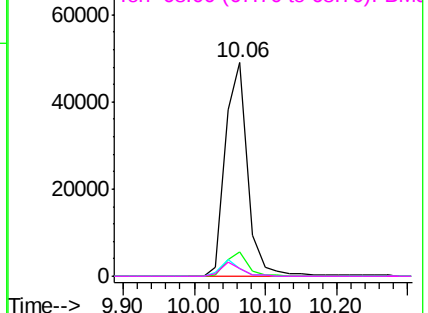

#8

Nitrobenzene-d5

Concen: 1.05 ng

RT: 8.47 min Scan# 377

Delta R.T. 0.00 min

Lab File: BM004562.D

Acq: 05 Mar 2016 18:44


Tgt Ion: 82 Resp: 4833

Ion Ratio Lower Upper

82 100

128 48.3 38.6 58.0



54 48.1 38.5 57.7




Abundance Ion 82.00 (81.70 to 82.70): B

Ion 128.00 (127.70 to 128.70): B

Ion 54.00 (53.70 to 54.70): B

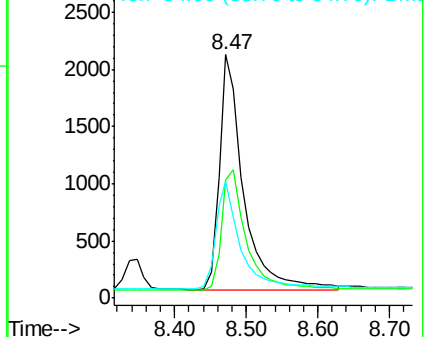



#9

Nitrobenzene

Concen: 1.04 ng

RT: 8.51 min Scan# 381

Delta R.T. 0.00 min

Lab File: BM004562.D

Acq: 05 Mar 2016 18:44

Instrument :

BNA_M





ClientSampleId :

SSTDICCC001

Tgt Ion:	77	Resp:	5290
Ion	Ratio	Lower	Upper
77	100		
123	55.2	0.0	0.0#
65	12.4	0.0	0.0#

Manual Integrations
APPROVED

UMANGI
3/7/2016 12:36:42 PM

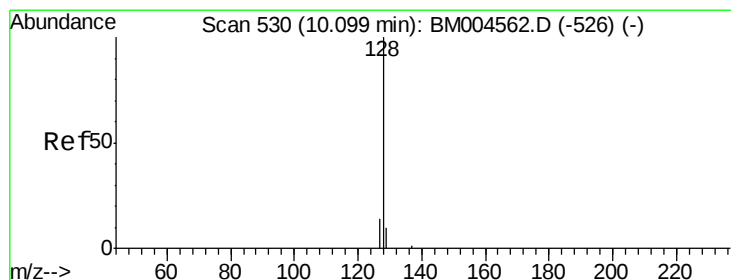

#10

Naphthalene

Concen: 0.86 ng




RT: 10.10 min Scan# 530


Delta R.T. 0.00 min

Lab File: BM004562.D

Acq: 05 Mar 2016 18:44

Tgt Ion:	128	Resp:	20627
Ion	Ratio	Lower	Upper
128	100		
129	10.9	8.7	13.1
127	14.1	11.3	16.9









#11
Hexachlorobutadiene
Concen: 0.96 ng
RT: 10.39 min Scan# 547
Delta R.T. 0.00 min
Lab File: BM004562.D
Acq: 05 Mar 2016 18:44

Instrument :
BNA_M
ClientSampleId :
SSTDICCC001

Tgt Ion	Ratio	Resp	Lower	Upper
225	100	3938		
223	62.4	0.0	0.0	0.0
227	63.8	0.0	0.0	0.0




Manual Integrations
APPROVED


UMANGI
3/7/2016 12:36:42 PM



#12
2-Methylnaphthalene
Concen: 0.99 ng
RT: 11.75 min Scan# 654
Delta R.T. 0.00 min
Lab File: BM004562.D
Acq: 05 Mar 2016 18:44

Tgt Ion	Ratio	Resp	Lower	Upper
142	100	14398		
141	90.4	72.3	108.5	
115	31.8	25.4	38.2	





#13

Acenaphthene-d10

Concen: 5.00 ng

RT: 13.97 min Scan# 844

Delta R.T. 0.00 min

Lab File: BM004562.D


Acq: 05 Mar 2016 18:44

Instrument :

BNA_M

ClientSampleId :




SSTDICCC001

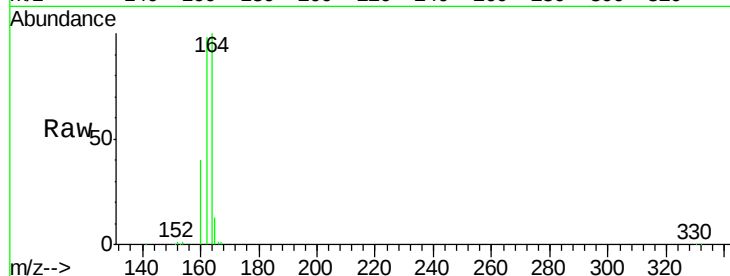

Tgt Ion:	164	Resp:	56139
Ion Ratio	Lower	Upper	
164	100		
162	97.7	78.2	117.2
160	39.9	31.9	47.9

Manual Integrations
APPROVED

UMANGI
3/7/2016 12:36:42 PM

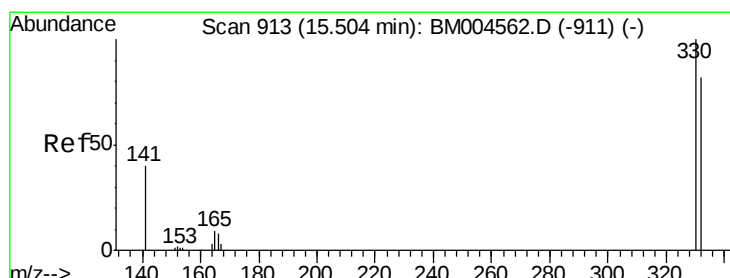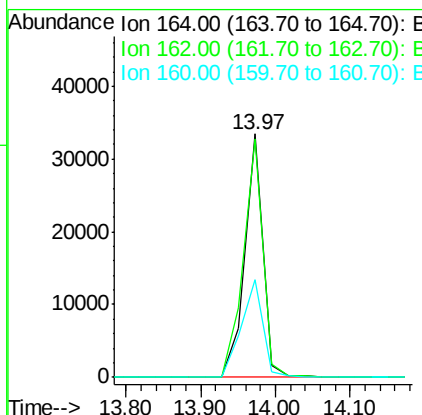

#14

2,4,6-Tribromophenol

Concen: 1.01 ng




RT: 15.50 min Scan# 913


Delta R.T. 0.00 min

Lab File: BM004562.D

Acq: 05 Mar 2016 18:44

Tgt Ion:	330	Resp:	1761
Ion Ratio	Lower	Upper	
330	100		
332	93.7	0.0	0.0#
141	44.7	0.0	0.0#

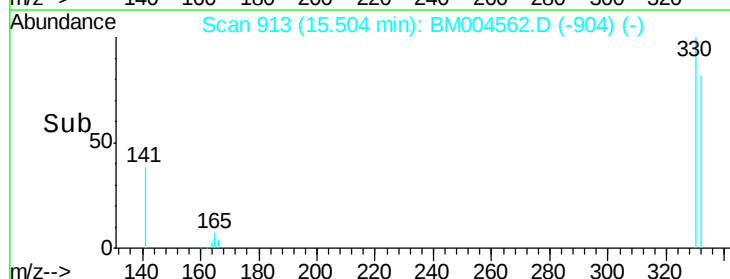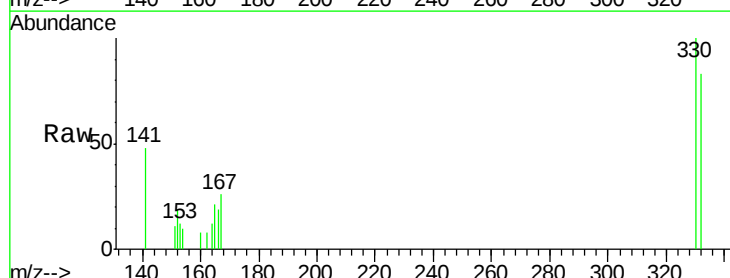

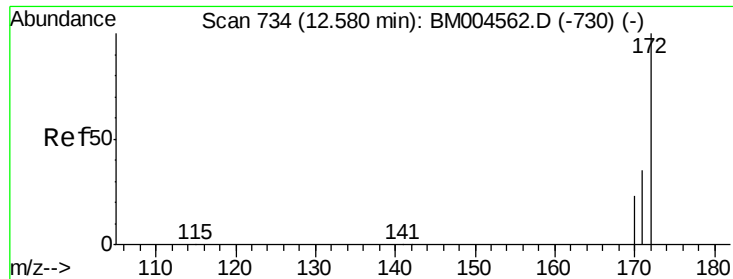





#15
2-Fluorobiphenyl
Concen: 0.92 ng
RT: 12.58 min Scan# 734
Delta R.T. 0.00 min
Lab File: BM004562.D
Acq: 05 Mar 2016 18:44

Instrument :
BNA_M
ClientSampleId :
SSTDICCC001

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.7	28.6	42.8
170	23.9	19.1	28.7




Manual Integrations
APPROVED


UMANGI
3/7/2016 12:36:42 PM

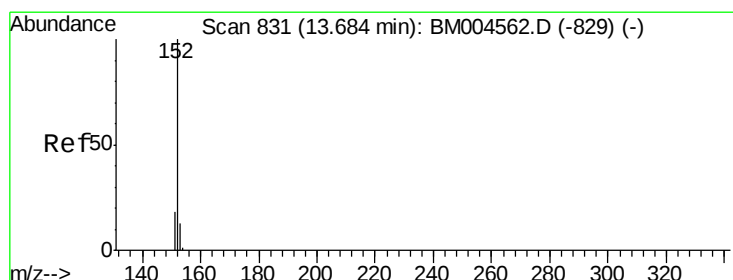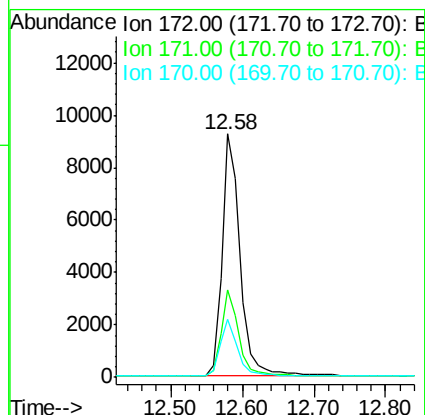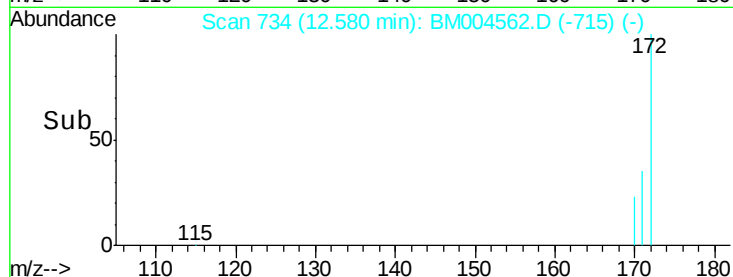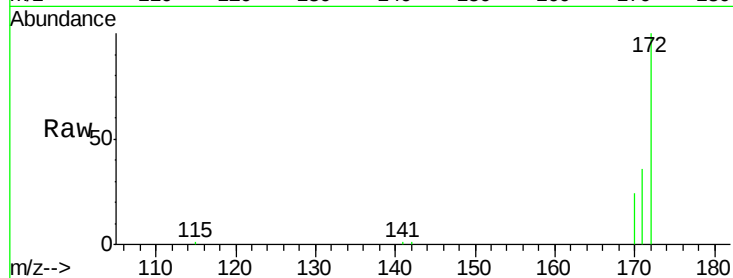

#16
Acenaphthylene
Concen: 0.96 ng
RT: 13.68 min Scan# 831
Delta R.T. 0.00 min
Lab File: BM004562.D
Acq: 05 Mar 2016 18:44

Tgt Ion	Ratio	Lower	Upper
152	100		
151	19.1	9.2	13.8#
153	13.2	51.4	77.0#

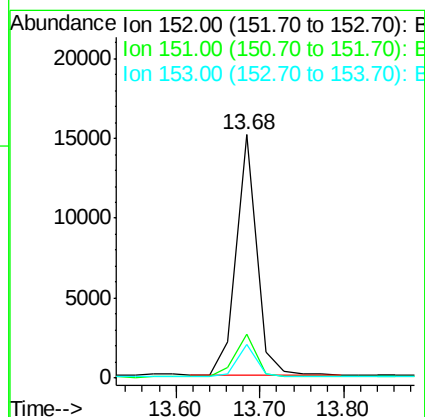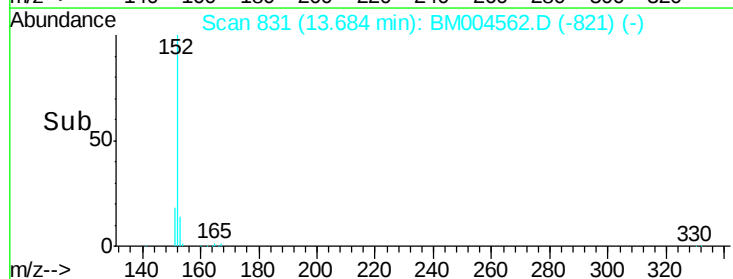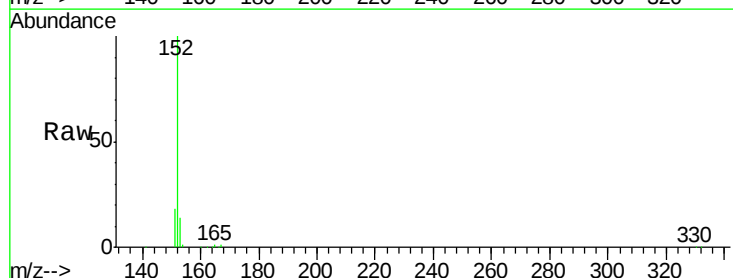







#17
Acenaphthene
Concen: 0.88 ng
RT: 14.04 min Scan# 847
Delta R.T. 0.00 min
Lab File: BM004562.D
Acq: 05 Mar 2016 18:44

Instrument :
BNA_M
ClientSampleId :
SSTDICCC001

Tgt Ion	Ratio	Resp Lower	Resp Upper
154	100		
153	0.0	0.0	0.0
152	0.0	0.2	0.2#




Manual Integrations
APPROVED


UMANGI
3/7/2016 12:36:42 PM

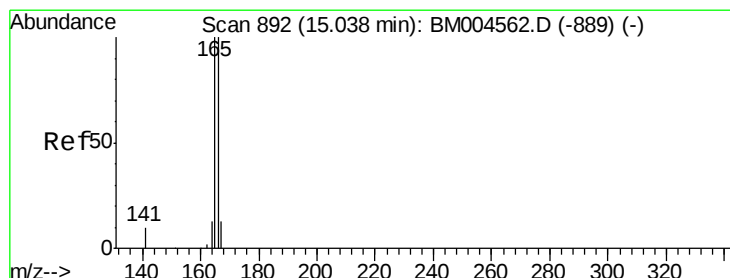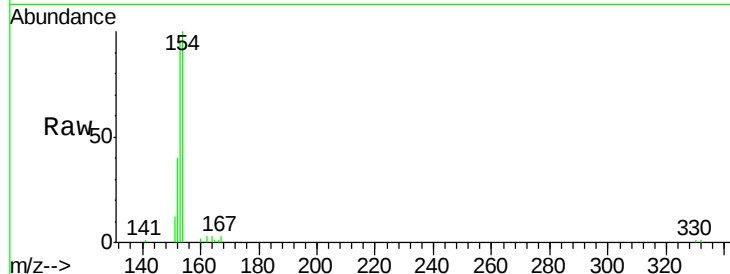

#18
Fluorene
Concen: 1.01 ng
RT: 15.04 min Scan# 892
Delta R.T. 0.00 min
Lab File: BM004562.D
Acq: 05 Mar 2016 18:44

Tgt Ion	Ratio	Resp Lower	Resp Upper
166	100		
165	97.5	0.0	0.0#
167	13.2	20.0	30.0#

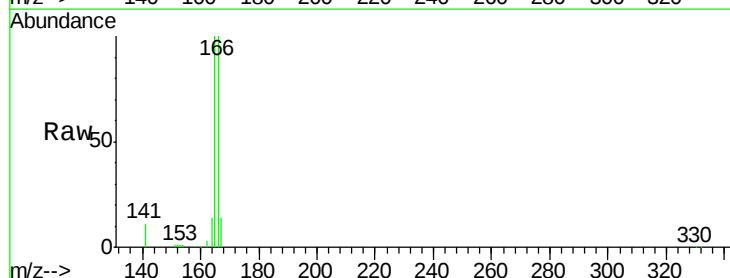



#19

Phenanthrene-d10

Concen: 5.00 ng

RT: 16.73 min Scan# 964

Delta R.T. 0.00 min

Lab File: BM004562.D

Acq: 05 Mar 2016 18:44

Instrument :

BNA_M





ClientSampleId :

SSTDICCC001

Tgt Ion:	188	Resp:	142828
Ion Ratio	Lower	Upper	
188	100		
94	7.5	6.0	9.0
80	6.6	5.3	7.9

Manual Integrations
APPROVED

UMANGI
3/7/2016 12:36:42 PM

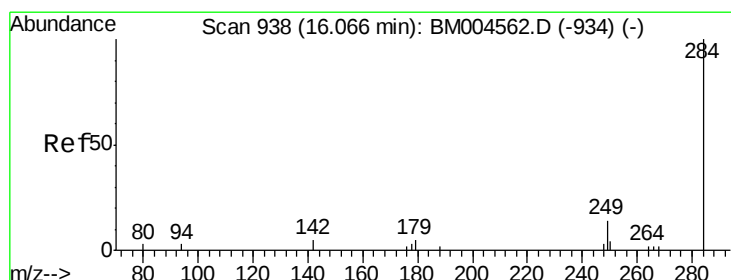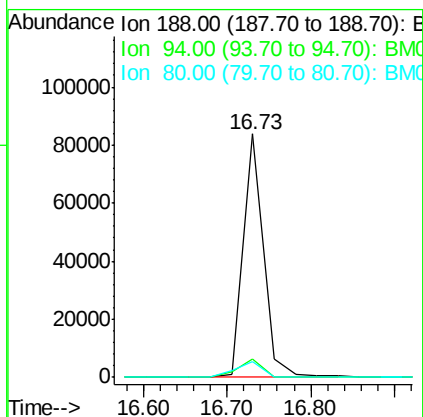

#20

Hexachlorobenzene

Concen: 0.93 ng




RT: 16.07 min Scan# 938


Delta R.T. 0.00 min

Lab File: BM004562.D

Acq: 05 Mar 2016 18:44

Tgt Ion:	284	Resp:	5873
Ion Ratio	Lower	Upper	
284	100		
142	0.0	0.0	0.0
249	0.0	0.0	0.0

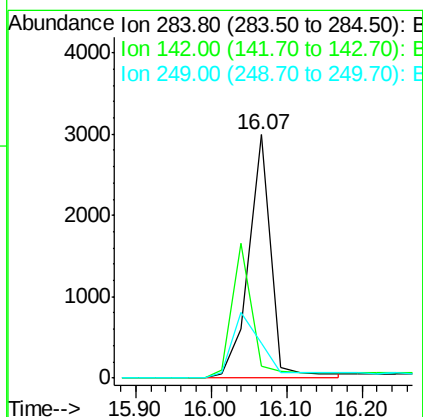




#21
 Pentachlorophenol
 Concen: 0.52 ng
 RT: 16.47 min Scan# 954
 Delta R.T. 0.00 min
 Lab File: BM004562.D
 Acq: 05 Mar 2016 18:44

Instrument :
 BNA_M
 ClientSampleId :
 SSTD1CCC001




Tgt Ion	Ratio	Lower	Upper
266	100		
268	78.3	62.6	94.0
264	71.7	57.4	86.0

Manual Integrations
 APPROVED

UMANGI
 3/7/2016 12:36:42 PM




Abundance Ion 265.70 (265.40 to 266.40): E
 Ion 268.00 (267.70 to 268.70): E
 Ion 264.00 (263.70 to 264.70): E


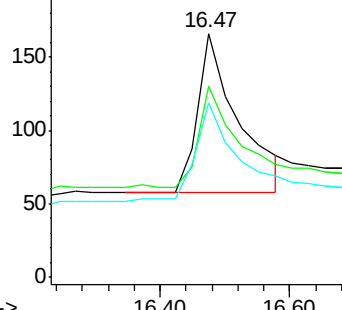



#22
 Phenanthrene
 Concen: 0.80 ng
 RT: 16.78 min Scan# 966
 Delta R.T. 0.00 min
 Lab File: BM004562.D
 Acq: 05 Mar 2016 18:44

Tgt Ion	Ratio	Lower	Upper
178	100		
176	18.6	0.0	0.0#
179	16.1	0.0	0.0#



Abundance Ion 178.00 (177.70 to 178.70): E
 Ion 176.00 (175.70 to 176.70): E
 Ion 179.00 (178.70 to 179.70): E

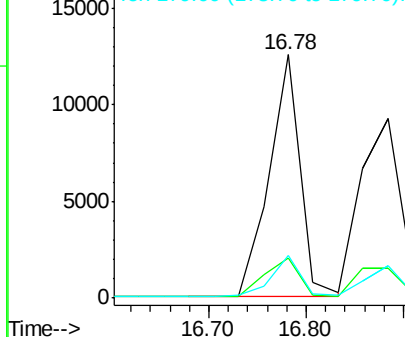

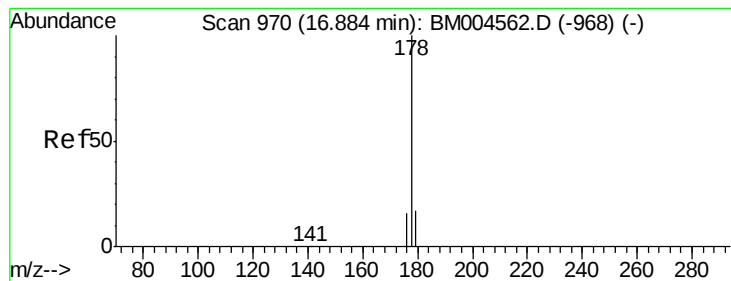

#23

Anthracene

Concen: 0.83 ng

RT: 16.88 min Scan# 970

Delta R.T. 0.00 min

Lab File: BM004562.D

Acq: 05 Mar 2016 18:44

Instrument :

BNA_M





ClientSampleId :

SSTDICCC001

Tgt Ion	Ratio	Lower	Upper
178	100		
176	0.0	0.0	0.0
179	15.1	0.0	0.0

Manual Integrations
APPROVED

UMANGI
3/7/2016 12:36:42 PM

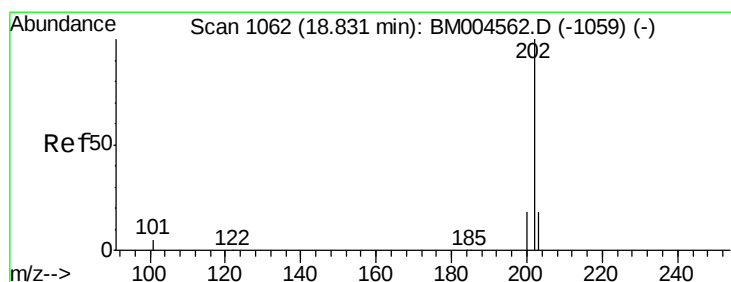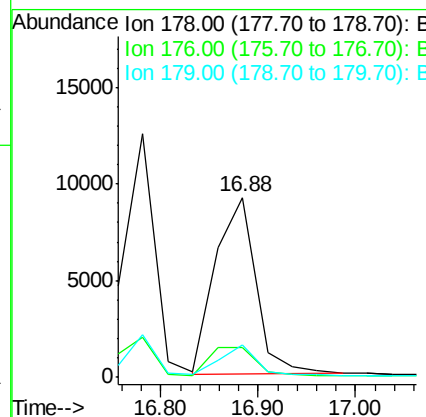

#24

Fluoranthene

Concen: 0.79 ng




RT: 18.83 min Scan# 1062


Delta R.T. 0.00 min

Lab File: BM004562.D

Acq: 05 Mar 2016 18:44

Tgt Ion	Ratio	Lower	Upper
202	100		
101	13.2	12.2	18.4
203	17.4	14.6	21.8

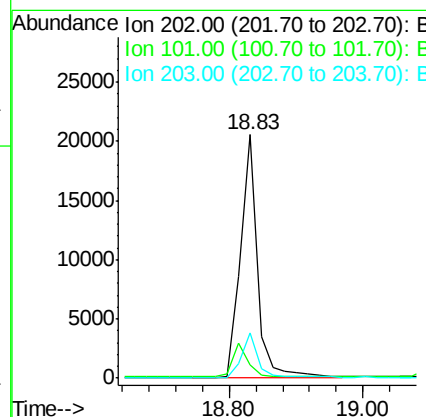



#25

Chrysene-d12

Concen: 5.00 ng

RT: 20.98 min Scan# 1183

Delta R.T. 0.00 min

Lab File: BM004562.D


Acq: 05 Mar 2016 18:44

Instrument :

BNA_M

ClientSampleId :

SSTDICCC001



Tgt Ion: 240 Resp: 119900

Ion Ratio Lower Upper


240 100

120 4.4 3.5 5.3

236 25.4 20.3 30.5

Manual Integrations
APPROVED



UMANGI
3/7/2016 12:36:42 PM



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

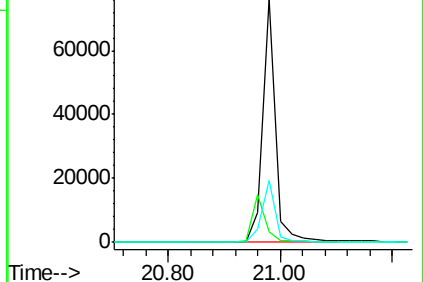

#26

Benzidine

Concen: 0.43 ng

RT: 19.07 min Scan# 1076

Delta R.T. 0.00 min

Lab File: BM004562.D

Acq: 05 Mar 2016 18:44


Tgt Ion: 184 Resp: 4097

Ion Ratio Lower Upper

184 100

185 24.2 19.4 29.0



183 20.6 16.5 24.7




Abundance Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E

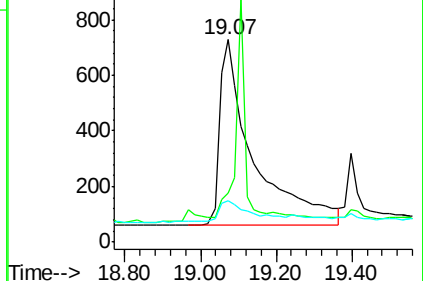







#27
 Pyrene
 Concen: 0.82 ng
 RT: 19.19 min Scan# 1083
 Delta R.T. 0.00 min
 Lab File: BM004562.D
 Acq: 05 Mar 2016 18:44

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC001

Tgt Ion	Ratio	Resp Lower	Resp Upper
202	100		
200	20.9	0.2	0.2#
203	17.3	0.0	0.0#




Manual Integrations
 APPROVED


UMANGI
 3/7/2016 12:36:42 PM

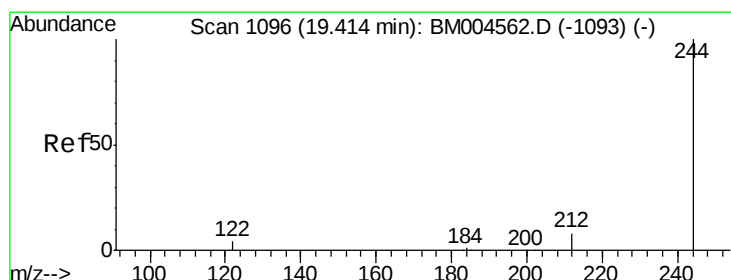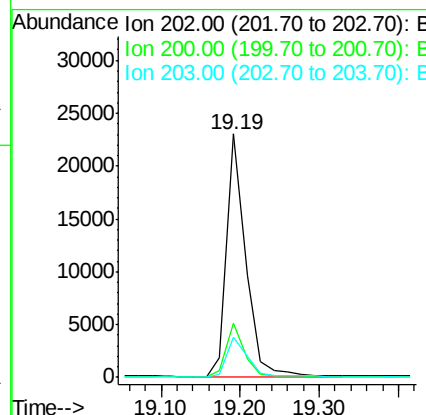

#28
 Terphenyl-d14
 Concen: 0.69 ng
 RT: 19.41 min Scan# 1096
 Delta R.T. 0.00 min
 Lab File: BM004562.D
 Acq: 05 Mar 2016 18:44

Tgt Ion	Ratio	Resp Lower	Resp Upper
244	100		
212	8.7	7.0	10.4
122	5.3	4.2	6.4

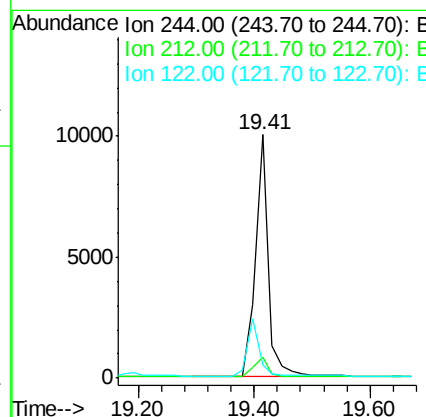



#29

Benzo(a)anthracene

Concen: 0.84 ng m

RT: 20.96 min Scan# 1182

Delta R.T. 0.00 min

Lab File: BM004562.D


Acq: 05 Mar 2016 18:44

Instrument :

BNA_M

ClientSampleId :




SSTDICCC001



Tgt Ion	Ratio	Lower	Upper
228	100		
226	25.4	20.3	30.5
229	20.4	16.3	24.5

Manual Integrations
APPROVED

UMANGI
3/7/2016 12:36:42 PM

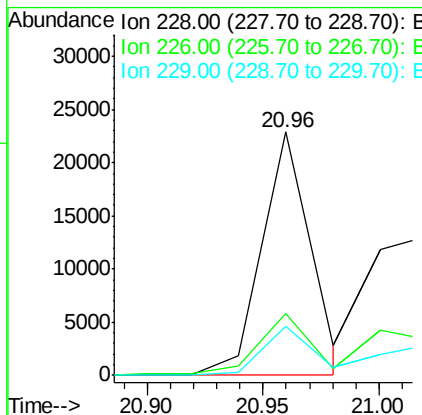

#30

3,3'-Dichlorobenzidine

Concen: 1.00 ng




RT: 20.92 min Scan# 1180


Delta R.T. 0.00 min

Lab File: BM004562.D

Acq: 05 Mar 2016 18:44

Tgt Ion	Ratio	Lower	Upper
252	100		
254	67.4	53.9	80.9
126	8.6	6.9	10.3





#31

Chrysene

Concen: 0.70 ng m

RT: 21.02 min Scan# 1185

Delta R.T. 0.00 min

Lab File: BM004562.D

Acq: 05 Mar 2016 18:44

Instrument :

BNA_M


ClientSampleId :

SSTDICCC001




Tgt Ion:	228	Resp:	34497
Ion Ratio	Lower	Upper	
228	100		
226	25.4	20.3	30.5
229	22.2	17.8	26.6

Manual Integrations
APPROVED

UMANGI
3/7/2016 12:36:42 PM



Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

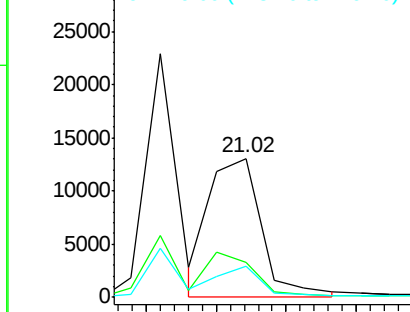

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.94 ng

RT: 20.90 min Scan# 1179




Delta R.T. 0.00 min


Lab File: BM004562.D

Acq: 05 Mar 2016 18:44

Tgt Ion:	149	Resp:	23648
Ion Ratio	Lower	Upper	
149	100		
167	30.4	0.6	0.8#
279	2.1	0.0	0.0#

Abundance Ion 149.00 (148.70 to 149.70): E
Ion 167.00 (166.70 to 167.70): E
Ion 279.00 (278.70 to 279.70): E

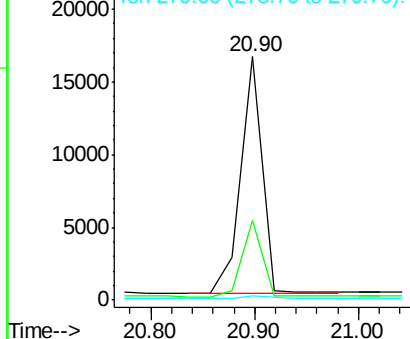







#33
 Indeno(1,2,3-cd)pyrene
 Concen: 0.90 ng
 RT: 25.16 min Scan# 1502
 Delta R.T. 0.00 min
 Lab File: BM004562.D
 Acq: 05 Mar 2016 18:44

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC001

Tgt Ion	Ratio	Lower	Upper
276	100		
138	40.4	22.8	34.2#
277	24.8	15.2	22.8#




Manual Integrations
 APPROVED


UMANGI
 3/7/2016 12:36:42 PM

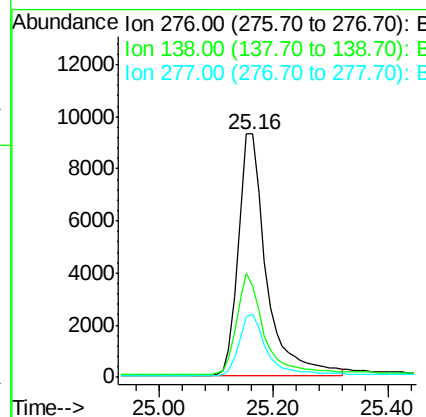

#34
 Perylene-d12
 Concen: 5.00 ng
 RT: 23.08 min Scan# 1302
 Delta R.T. 0.00 min
 Lab File: BM004562.D
 Acq: 05 Mar 2016 18:44

Tgt Ion	Ratio	Lower	Upper
264	100		
260	26.8	21.4	32.2
265	22.3	17.8	26.8

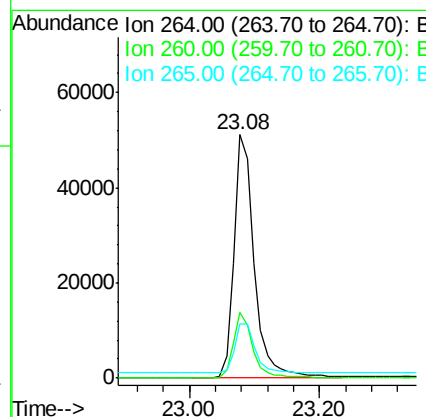

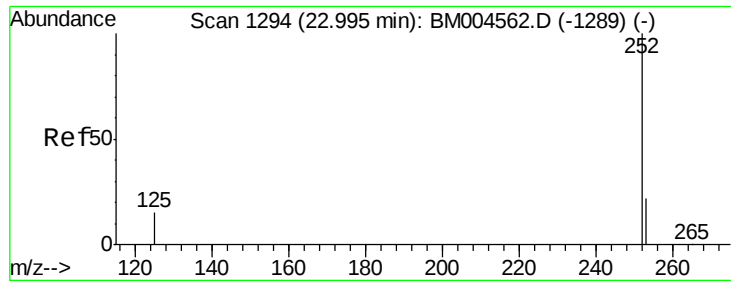





#35
Benzo(a)pyrene
Concen: 0.94 ng
RT: 22.99 min Scan# 1294
Delta R.T. 0.00 min
Lab File: BM004562.D
Acq: 05 Mar 2016 18:44

Instrument :
BNA_M
ClientSampleId :
SSTDICCC001

Tgt Ion:	252	Resp:	30551
Ion Ratio	Lower	Upper	
252	100		
253	23.8	19.0	28.6
125	18.0	14.4	21.6




Manual Integrations
APPROVED


UMANGI
3/7/2016 12:36:42 PM



#36
Dibenzo(a,h)anthracene
Concen: 0.91 ng
RT: 25.16 min Scan# 1502
Delta R.T. 0.00 min
Lab File: BM004562.D
Acq: 05 Mar 2016 18:44


Tgt Ion:	278	Resp:	24528
Ion Ratio	Lower	Upper	
278	100		
139	27.1	21.7	32.5
279	25.3	20.2	30.4



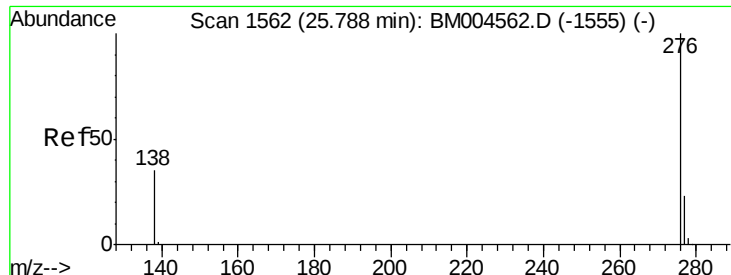

#37
 Benzo(g,h,i)perylene
 Concen: 0.90 ng
 RT: 25.79 min Scan# 1562
 Delta R.T. 0.00 min
 Lab File: BM004562.D
 Acq: 05 Mar 2016 18:44

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC001



Tgt Ion:	276	Resp:	27257
Ion Ratio	Lower	Upper	
276	100		
277	23.9	19.1	28.7
138	36.6	29.3	43.9

Manual Integrations
 APPROVED

UMANGI
 3/7/2016 12:36:42 PM

