


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030516\
 Data File : BM004556.D
 Acq On : 05 Mar 2016 15:06
 Operator : SJ/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM030516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 07 07:54:56 2016

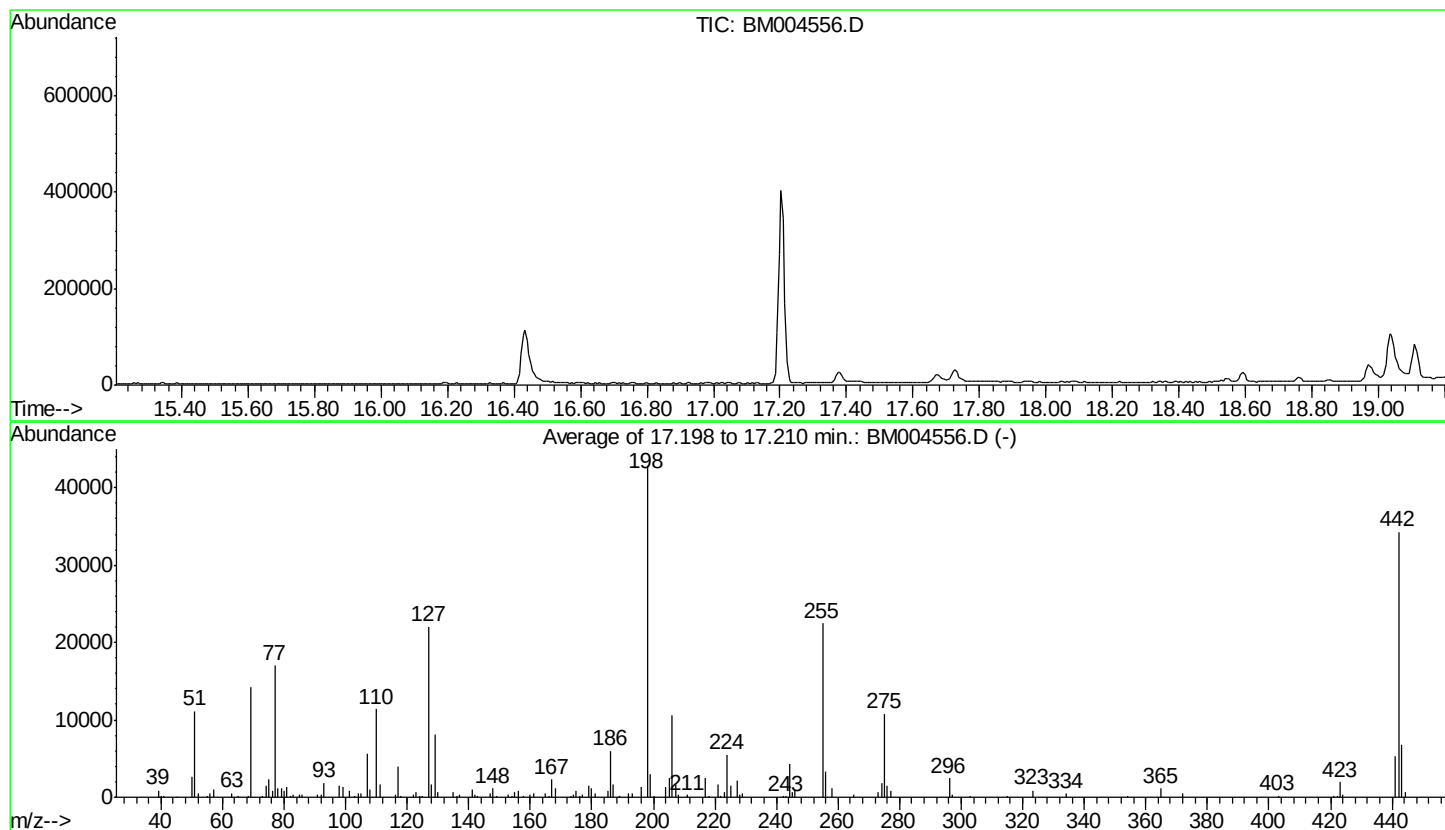

AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.0	11159	PASS
68	69	0.00	2	1.7	237	PASS
69	198	0.00	100	33.1	14178	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.5	22061	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	42853	PASS
199	198	5	9	6.8	2920	PASS
275	198	10	60	25.1	10755	PASS
365	198	1	100	2.7	1150	PASS
441	442	0.01	24	15.3	5245	PASS
442	198	50	100	80.1	34325	PASS
443	442	15	24	19.6	6733	PASS