

Quantitation Report (Qedit)




Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA M\DATA\BM030518\
 Data File : BM014469.D
 Acq On : 05 Mar 2018 12:47
 Operator : SJ/JU
 Sample : J1631-15
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Quant Time: Mar 05 14:15:44 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 02 22:33:42 2018
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 BE603

Manual Integrations
 APPROVED

Sohil
 3/6/2018 5:46:48 PM

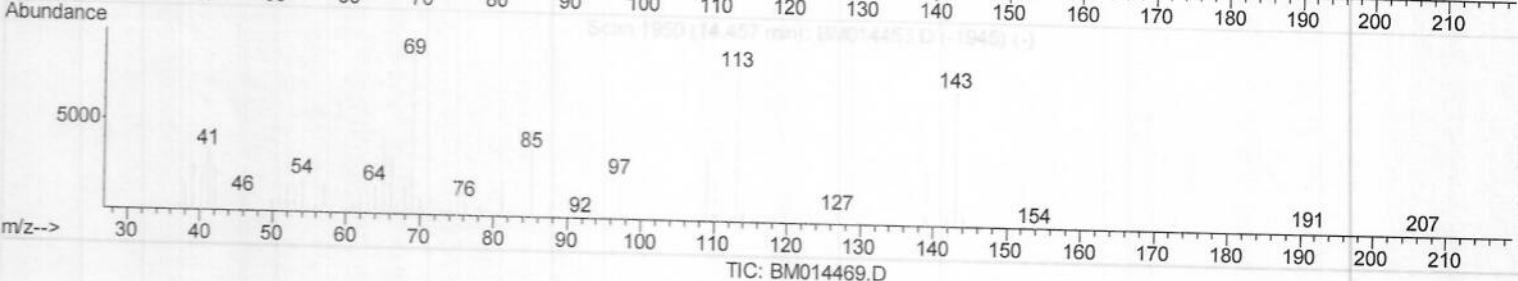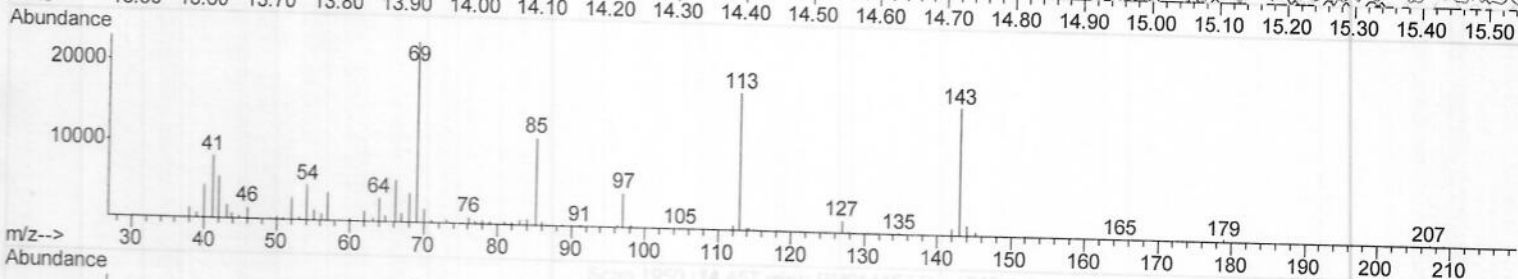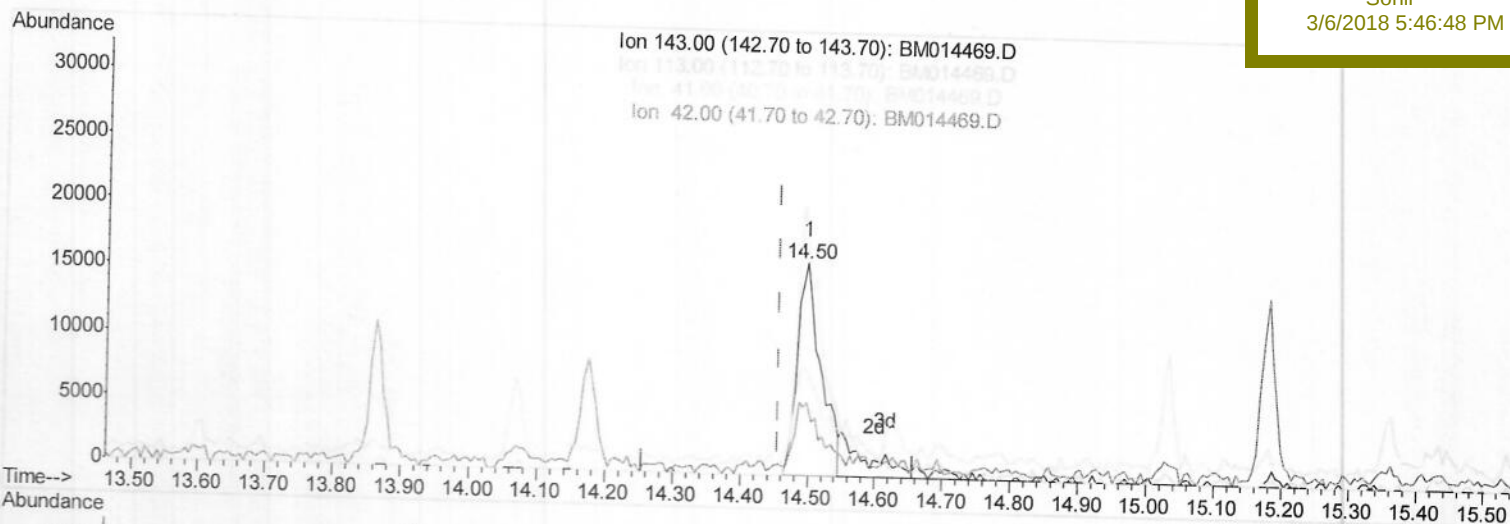

(51) 4-Nitrophenol-d4 (S)

14.498min (+0.041) 17.61ng/ul

response 39663

Ion	Exp%	Act%
143.00	100	100
113.00	114.60	107.85
41.00	34.80	50.08#
42.00	20.50	34.30#

Quantitation Report (Qedit)




Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA M\DATA\BM030518\
 Data File : BM014469.D
 Acq On : 05 Mar 2018 12:47
 Operator : SJ/JU
 Sample : J1631-15
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Quant Time: Mar 05 14:15:44 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 02 22:33:42 2018
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 BE603

Manual Integrations
 APPROVED

Sohil
 3/6/2018 5:46:48 PM

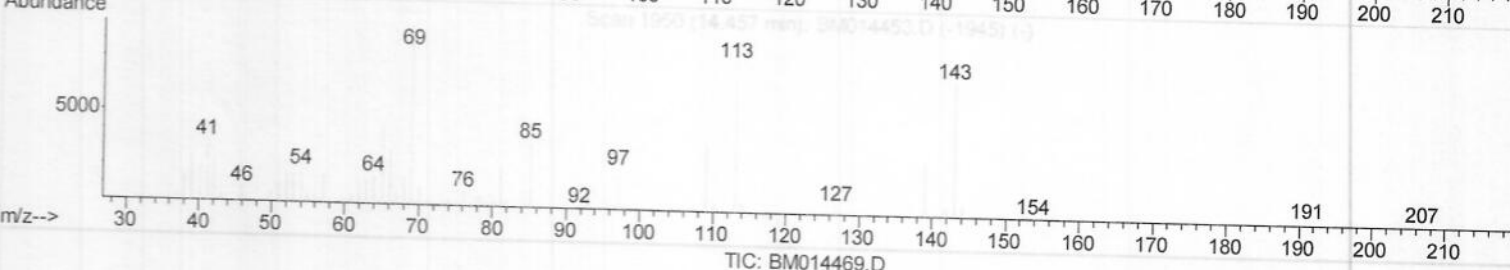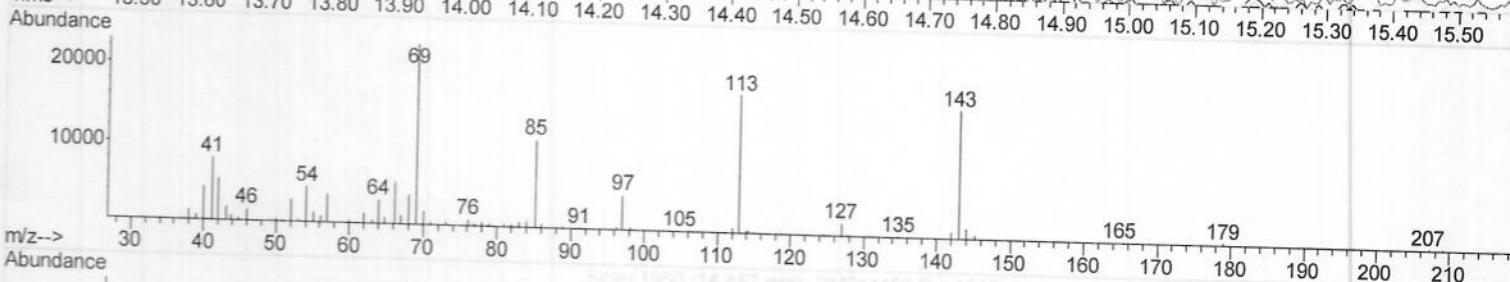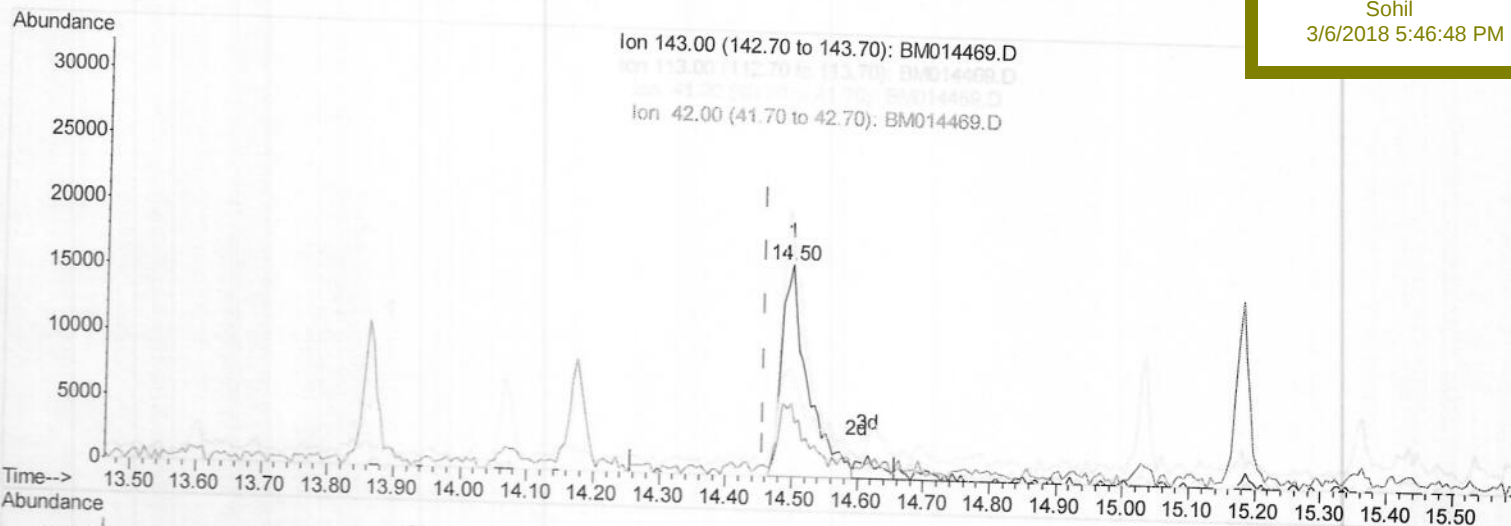

(51) 4-Nitrophenol-d4 (S)
 14.498min (+0.041) 19.99ng/ul m
 response 45025

SJ
03/06/18

Ion	Exp%	Act%
143.00	100	100
113.00	114.60	107.85
41.00	34.80	50.08#
42.00	20.50	34.30#

Quantitation Report (Qedit)


Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA M\DATA\BM030518\
 Data File : BM014469.D
 Acq On : 05 Mar 2018 12:47
 Operator : SJ/JU
 Sample : J1631-15
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BE603

Quant Time: Mar 05 14:15:44 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 02 22:33:42 2018
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 3/6/2018 5:46:48 PM

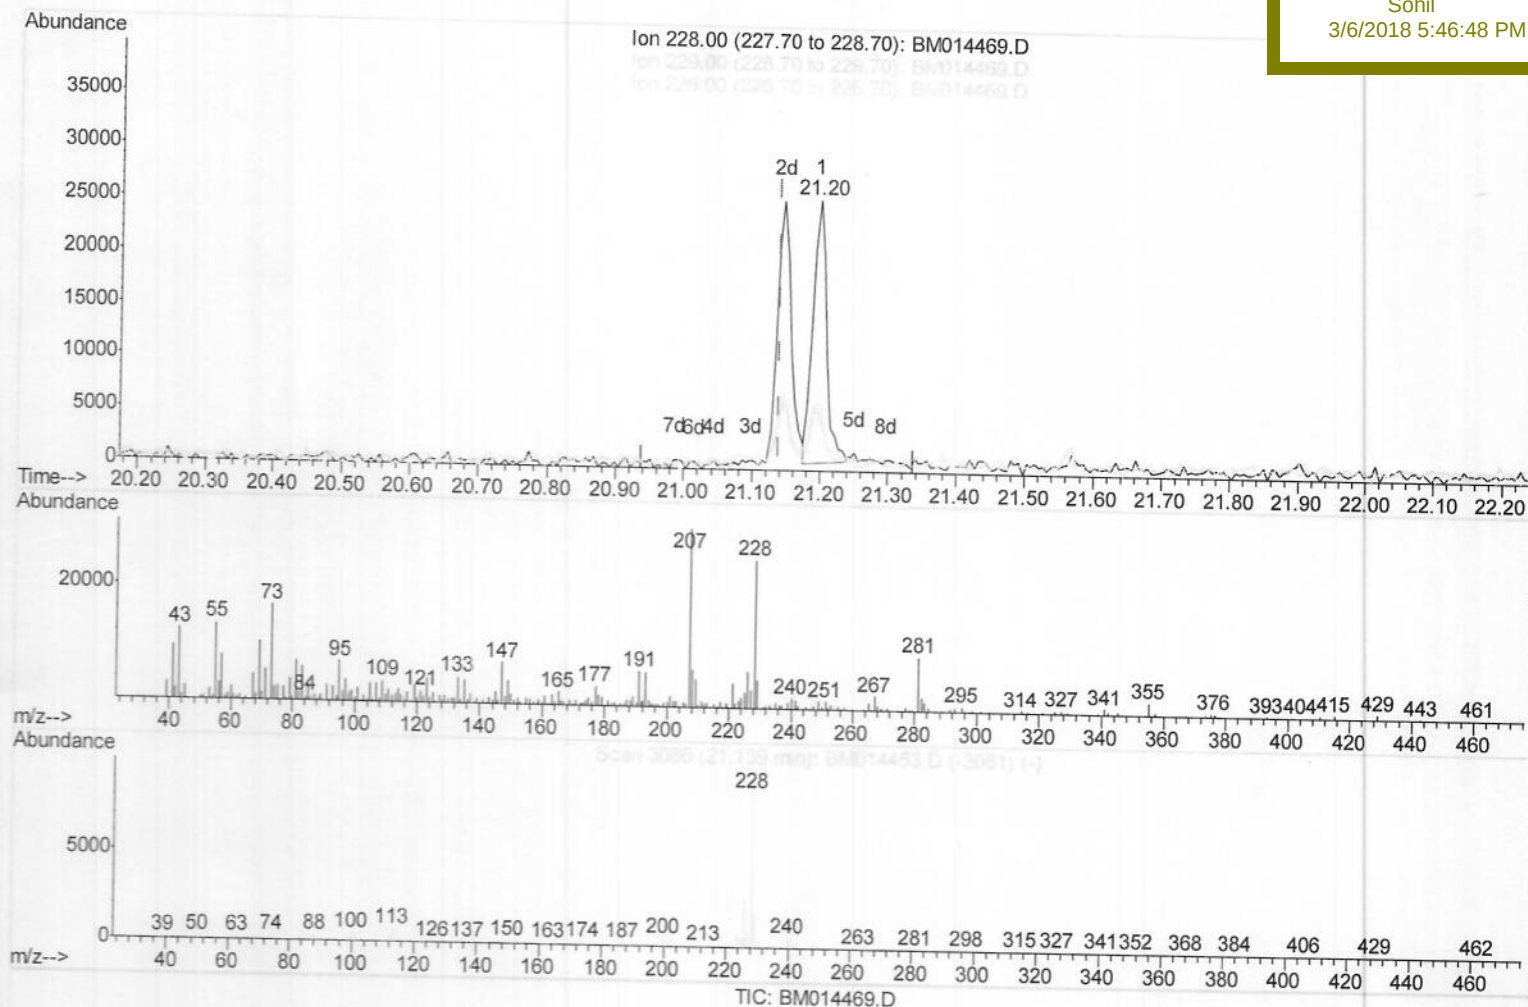

(80) Benzo(a)anthracene

21.197min (+0.059) 1.40ng/ul

response 35048

Ion	Exp%	Act%
228.00	100	100
229.00	19.20	19.67
226.00	26.70	25.22
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA M\DATA\BM030518\
 Data File : BM014469.D
 Acq On : 05 Mar 2018 12:47
 Operator : SJ/JU
 Sample : J1631-15
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Quant Time: Mar 05 14:15:44 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 02 22:33:42 2018
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 BE603

Manual Integrations
 APPROVED

Sohil
 3/6/2018 5:46:48 PM

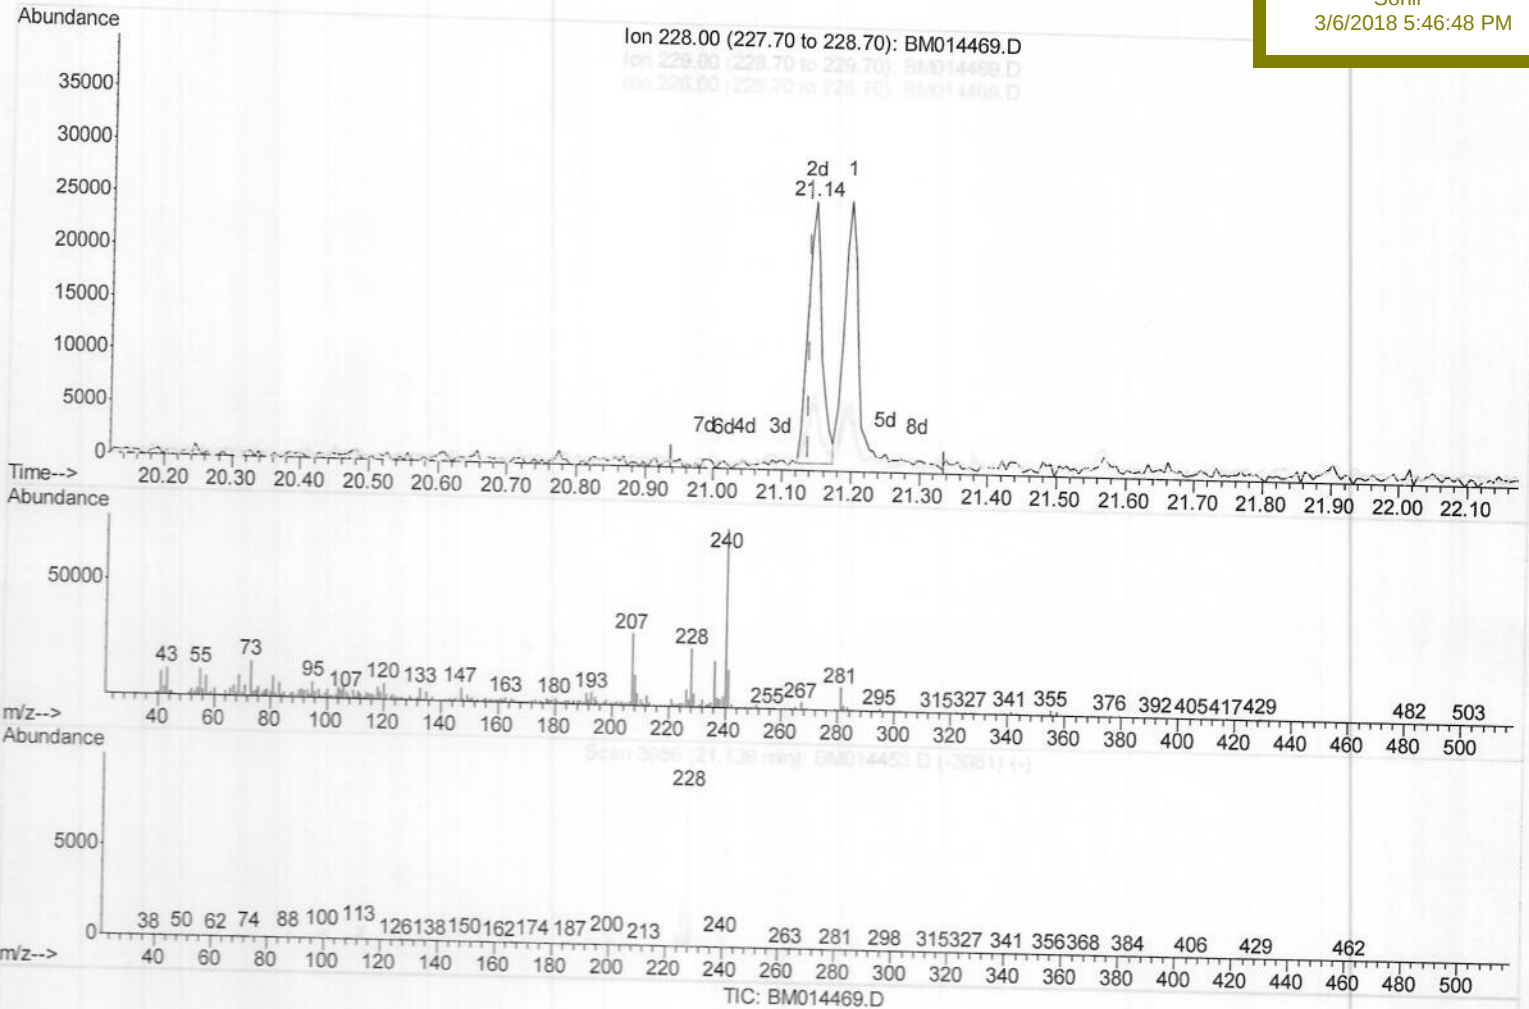

(80) Benzo(a)anthracene

21.144min (+0.006) 1.41ng/ul m

response 35186

Ion Exp% Act%

228.00 100 100

229.00 19.20 24.73#

226.00 26.70 29.22

0.00 0.00 0.00

SJ
 03106118

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA M\DATA\BM030518\
 Data File : BM014469.D
 Acq On : 05 Mar 2018 12:47
 Operator : SJ/JU
 Sample : J1631-15
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 Client Sample Id :
 BE603

Manual Integrations
 APPROVED

Sohil
 3/6/2018 5:46:48 PM

Quant Time: Mar 05 14:32:29 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 02 22:33:42 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.51	152	84526	20.00	ng/ul	0.00
18) Naphthalene-d8	10.29	136	343735	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.17	164	197529	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.94	188	431146	20.00	ng/ul	0.00
75) Chrysene-d12	21.16	240	400874	20.00	ng/ul	0.00
83) Perylene-d12	23.34	264	354339	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.09	96	8828	4.47	ng/uL	0.00
5) Phenol-d5	6.73	99	189527	26.53	ng/ul	0.00
7) Bis-(2-Chloroethyl) ether-d	6.86	67	125732	29.07	ng/ul	0.00
9) 2-Chlorophenol-d4	7.06	132	162594	29.68	ng/ul	0.00
13) 4-Methylphenol-d8	8.25	113	163837	26.21	ng/ul	0.00
19) Nitrobenzene-d5	8.67	128	80124	31.54	ng/ul	0.00
22) 2-Nitrophenol-d4	9.39	143	95226	36.22	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.95	165	146030	26.82	ng/ul	0.01
29) 4-Chloroaniline-d4	10.45	131	135078	25.18	ng/ul	0.00
43) Dimethylphthalate-d6	13.60	166	492329	30.18	ng/ul	0.00
46) Acenaphthylene-d8	13.87	160	620140	30.83	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	45025m	19.99	ng/ul	0.04
57) Fluorene-d10	15.18	176	411294	28.14	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.36	200	53422	20.66	ng/ul	0.01
70) Anthracene-d10	17.04	188	581099	27.94	ng/ul	0.00
76) Pyrene-d10	19.35	212	587356	28.41	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.20	264	474659	27.52	ng/ul	0.00
Target Compounds						
44) Dimethylphthalate	13.64	163	82415	5.124	ng/ul	Ovalue 96
80) Benzo(a)anthracene	21.14	228	35186m	1.406	ng/ul	95
81) Bis(2-ethylhexyl)phthalate	21.07	149	28709	1.820	ng/ul	95
82) Chrysene	21.20	228	35114	1.505	ng/ul	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA M\DATA\BM030518\
Data File : BM014469.D
Acq On : 05 Mar 2018 12:47
Operator : SJ/JU
Sample : J1631-15
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Mar 05 14:32:29 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 02 22:33:42 2018
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
BE603

Manual Integrations
APPROVED

Sohil
3/6/2018 5:46:48 PM

