

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030521\
 Data File : BM028993.D
 Acq On : 05 Mar 2021 13:12
 Operator : CG/JU
 Sample : PB134957BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB134957BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM028993.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.246	379	384	398	rBV	318203	438316	76.13%	13.786%
2	6.875	654	661	672	rBV	279026	430848	74.83%	13.551%
3	7.681	792	798	805	rVB	51173	75651	13.14%	2.379%
4	8.857	991	998	1010	rVB	172541	269379	46.78%	8.473%
5	10.475	1267	1273	1282	rVB	60350	95220	16.54%	2.995%
6	12.963	1690	1696	1704	rVB	372392	508142	88.25%	15.983%
7	14.351	1925	1932	1938	rBV	75547	107835	18.73%	3.392%
8	15.845	2181	2186	2193	rVB	273758	354579	61.58%	11.153%
9	17.098	2393	2399	2405	rVB	80610	109463	19.01%	3.443%
10	19.721	2840	2845	2850	rBV	501900	575782	100.00%	18.110%
11	21.268	3104	3108	3114	rBV2	93231	107090	18.60%	3.368%
12	23.433	3471	3476	3485	rVB2	63062	107055	18.59%	3.367%


Sum of corrected areas: 3179360

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030521\
Data File : BM028993.D
Acq On : 05 Mar 2021 13:12
Operator : CG/JU
Sample : PB134957BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB134957BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

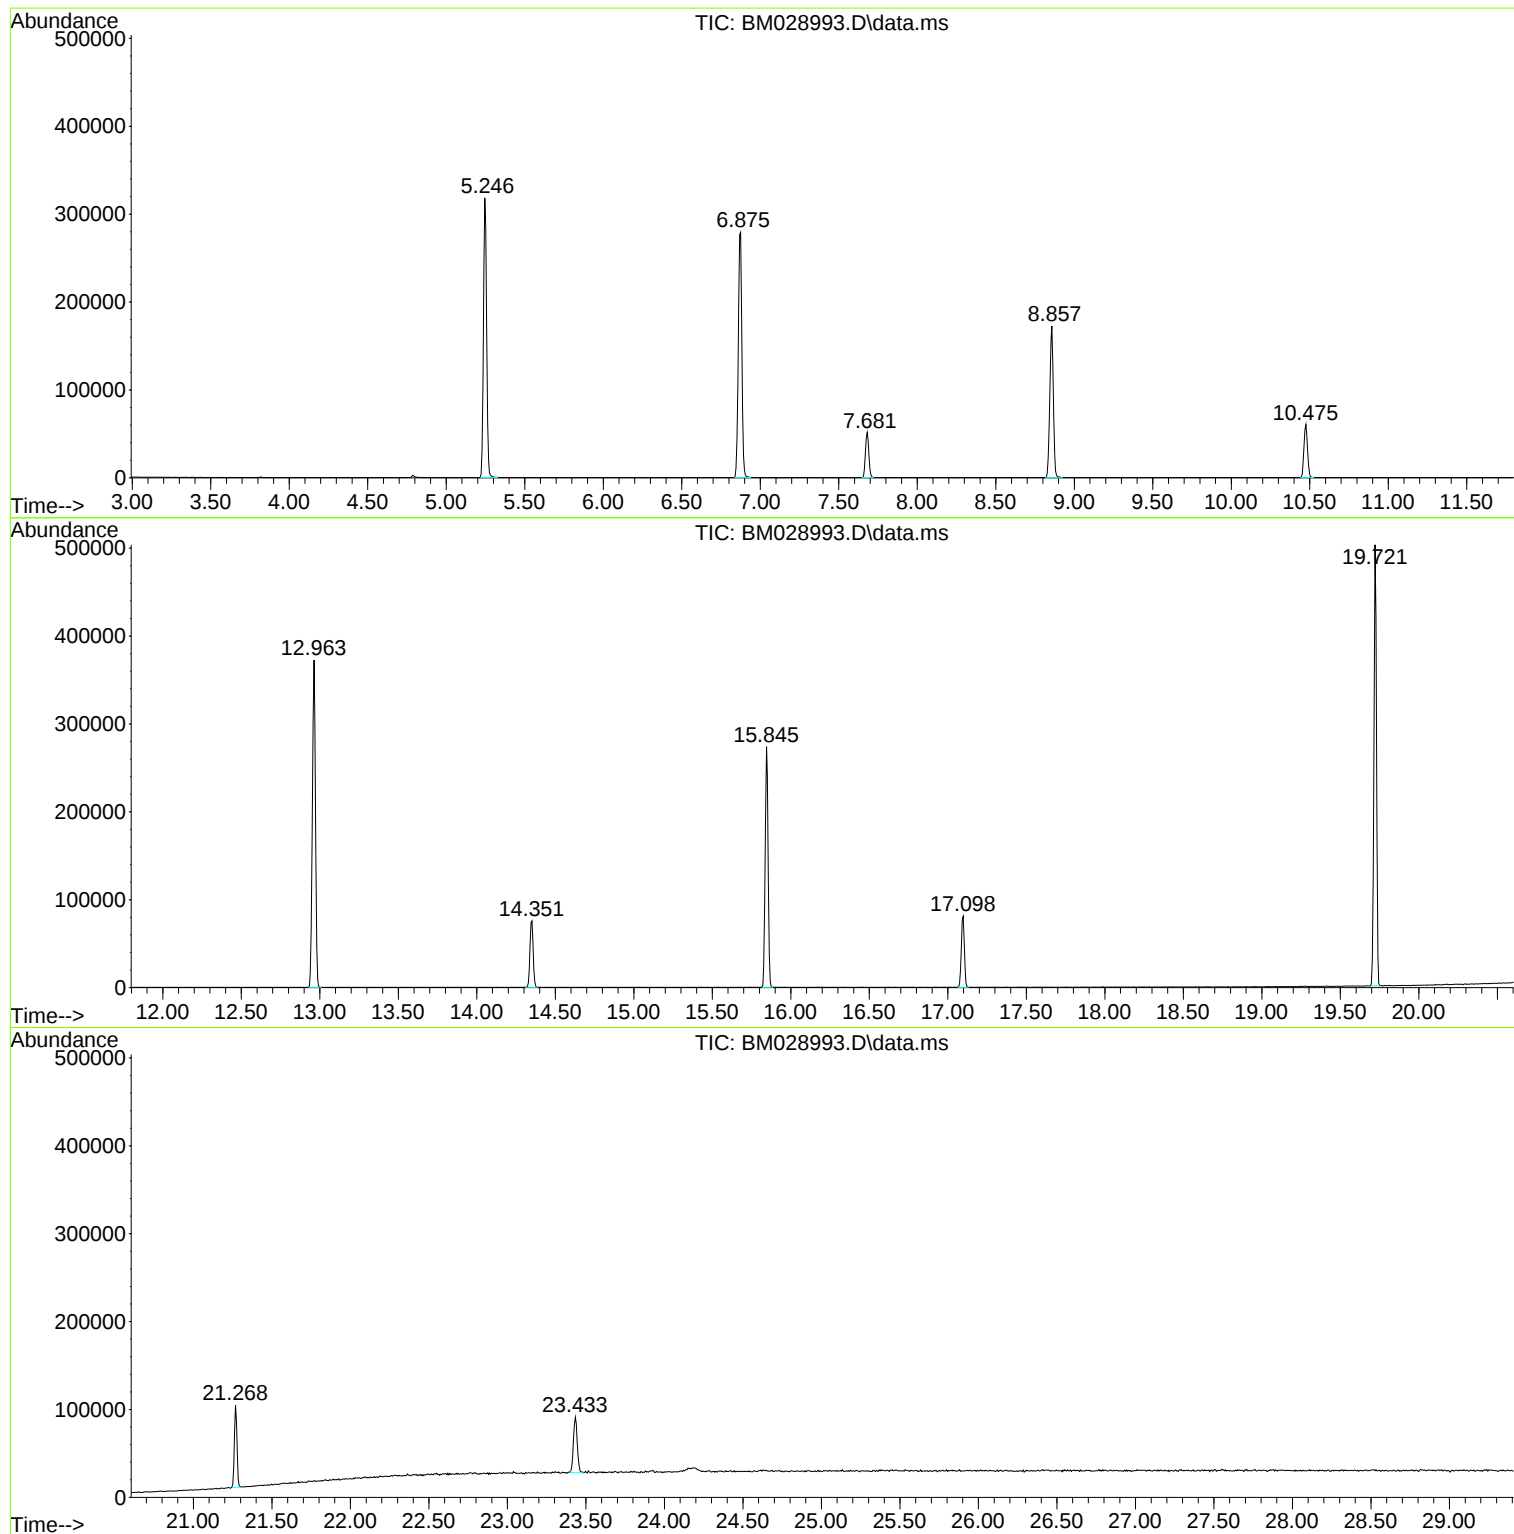

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030521\
Data File : BM028993.D
Acq On : 05 Mar 2021 13:12
Operator : CG/JU
Sample : PB134957BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB134957BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030521\
Data File : BM028993.D
Acq On : 05 Mar 2021 13:12
Operator : CG/JU
Sample : PB134957BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB134957BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------