
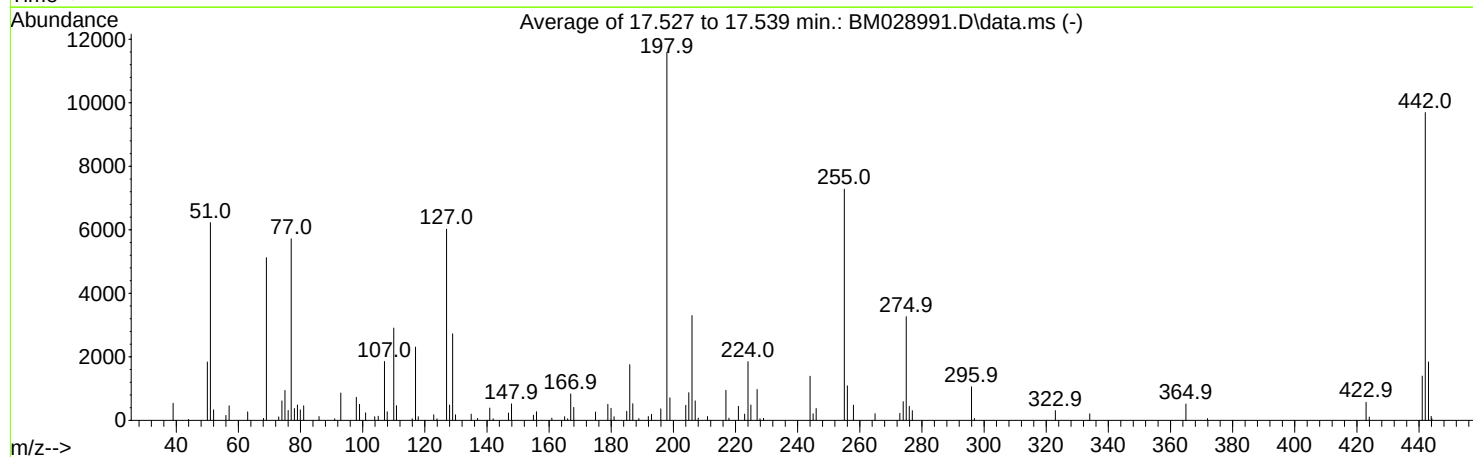


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030521\
 Data File : BM028991.D
 Acq On : 05 Mar 2021 11:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 05 13:17:12 2021

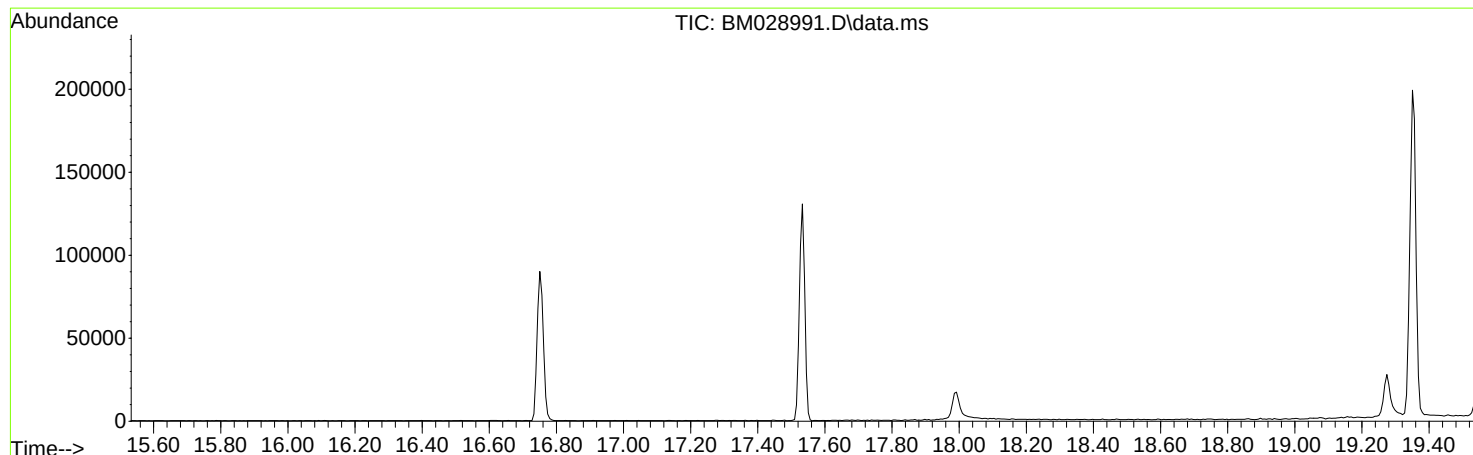

AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.8	6229	PASS
68	69	0.00	2	1.2	60	PASS
69	198	0.00	100	44.2	5124	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.0	6020	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	11583	PASS
199	198	5	9	6.1	711	PASS
275	198	10	60	28.2	3263	PASS
365	198	1	100	4.4	513	PASS
441	198	0.01	100	12.1	1398	PASS
442	442	50	100	100.0	9695	PASS
443	442	15	24	19.0	1840	PASS




	DDT Breakdown	
Date	Instrument Name	DFTPP Data File
3/5/2021	BNA_M	<u>BM028991.D</u>
Compound Name	Response	Retention Time
DDT	46149	20.57
DDD	270	20.13
DDE	0	19.9
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
270	46419	0.58

Instrument :
 BNA_M
ClientSampleId :
 DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030521\
 Data File : BM028991.D
 Acq On : 05 Mar 2021 11:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Mar 06 04:04:09 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 05 13:17:12 2021
 Response via : Initial Calibration

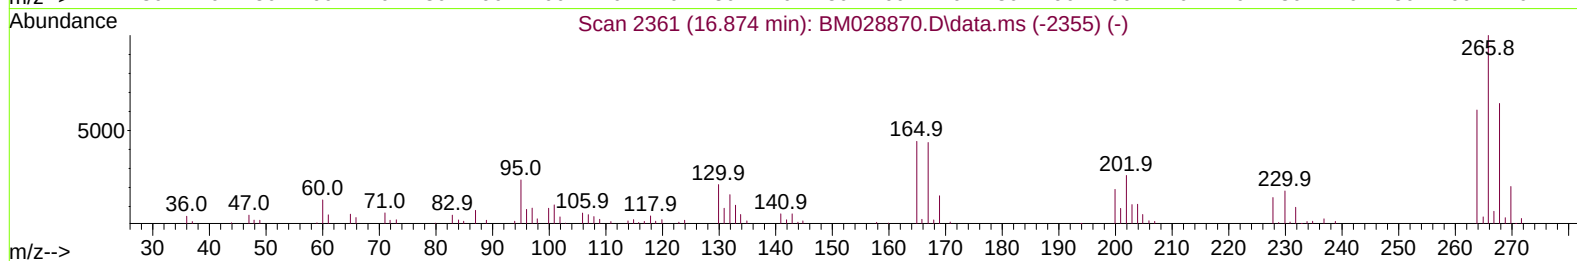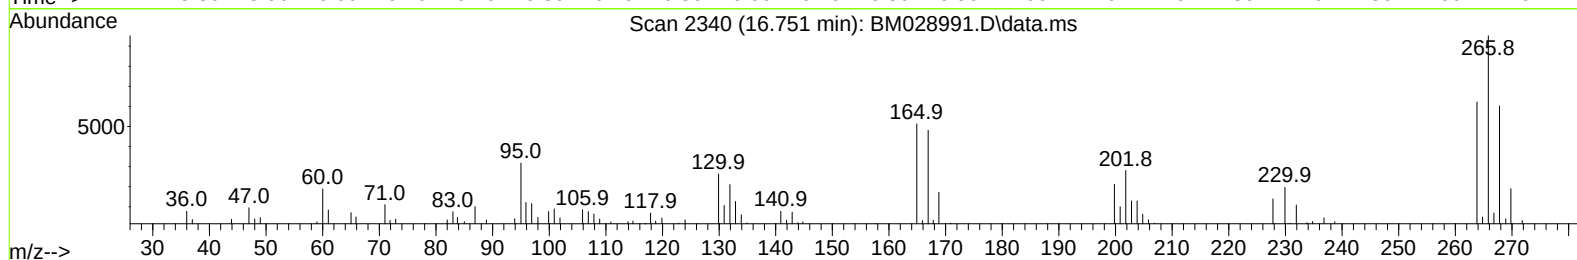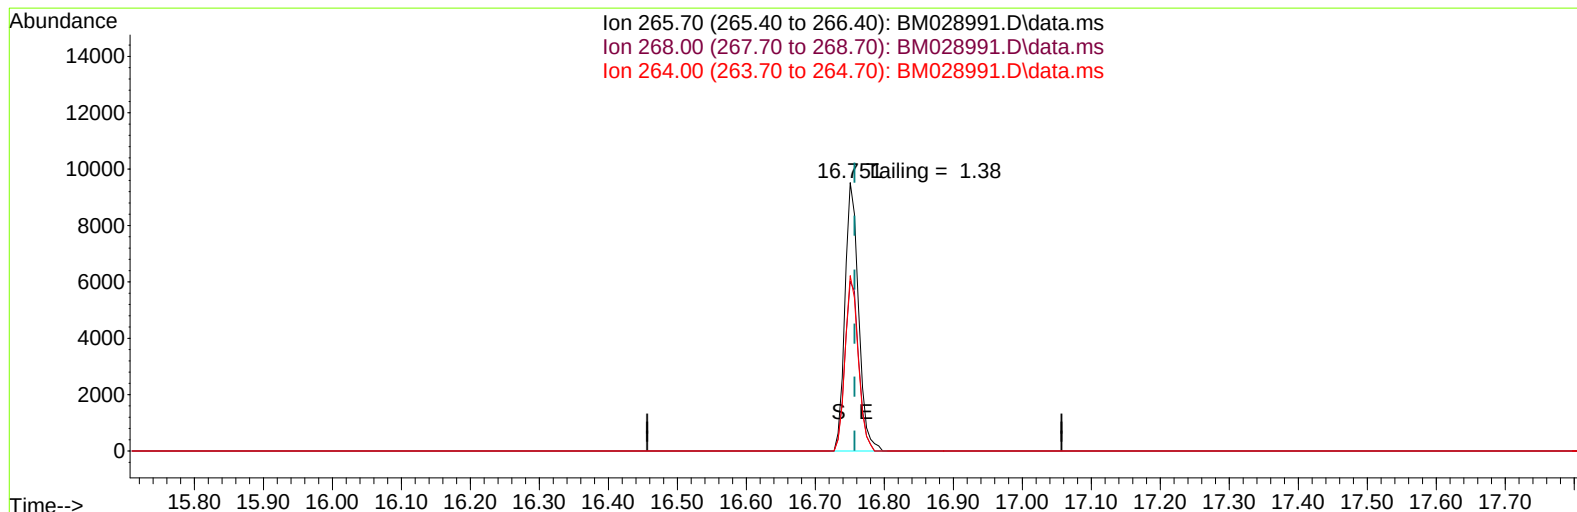

TIC: BM028991.D\data.ms

(70) Pentachlorophenol (C)

16.751min (-0.006) 0.00 ng




response 13046

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	63.22
264.00	63.30	65.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030521\
Data File : BM028991.D
Acq On : 05 Mar 2021 11:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 06 04:04:09 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 05 13:17:12 2021
Response via : Initial Calibration

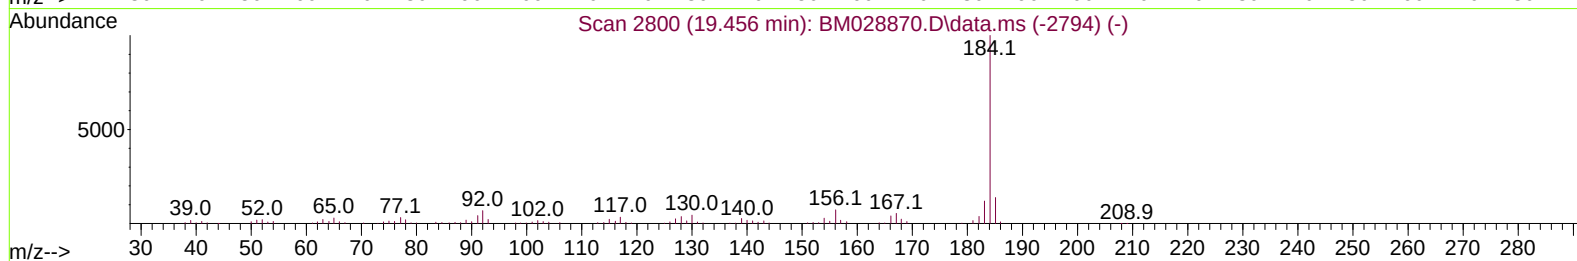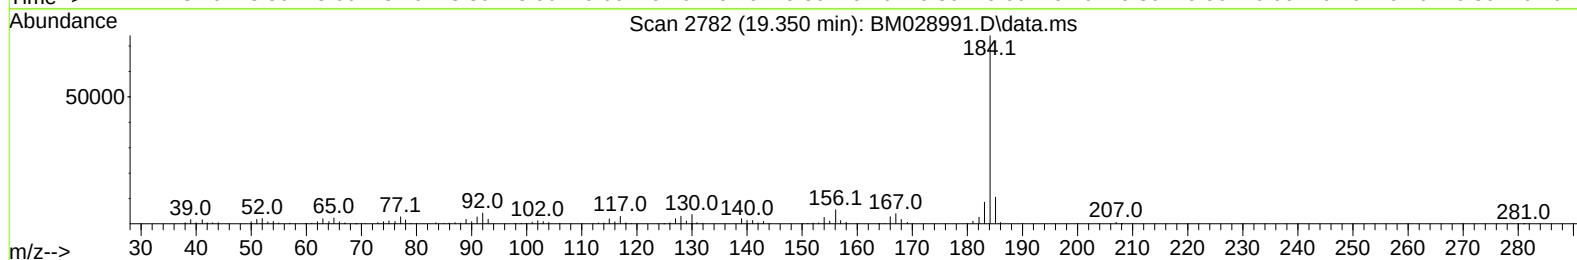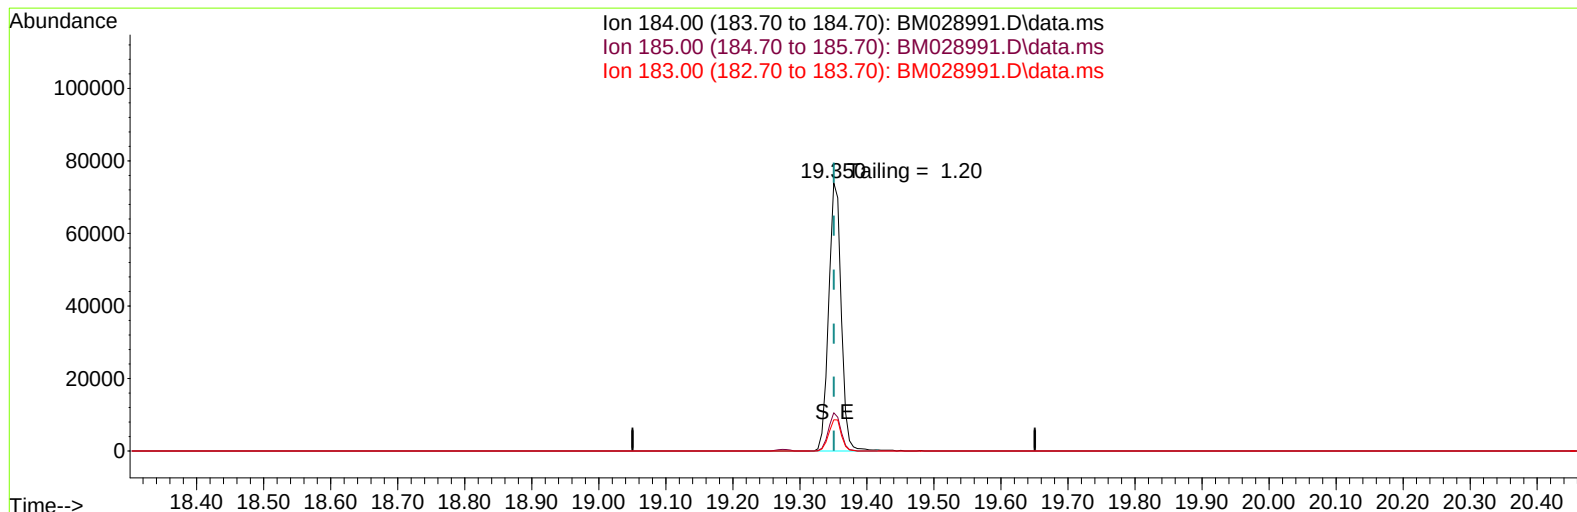

TIC: BM028991.D\data.ms

(77) Benzidine

19.350min (-0.000) 0.00 ng

response 96351

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.29
183.00	12.10	11.65
0.00	0.00	0.00