

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030524\
 Data File : BM044507.D
 Acq On : 05 Mar 2024 18:16
 Operator : MA/JU
 Sample : SP6444
 Misc : SFAM SURROGATE
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SP6444

Quant Time: Mar 05 23:25:38 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 05 23:05:11 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.733	152	203489	20.000	ng/ul	0.00
20) Naphthalene-d8	10.516	136	918739	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.368	164	582213	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.121	188	1215789	20.000	ng/ul	0.00
79) Chrysene-d12	21.303	240	1101155	20.000	ng/ul	0.00
88) Perylene-d12	23.556	264	1272351	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.287	96	96191	16.033	ng/uL	0.00
4) Pyridine-d5	3.681	84	1414179	80.083	ng/ul	0.00
7) Phenol-d5	6.904	99	1535303	73.386	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.081	67	982109	75.999	ng/ul	0.00
11) 2-Chlorophenol-d4	7.269	132	1221549	79.455	ng/ul	0.00
15) 4-Methylphenol-d8	8.433	113	1233187	75.056	ng/ul	0.00
21) Nitrobenzene-d5	8.892	128	653680	84.494	ng/ul	0.00
24) 2-Nitrophenol-d4	9.604	143	734576	88.078	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.133	165	1107276	78.010	ng/ul	0.00
31) 4-Chloroaniline-d4	10.663	131	1870094	79.329	ng/ul	0.00
46) Dimethylphthalate-d6	13.792	166	3575671	78.292	ng/ul	0.00
49) Acenaphthylene-d8	14.062	160	4189114	80.202	ng/ul	0.00
54) 4-Nitrophenol-d4	14.580	143	740512	78.185	ng/ul	0.00
60) Fluorene-d10	15.368	176	3000505	78.180	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.492	200	637919	80.831	ng/ul	0.00
73) Anthracene-d10	17.221	188	4597772	79.117	ng/ul	0.00
81) Pyrene-d10	19.515	212	5135627	76.041	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.421	264	5204792	77.827	ng/ul	0.00
Target Compounds						
48) 2,6-Dinitrotoluene	13.798	165	19980	2.152	ng/ul#	Qvalue 36


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030524\
Data File : BM044507.D
Acq On : 05 Mar 2024 18:16
Operator : MA/JU
Sample : SP6444
Misc : SFAM SURROGATE
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SP6444

Quant Time: Mar 05 23:25:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 05 23:05:11 2024
Response via : Initial Calibration

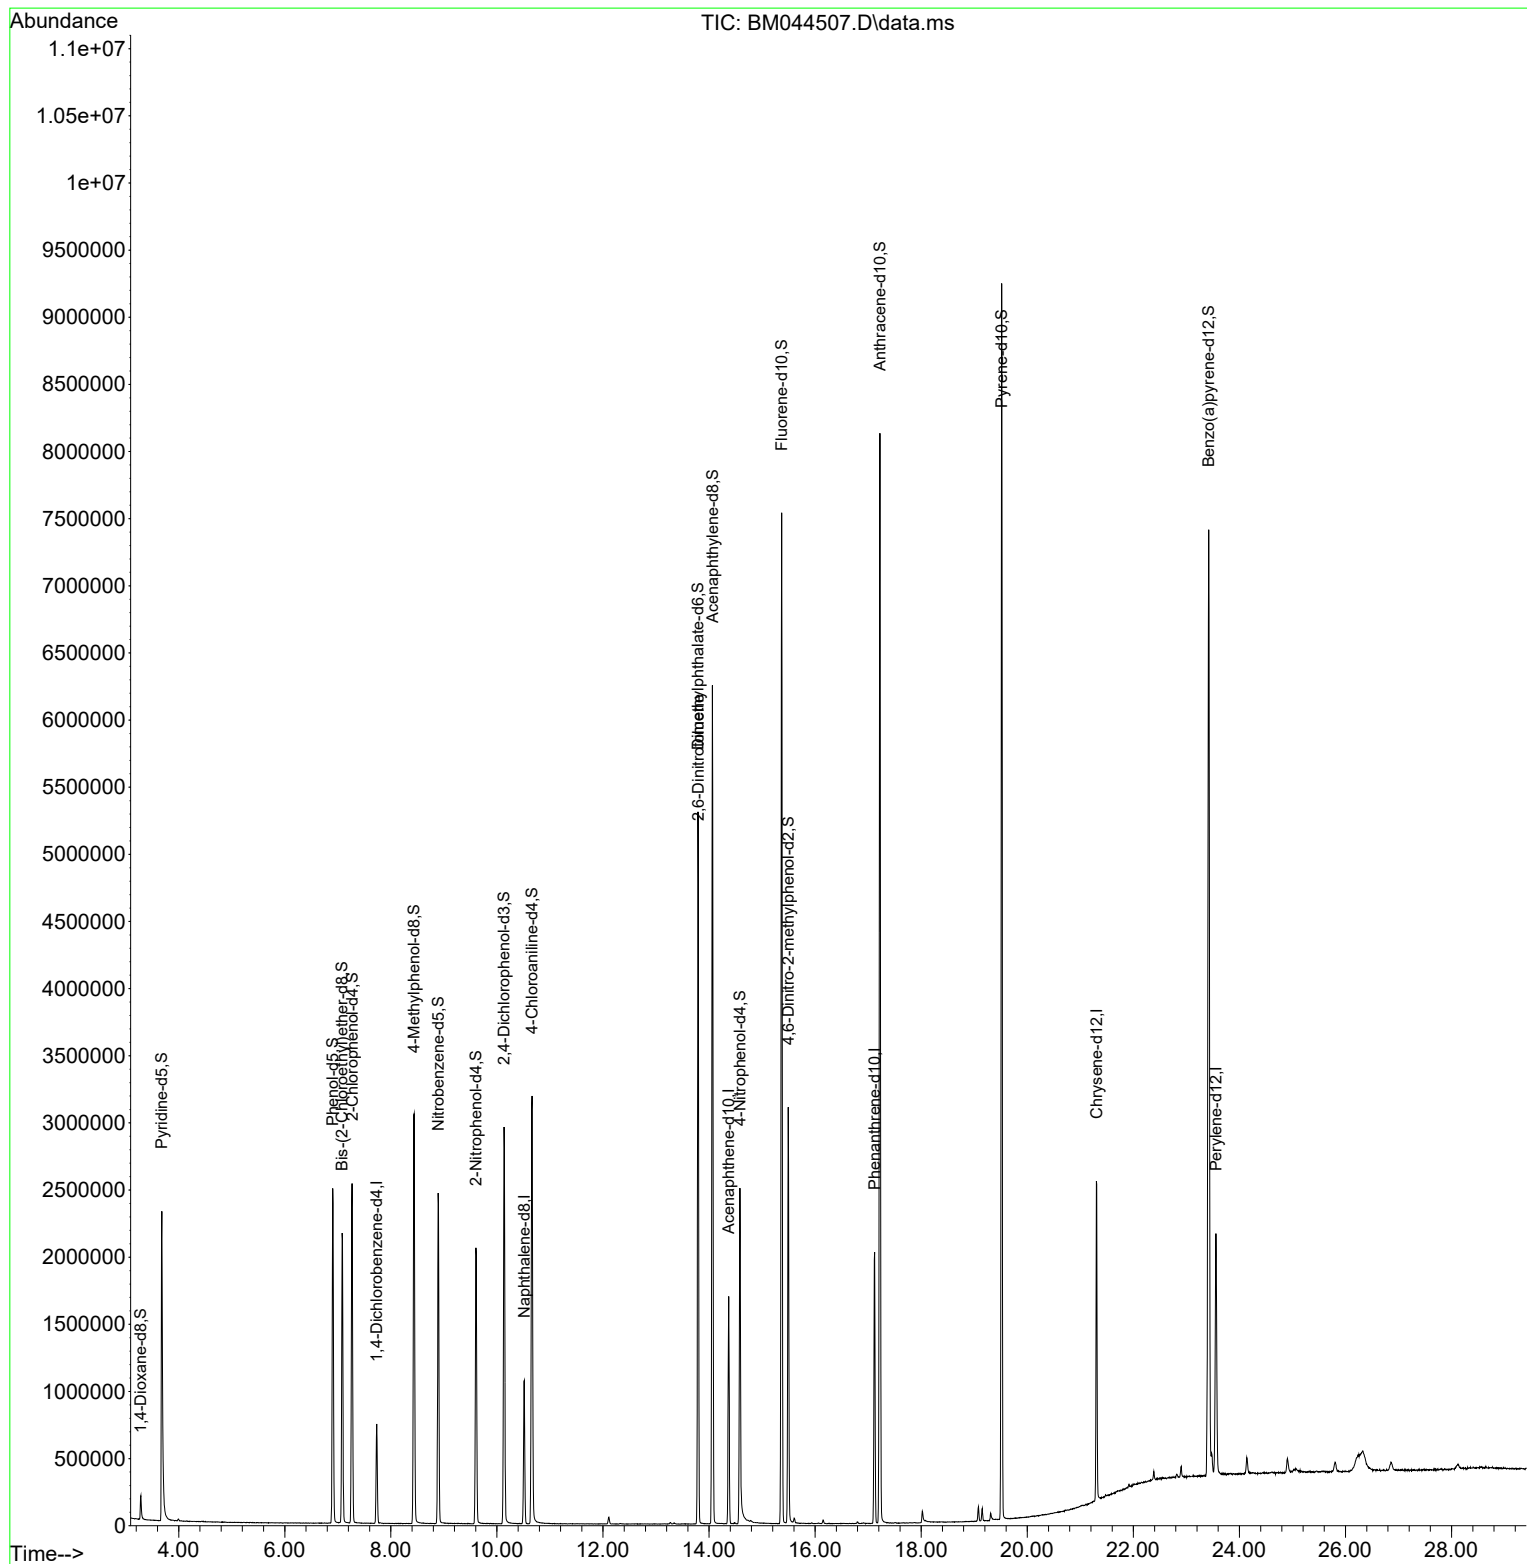

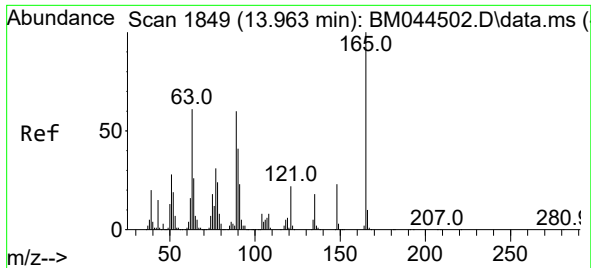

#48
 2,6-Dinitrotoluene
 Concen: 2.152 ng/ul
 RT: 13.798 min Scan# 1849
 Delta R.T. -0.165 min
 Lab File: BM044507.D
 Acq: 05 Mar 2024 18:16

Instrument :
 BNA_M
 ClientSampleId :
 SP6444

Tgt Ion:165 Resp: 19980
 Ion Ratio Lower Upper
 165 100
 89 1.9 48.4 72.6#
 121 34.8 17.7 26.5#

