

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030617\
 Data File : BM009085.D
 Acq On : 06 Mar 2017 18:15
 Operator : SJ/MA
 Sample : I2064-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AE8

Quant Time: Mar 07 03:40:05 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 07 03:37:41 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	147	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	459	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	282	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.36	188	53469	0.40	ng/ul	0.09
16) Chrysene-d12	21.45	240	654	0.40	ng/ul	0.00
20) Perylene-d12	23.64	264	51798	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	229	0.30	ng/ul	0.00
14) Fluoranthene-d10	19.30	212	595	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.67	202	139	0.06	ng/ul#	Qvalue 1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030617\
Data File : BM009085.D
Acq On : 06 Mar 2017 18:15
Operator : SJ/MA
Sample : I2064-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE8

Quant Time: Mar 07 03:40:05 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 03:37:41 2017
Response via : Initial Calibration

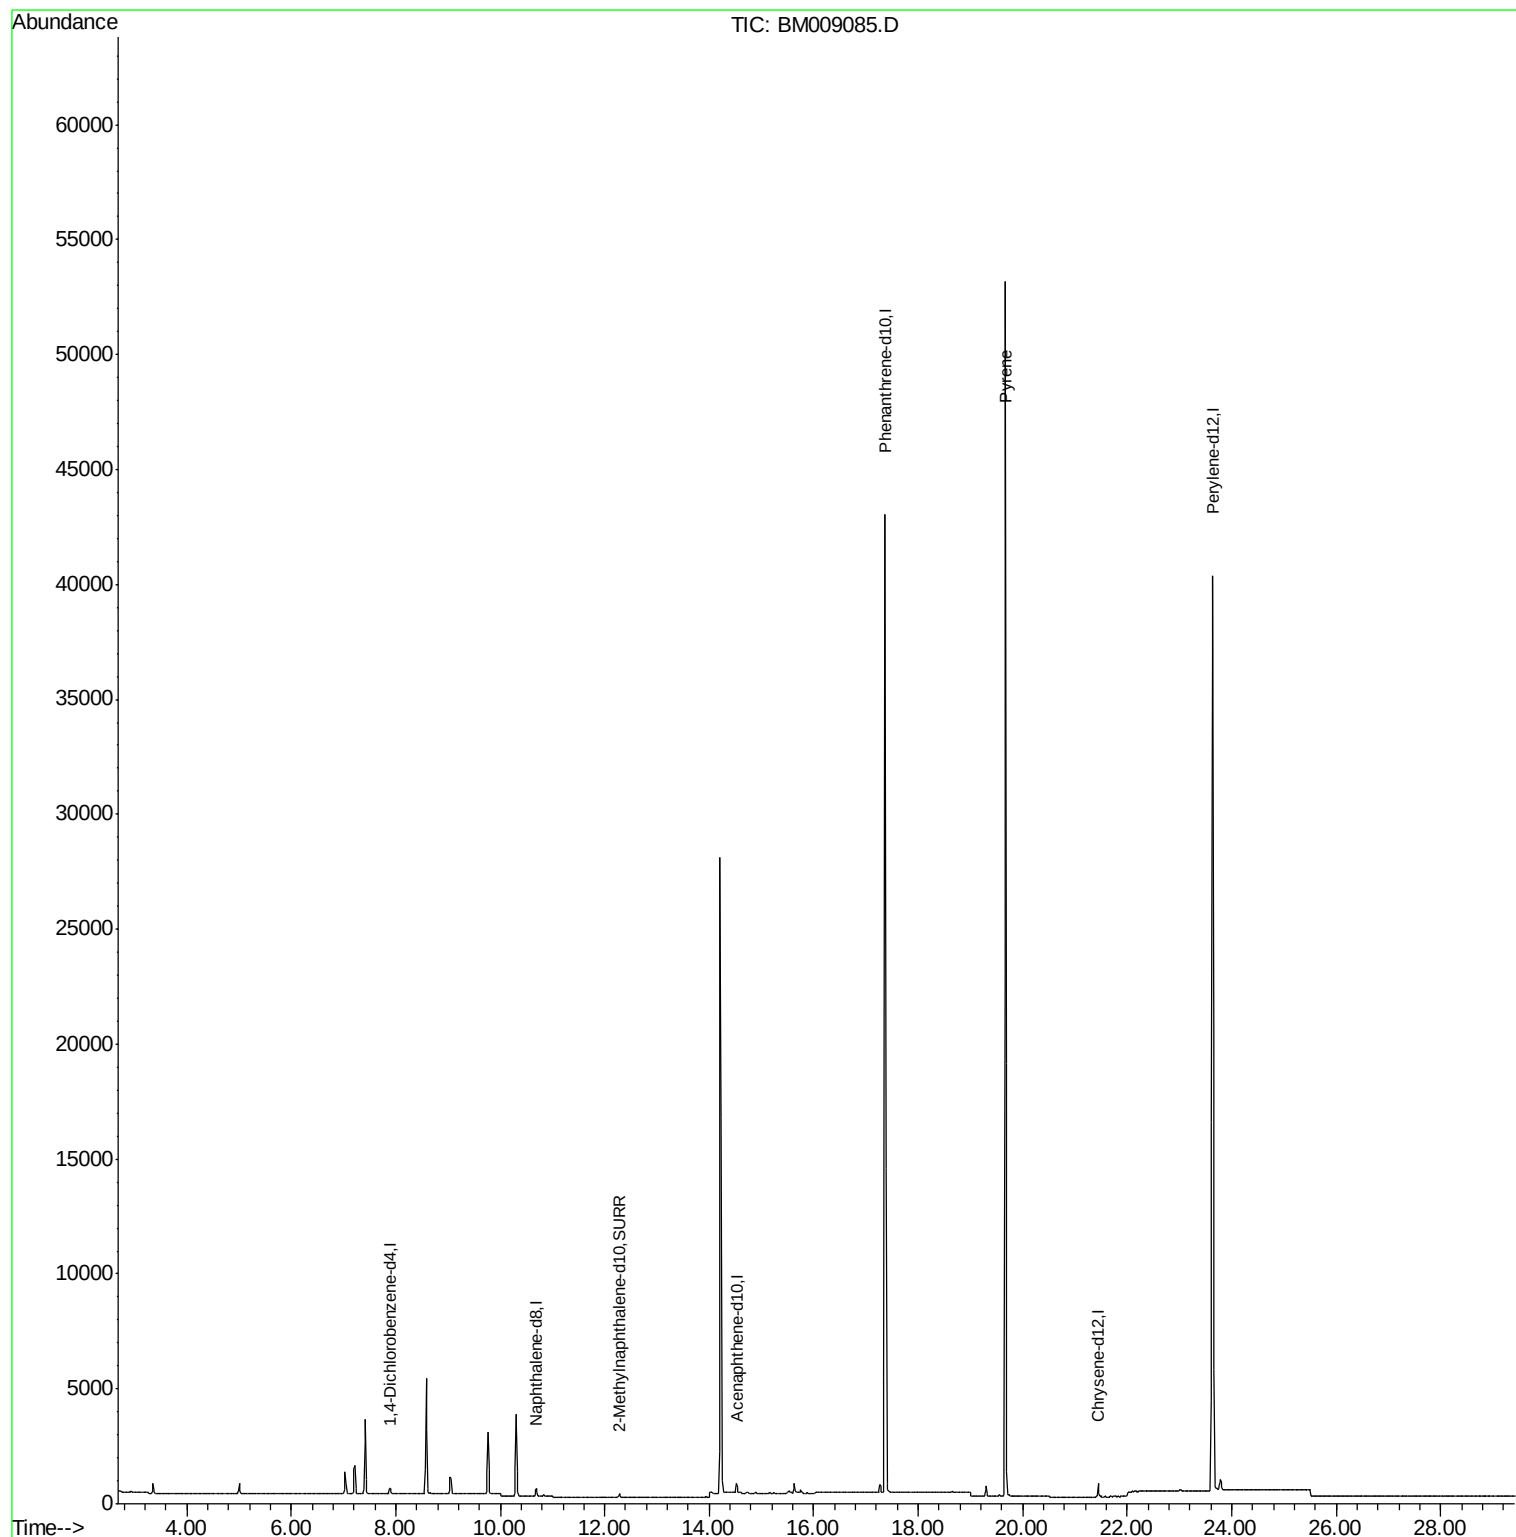

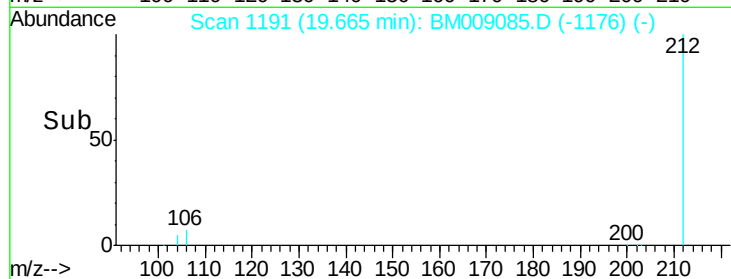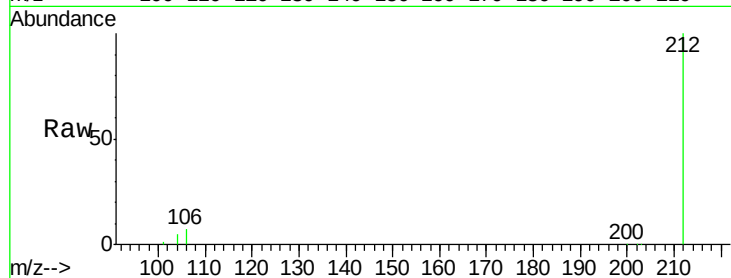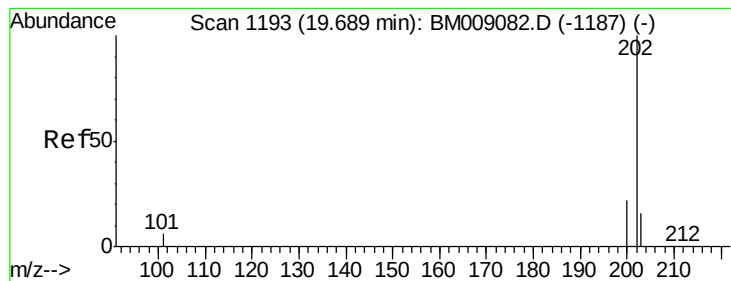

#17

Pyrene

Concen: 0.06 ng/ul

RT: 19.67 min Scan# 1191

Delta R.T. -0.02 min

Lab File: BM009085.D

Acq: 06 Mar 2017 18:15

Instrument :

BNA_M

ClientSampleId :

C0AE8

Tgt Ion: 202 Resp: 139

Ion Ratio Lower Upper

202 100

200 36.6 18.2 27.4#

203 150.7 15.6 23.4#

