

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030617\
 Data File : BM009086.D
 Acq On : 06 Mar 2017 18:51
 Operator : SJ/MA
 Sample : I2064-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AE9

Quant Time: Mar 07 03:40:10 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 07 03:37:41 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	153	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	454	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	287	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.36	188	53956	0.40	ng/ul	0.09
16) Chrysene-d12	21.45	240	642	0.40	ng/ul	0.00
20) Perylene-d12	23.64	264	50672	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	235	0.31	ng/ul	0.00
14) Fluoranthene-d10	19.30	212	579	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.53	166	125	0.09	ng/ul#	42
17) Pyrene	19.66	202	123	0.06	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030617\
Data File : BM009086.D
Acq On : 06 Mar 2017 18:51
Operator : SJ/MA
Sample : I2064-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE9

Quant Time: Mar 07 03:40:10 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 03:37:41 2017
Response via : Initial Calibration

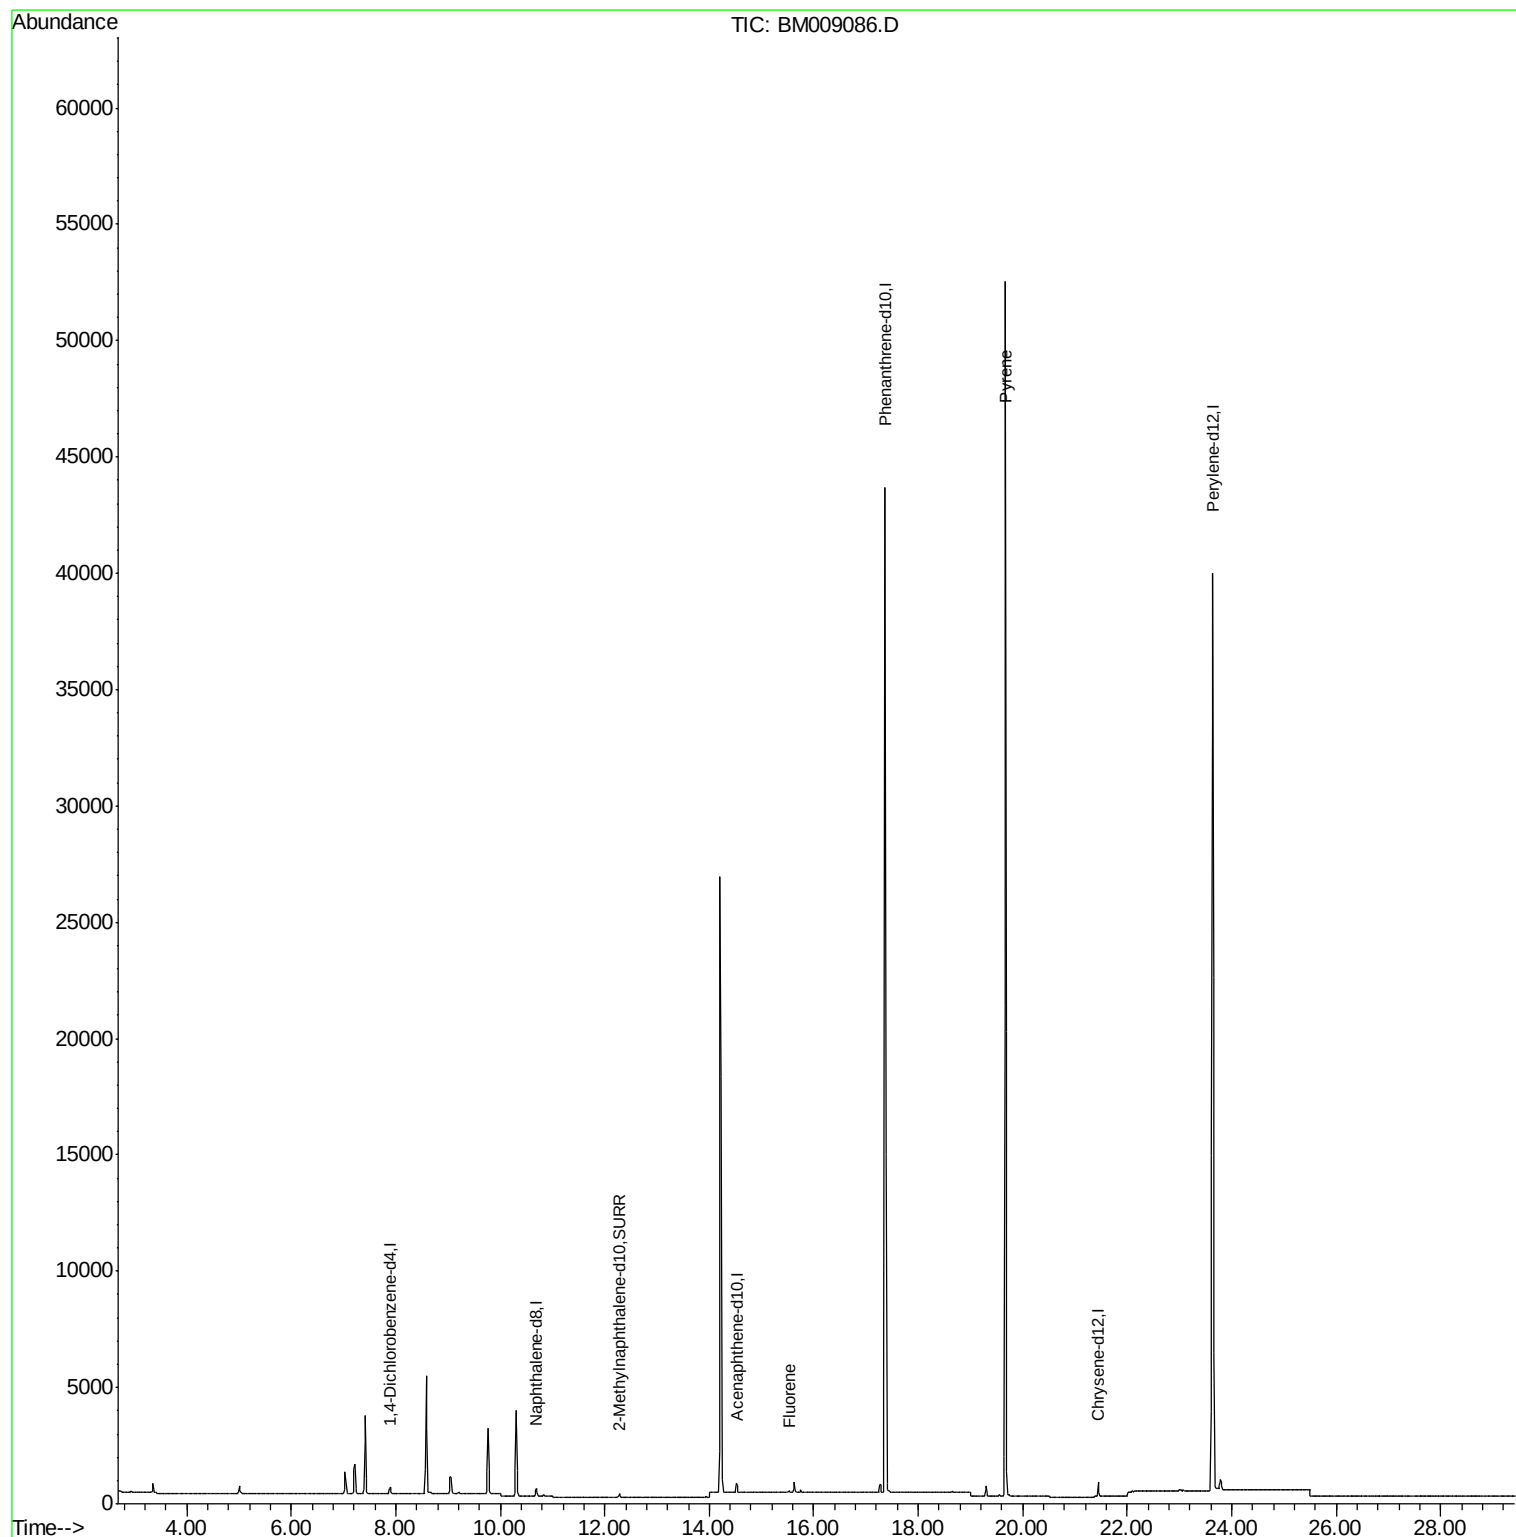


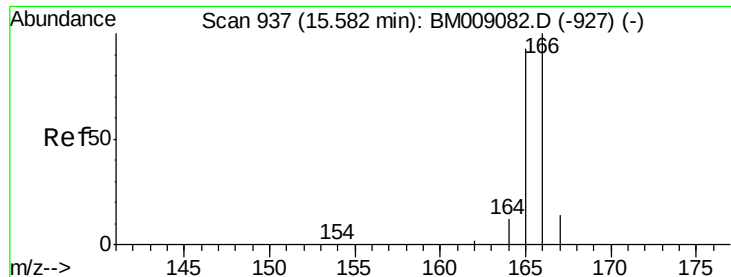


#9
Fluorene
 Concen: 0.09 ng/ul
 RT: 15.53 min Scan# 934
 Delta R.T. -0.05 min
 Lab File: BM009086.D
 Acq: 06 Mar 2017 18:51

Instrument :
 BNA_M
 ClientSampleId :
 C0AE9



Tgt Ion:166 Resp: 125
 Ion Ratio Lower Upper
 166 100
 165 47.2 73.4 110.2#
 167 68.9 14.6 22.0#

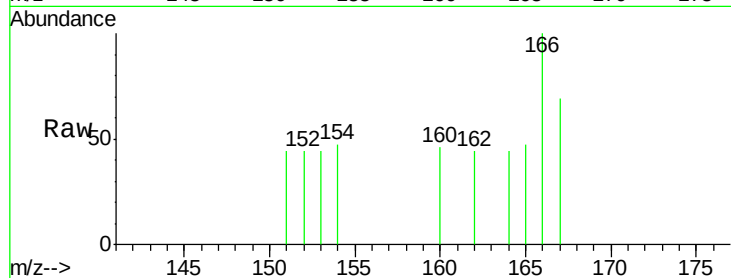

Abundance Ion 166.00 (165.70 to 166.70): E
 Ion 165.00 (164.70 to 165.70): E
 Ion 167.00 (166.70 to 167.70): E

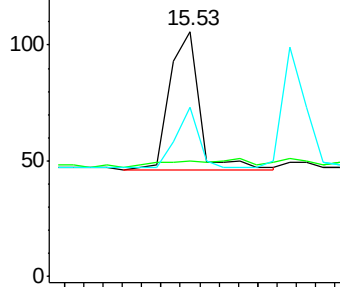


Time--> 15.40 15.50 15.60

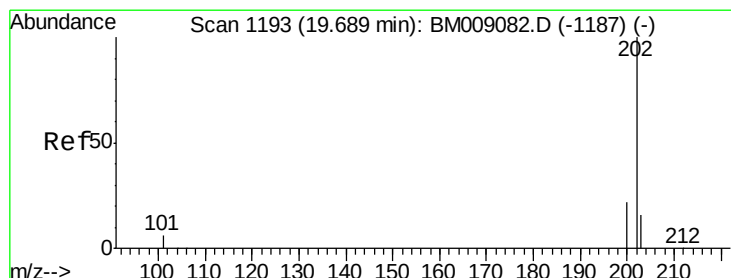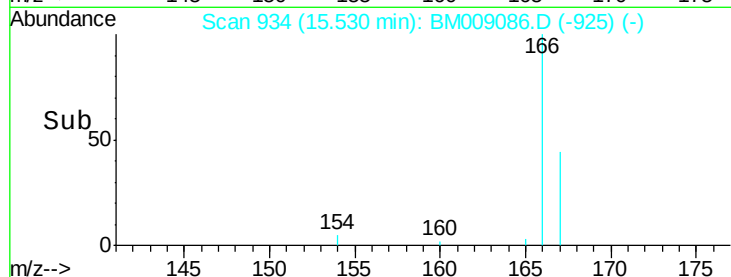


#17
Pyrene
 Concen: 0.06 ng/ul
 RT: 19.66 min Scan# 1191
 Delta R.T. -0.02 min
 Lab File: BM009086.D
 Acq: 06 Mar 2017 18:51

Tgt Ion:202 Resp: 123
 Ion Ratio Lower Upper
 202 100
 200 36.3 18.2 27.4#
 203 145.2 15.6 23.4#

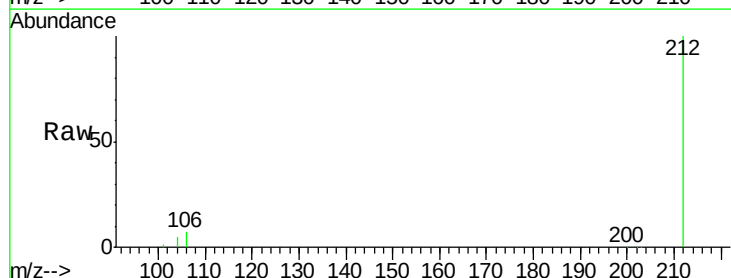

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 200.00 (199.70 to 200.70): E
 Ion 203.00 (202.70 to 203.70): E

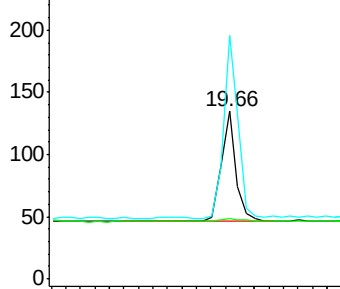

Time--> 19.50 19.60 19.70

