

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030617\
 Data File : BM009088.D
 Acq On : 06 Mar 2017 20:03
 Operator : SJ/MA
 Sample : I2064-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AE1

Quant Time: Mar 07 03:40:20 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 07 03:37:41 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	141	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	424	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	253	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.36	188	52055	0.40	ng/ul	0.09
16) Chrysene-d12	21.44	240	606	0.40	ng/ul	0.00
20) Perylene-d12	23.63	264	52035	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	223	0.32	ng/ul	0.00
14) Fluoranthene-d10	19.29	212	578	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.53	166	111	0.09	ng/ul#	44
17) Pyrene	19.66	202	118	0.06	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030617\
Data File : BM009088.D
Acq On : 06 Mar 2017 20:03
Operator : SJ/MA
Sample : I2064-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE1

Quant Time: Mar 07 03:40:20 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 03:37:41 2017
Response via : Initial Calibration




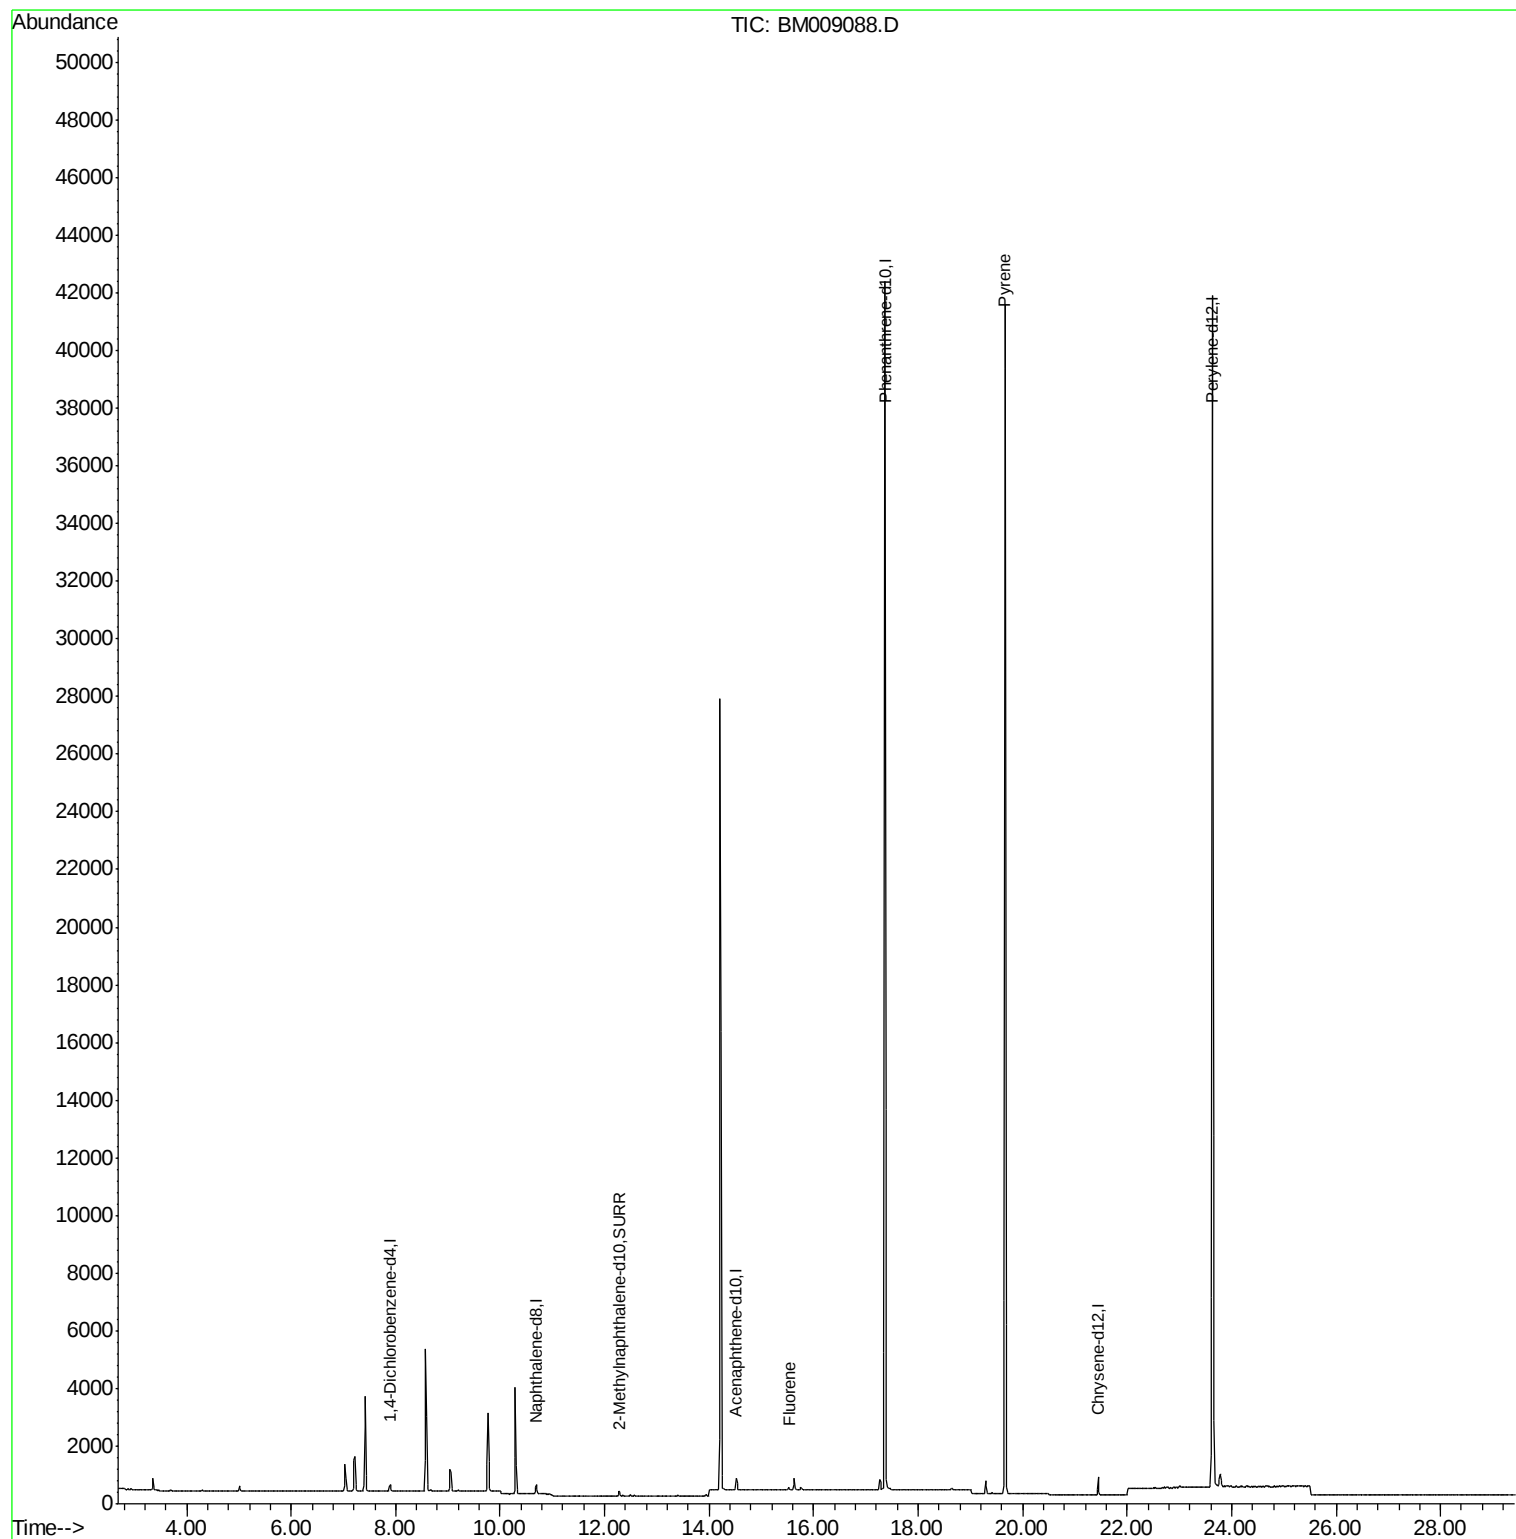


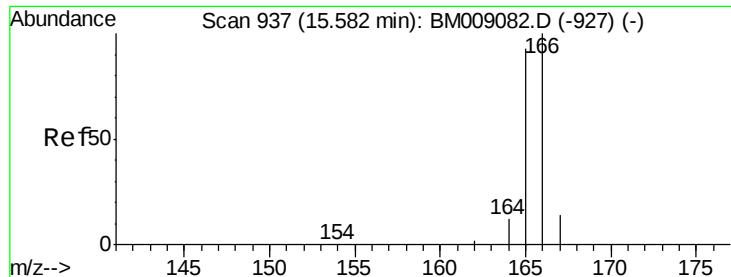

#9
Fluorene
 Concen: 0.09 ng/ul
 RT: 15.53 min Scan# 934
 Delta R.T. -0.05 min
 Lab File: BM009088.D
 Acq: 06 Mar 2017 20:03

Instrument :
 BNA_M
 ClientSampleId :
 C0AE1

Tgt Ion:166 Resp: 111
 Ion Ratio Lower Upper
 166 100
 165 51.0 73.4 110.2#
 167 71.4 14.6 22.0#

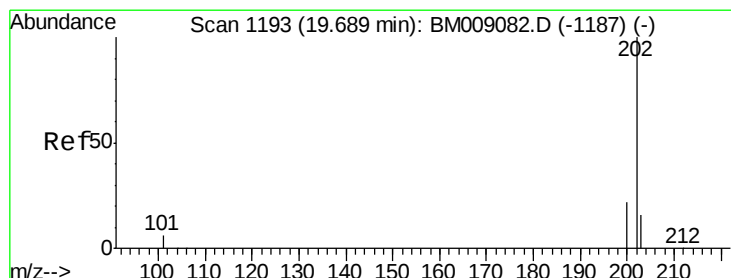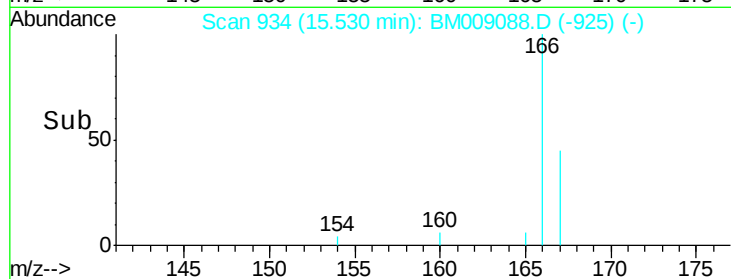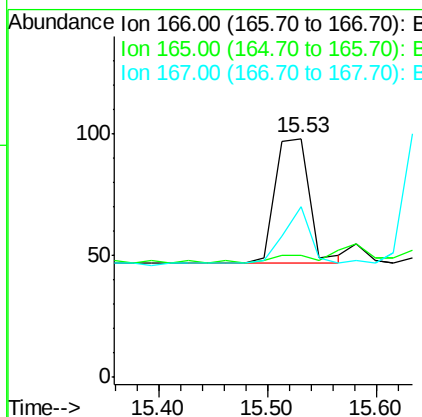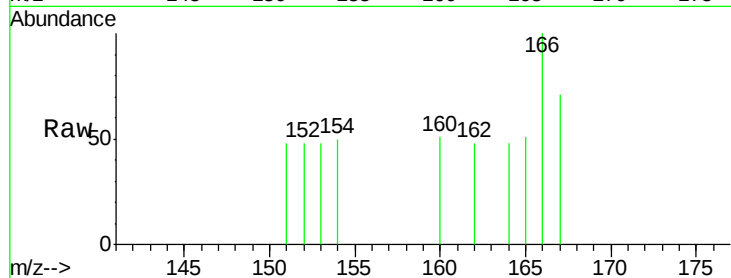

#17
Pyrene
 Concen: 0.06 ng/ul
 RT: 19.66 min Scan# 1190
 Delta R.T. -0.03 min
 Lab File: BM009088.D
 Acq: 06 Mar 2017 20:03

Tgt Ion:202 Resp: 118
 Ion Ratio Lower Upper
 202 100
 200 41.9 18.2 27.4#
 203 117.1 15.6 23.4#

