

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030617\
 Data File : BM009089.D
 Acq On : 06 Mar 2017 20:40
 Operator : SJ/MA
 Sample : I2064-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AE0

Quant Time: Mar 07 03:40:24 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 07 03:37:41 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	145	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	467	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	304	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.36	188	51950	0.40	ng/ul	0.09
16) Chrysene-d12	21.45	240	653	0.40	ng/ul	0.00
20) Perylene-d12	23.64	264	48147	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	220	0.28	ng/ul	0.00
14) Fluoranthene-d10	19.30	212	579	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.66	202	139	0.06	ng/ul#	Qvalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030617\
Data File : BM009089.D
Acq On : 06 Mar 2017 20:40
Operator : SJ/MA
Sample : I2064-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE0

Quant Time: Mar 07 03:40:24 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 03:37:41 2017
Response via : Initial Calibration

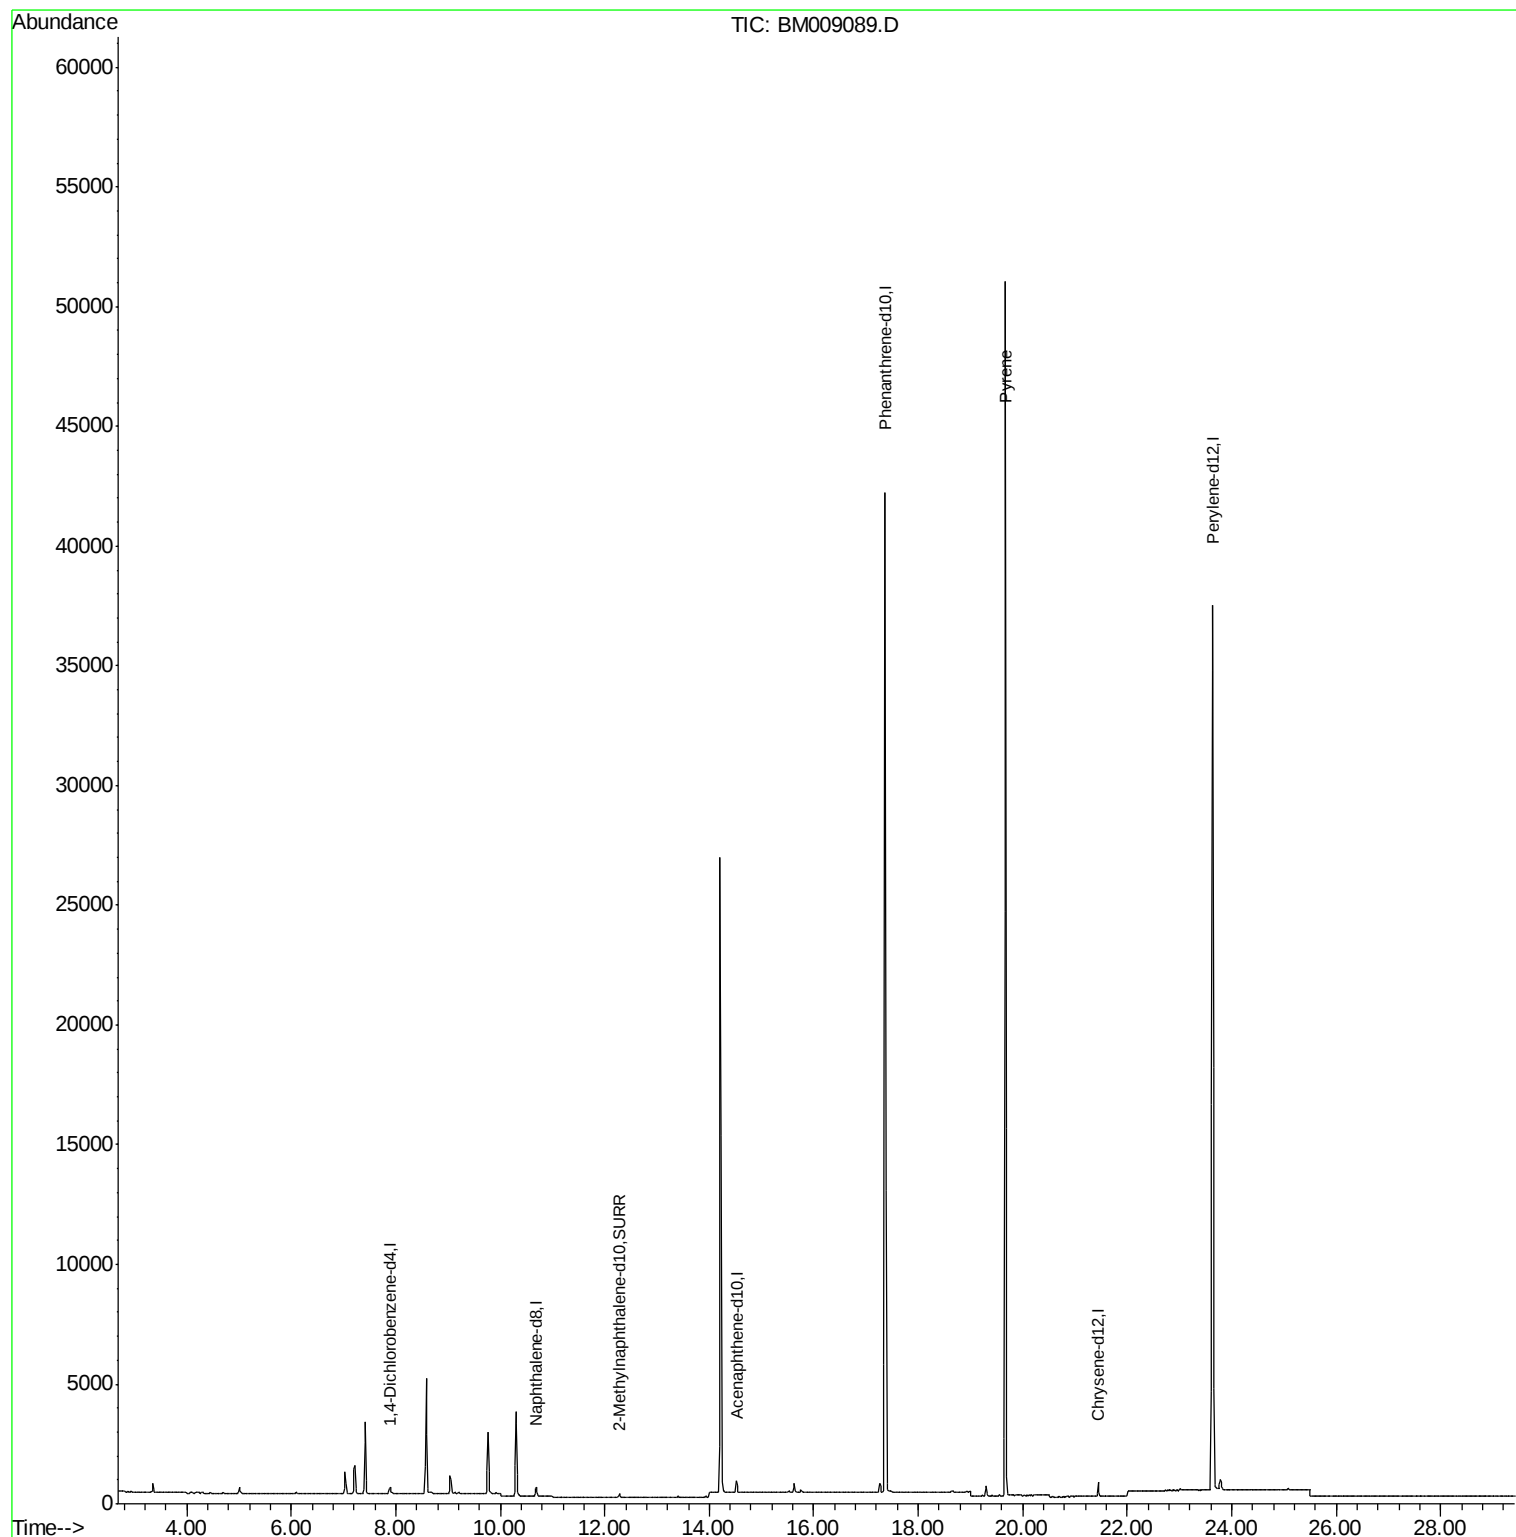

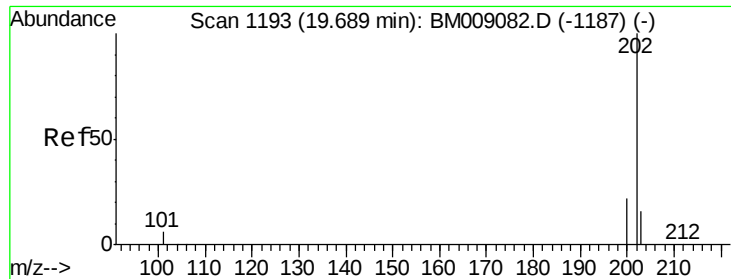

#17
 Pyrene
 Concen: 0.06 ng/ul
 RT: 19.66 min Scan# 1191
 Delta R.T. -0.02 min
 Lab File: BM009089.D
 Acq: 06 Mar 2017 20:40

Instrument :
 BNA_M
 ClientSampleId :
 C0AE0

Tgt Ion: 202 Resp: 139
 Ion Ratio Lower Upper
 202 100
 200 37.7 18.2 27.4#
 203 154.6 15.6 23.4#

