
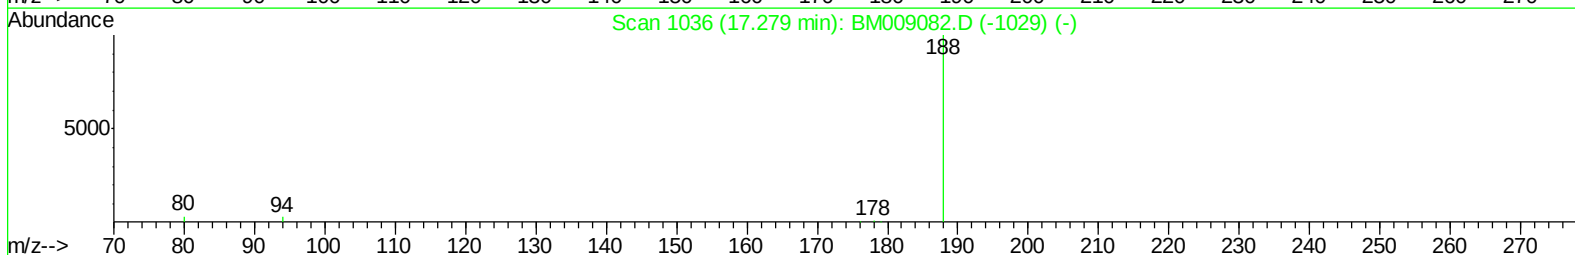
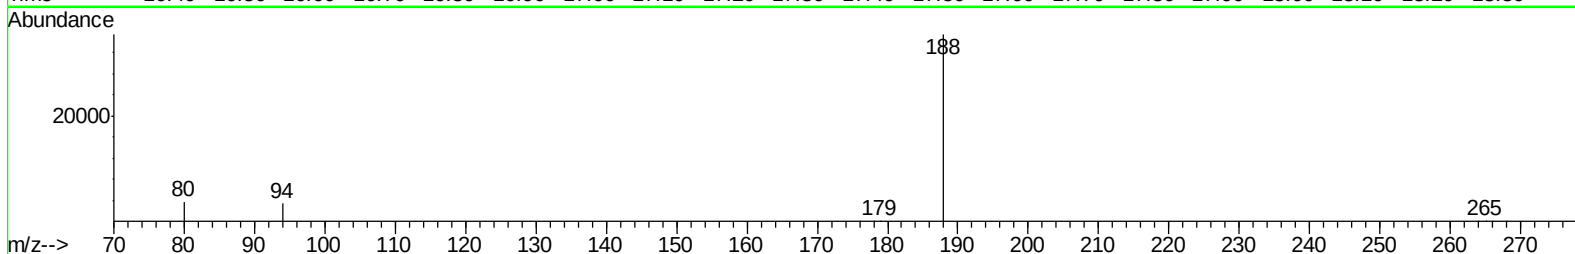


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030617\
Data File : BM009085.D
Acq On : 06 Mar 2017 18:15
Operator : SJ/MA
Sample : I2064-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 07 03:40:05 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 03:37:41 2017
Response via : Initial Calibration

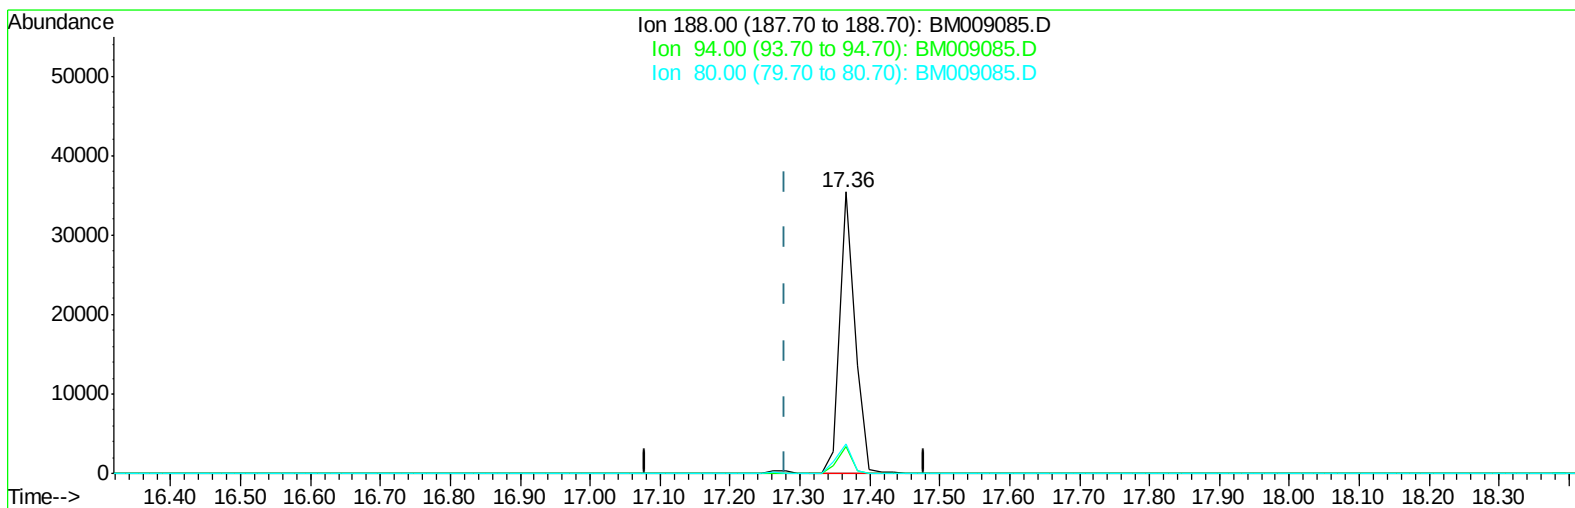

TIC: BM009085.D

(10) Phenanthrene-d10 (I)




17.365min (+0.086) 0.40ng/ul

response 53469

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	9.70
80.00	11.80	10.65
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030617\
Data File : BM009085.D
Acq On : 06 Mar 2017 18:15
Operator : SJ/MA
Sample : I2064-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 07 03:40:05 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 03:37:41 2017
Response via : Initial Calibration

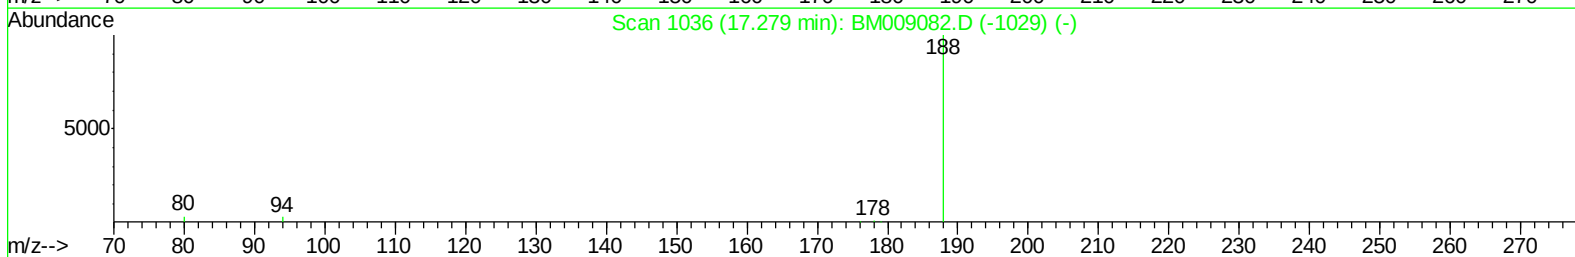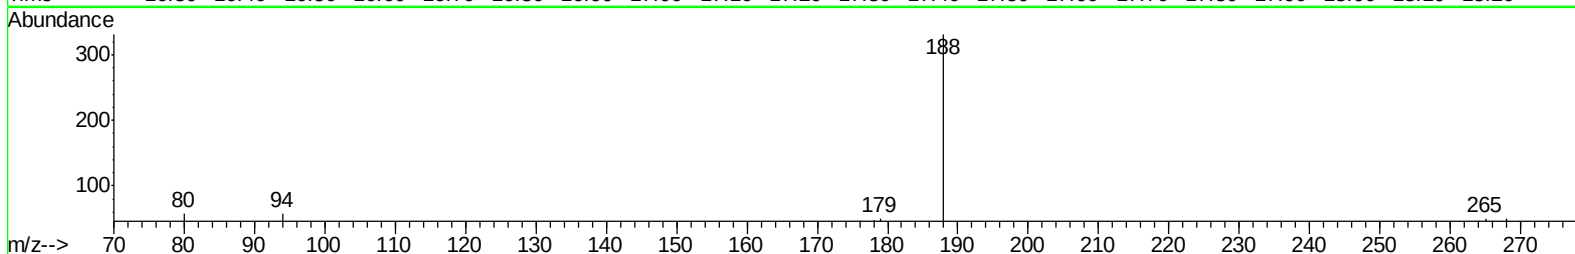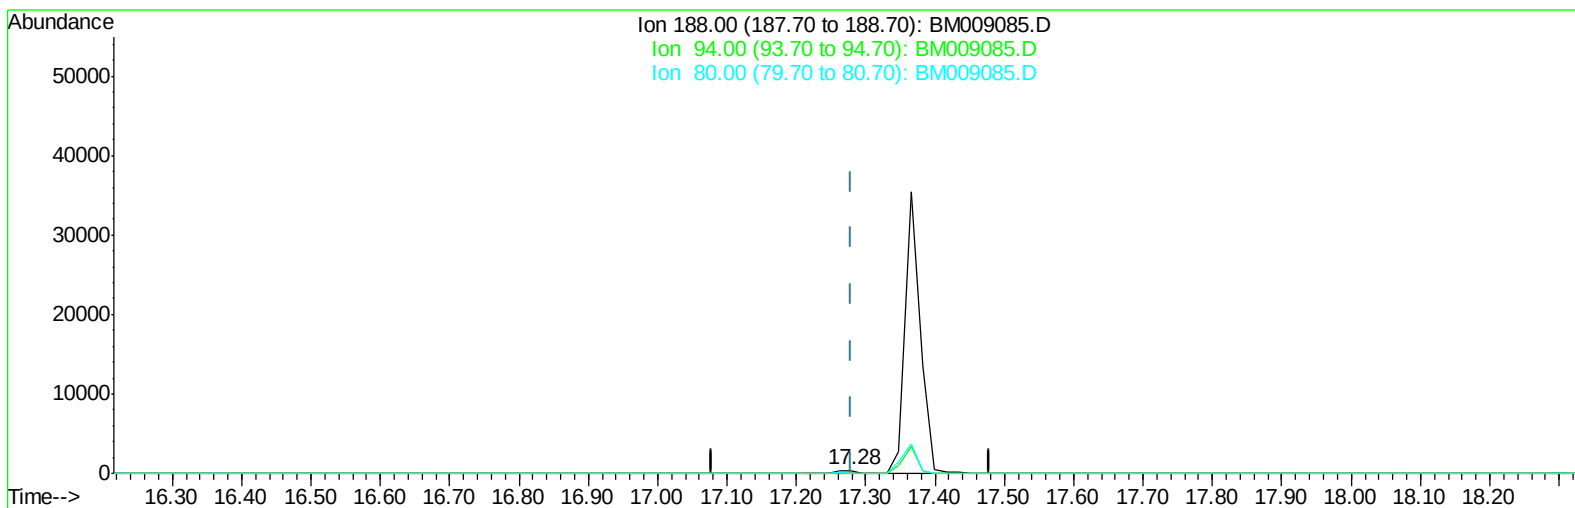

TIC: BM009085.D

(10) Phenanthrene-d10 (I)




17.279min (+0.000) 0.40ng/ul m

response 686

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	17.52#
80.00	11.80	17.52#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030617\
Data File : BM009085.D
Acq On : 06 Mar 2017 18:15
Operator : SJ/MA
Sample : I2064-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 07 03:40:05 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 03:37:41 2017
Response via : Initial Calibration

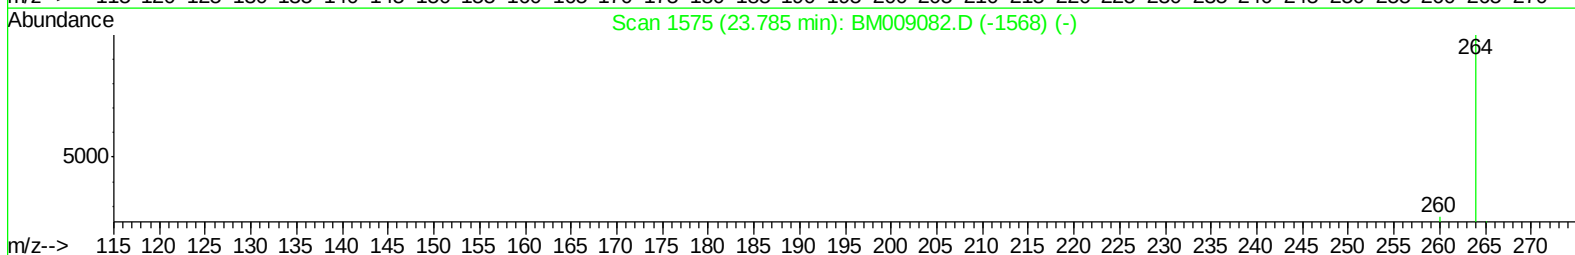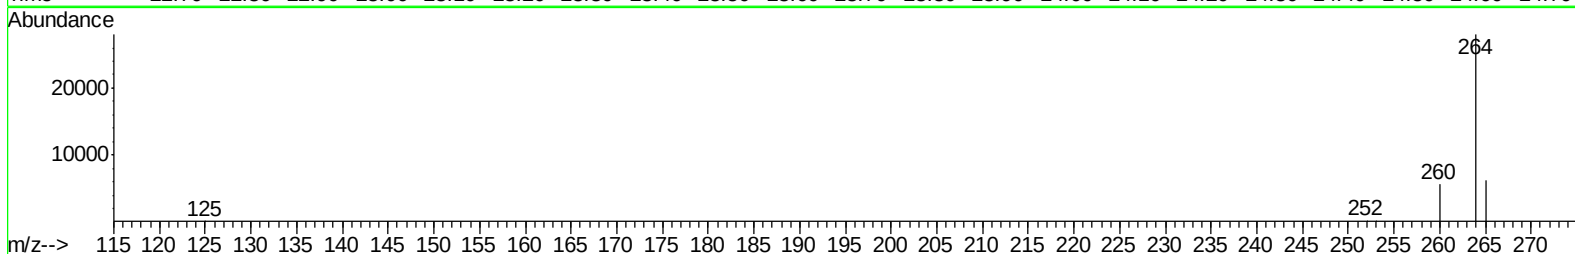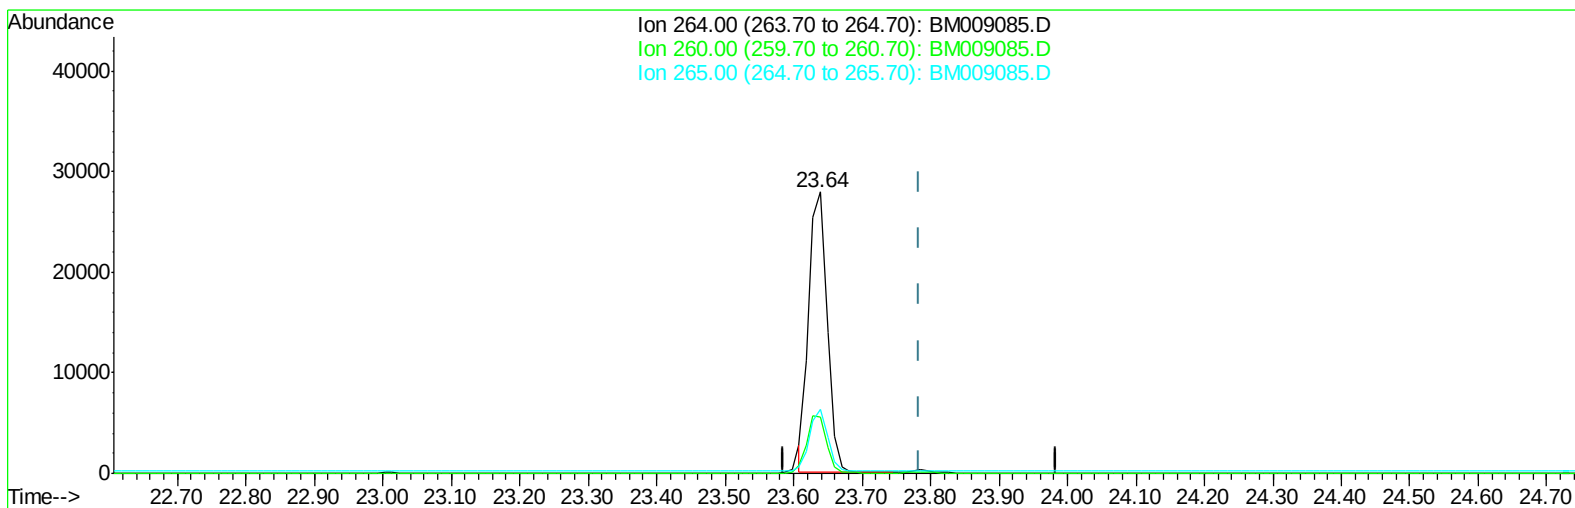

TIC: BM009085.D

(20) Perylene-d12 (I)




23.639min (-0.146) 0.40ng/ul

response 51798

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	19.88#
265.00	103.50	22.54#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030617\
Data File : BM009085.D
Acq On : 06 Mar 2017 18:15
Operator : SJ/MA
Sample : I2064-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 07 03:40:05 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 03:37:41 2017
Response via : Initial Calibration

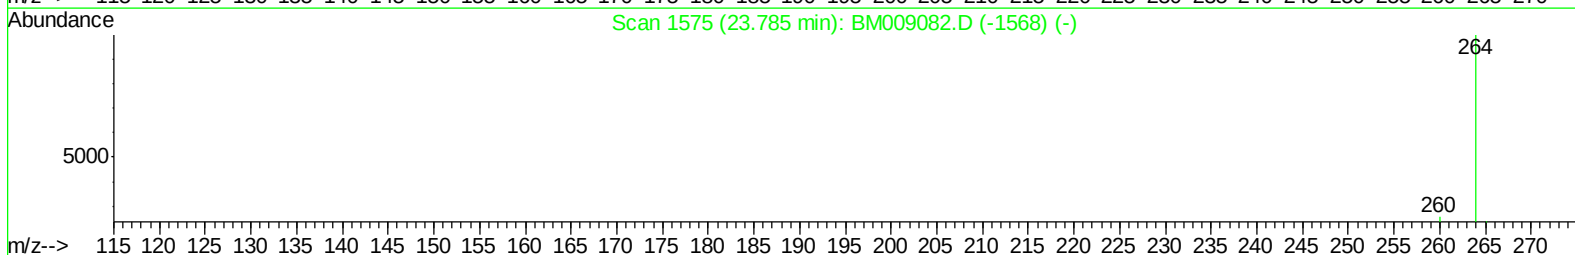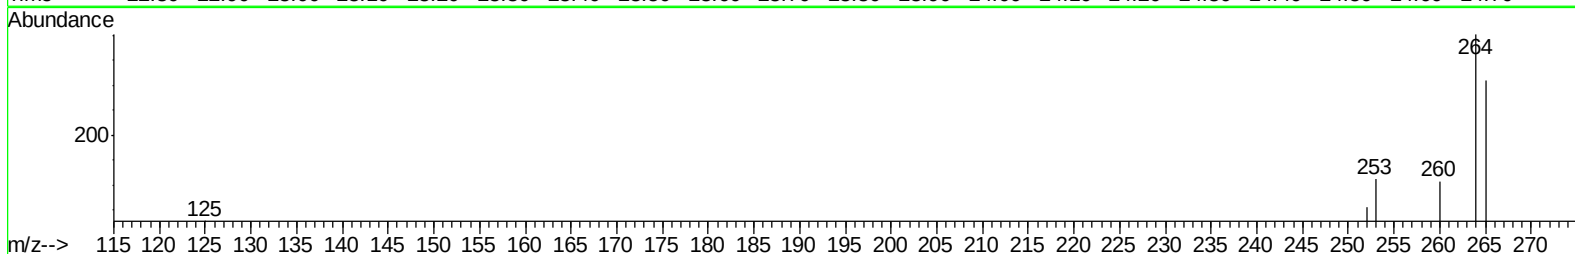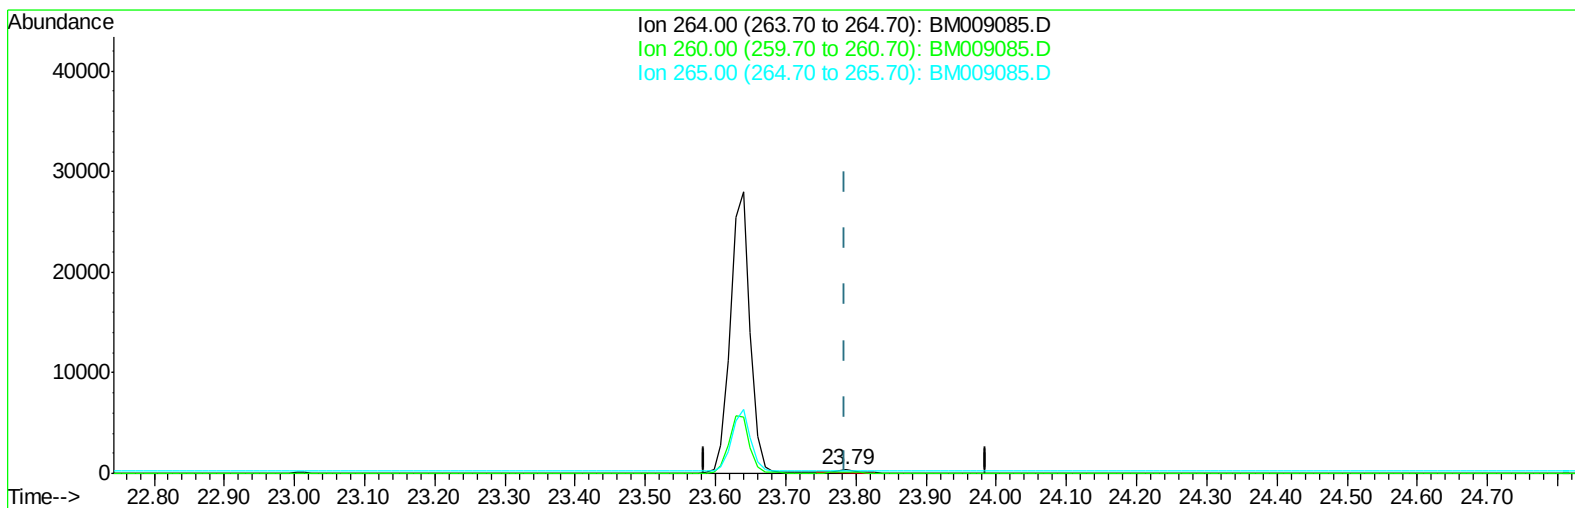

TIC: BM009085.D

(20) Perylene-d12 (I)

23.785min (+0.000) 0.40ng/ul m

response 620

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	34.53
265.00	103.50	79.56#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030617\
 Data File : BM009085.D
 Acq On : 06 Mar 2017 18:15
 Operator : SJ/MA
 Sample : I2064-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 07 04:01:34 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 07 03:37:41 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	147	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	459	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	282	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.28	188	686m	0.40	ng/ul	0.00
16) Chrysene-d12	21.45	240	654	0.40	ng/ul	0.00
20) Perylene-d12	23.79	264	620m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.28	152	229	0.30	ng/ul	0.00
14) Fluoranthene-d10	19.30	212	595	0.28	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030617\
Data File : BM009085.D
Acq On : 06 Mar 2017 18:15
Operator : SJ/MA
Sample : I2064-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 07 04:01:34 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 03:37:41 2017
Response via : Initial Calibration

