
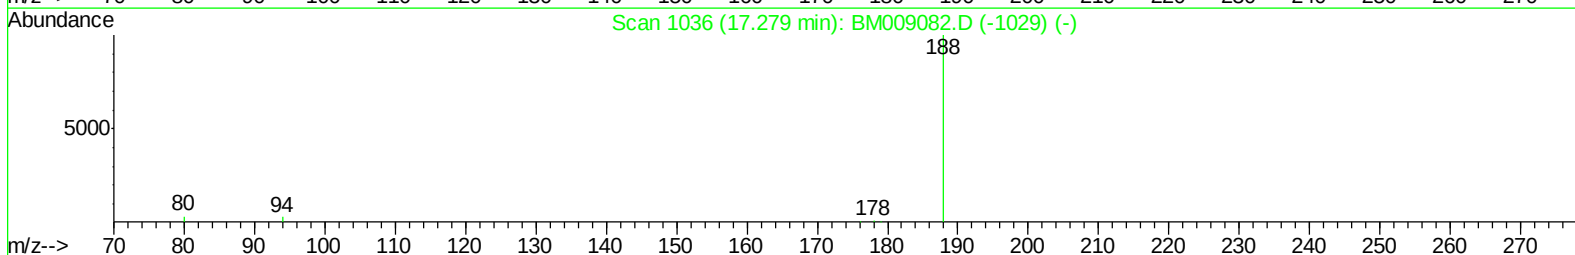
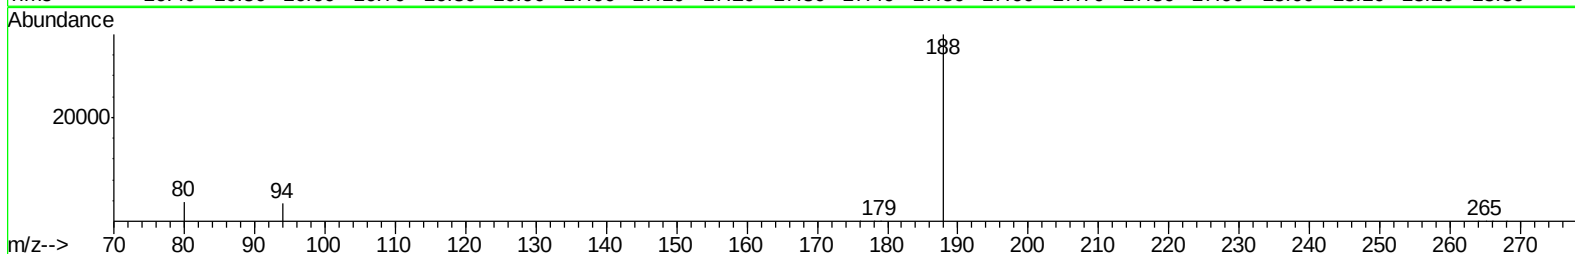


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030617\
Data File : BM009086.D
Acq On : 06 Mar 2017 18:51
Operator : SJ/MA
Sample : I2064-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Mar 07 03:40:10 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 03:37:41 2017
Response via : Initial Calibration

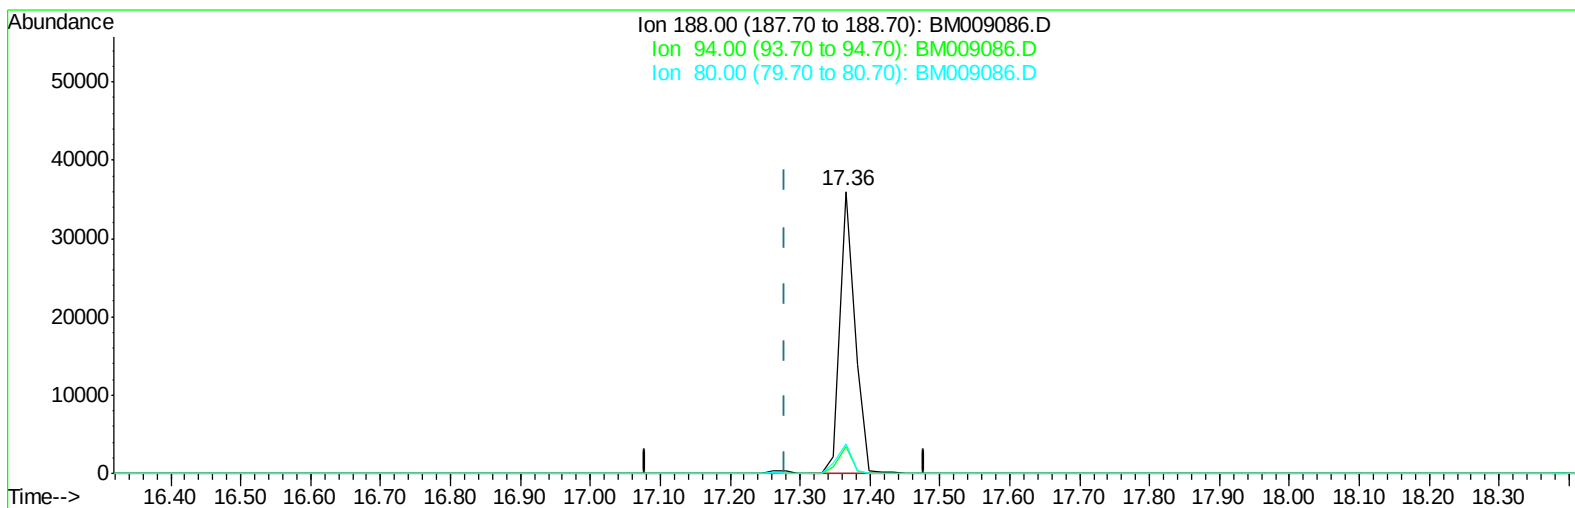

TIC: BM009086.D

(10) Phenanthrene-d10 (I)




17.365min (+0.086) 0.40ng/ul

response 53956

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	9.68
80.00	11.80	10.63
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030617\
Data File : BM009086.D
Acq On : 06 Mar 2017 18:51
Operator : SJ/MA
Sample : I2064-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Mar 07 03:40:10 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 03:37:41 2017
Response via : Initial Calibration

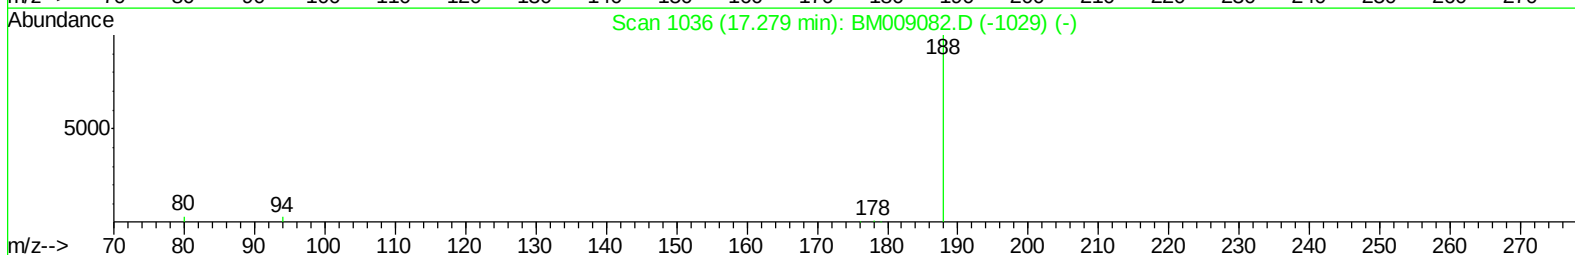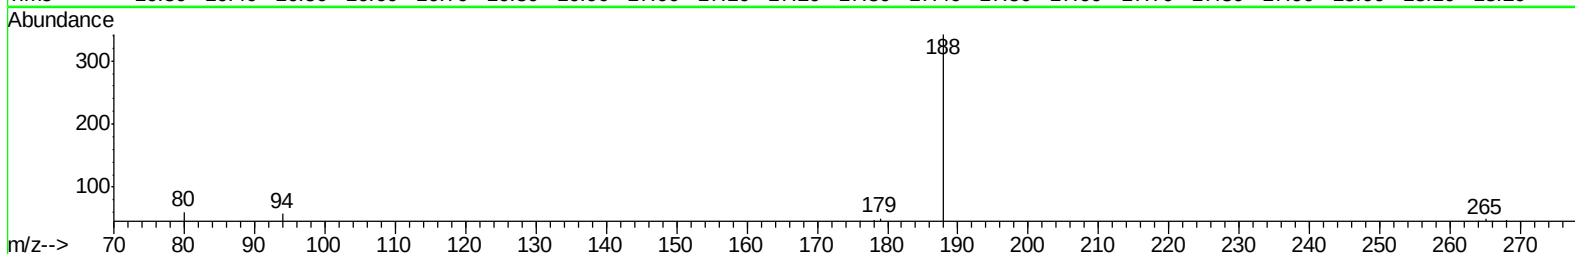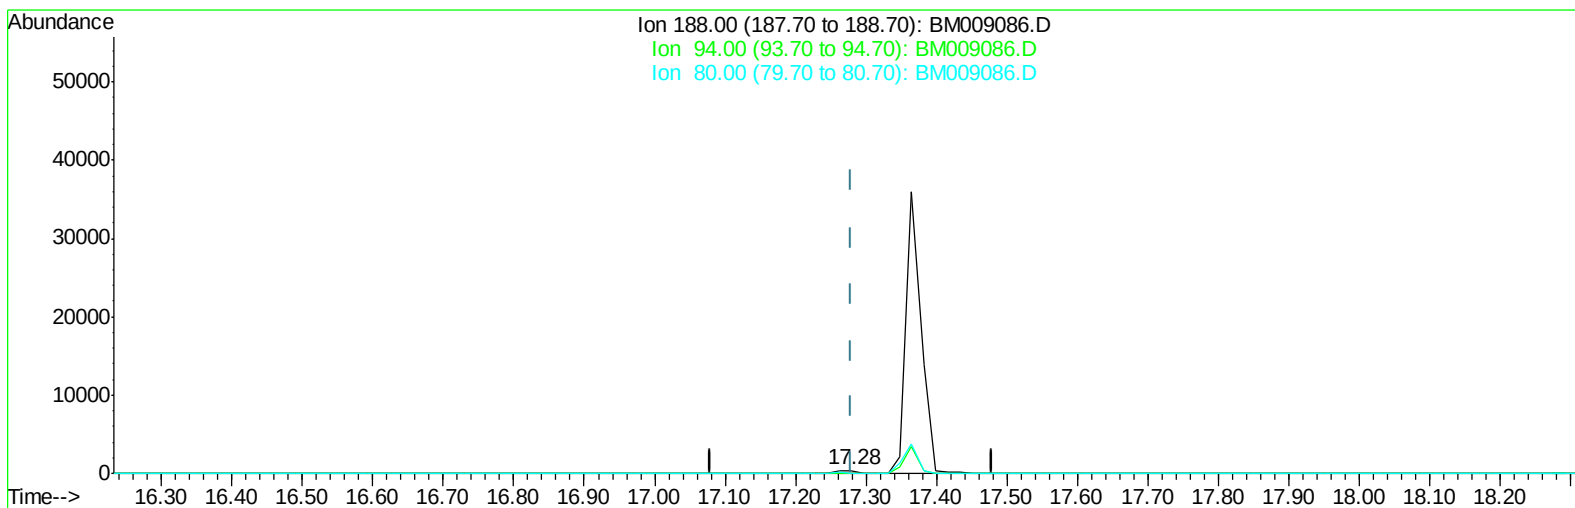

TIC: BM009086.D

(10) Phenanthrene-d10 (I)




17.279min (-0.000) 0.40ng/ul m

response 622

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	16.96#
80.00	11.80	17.84#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030617\
Data File : BM009086.D
Acq On : 06 Mar 2017 18:51
Operator : SJ/MA
Sample : I2064-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Mar 07 03:40:10 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 03:37:41 2017
Response via : Initial Calibration

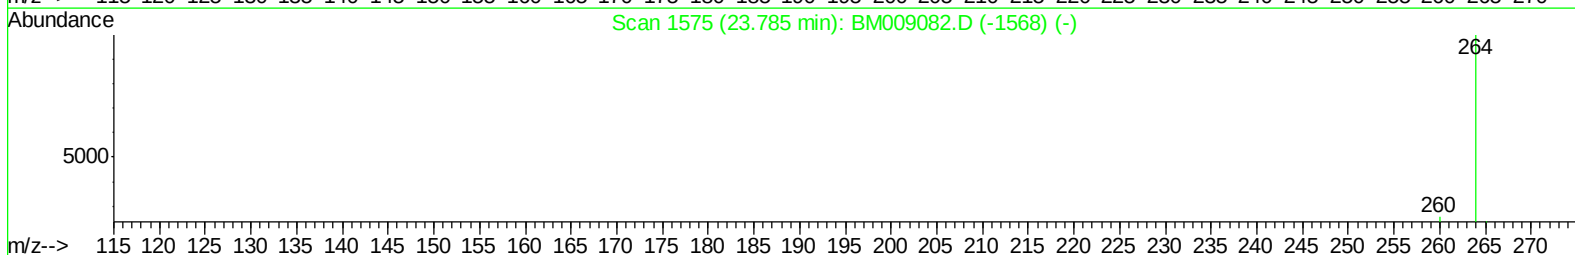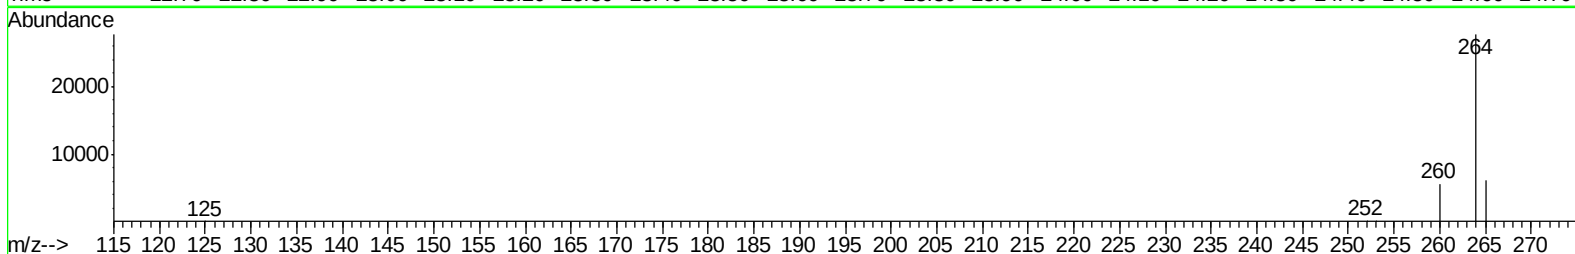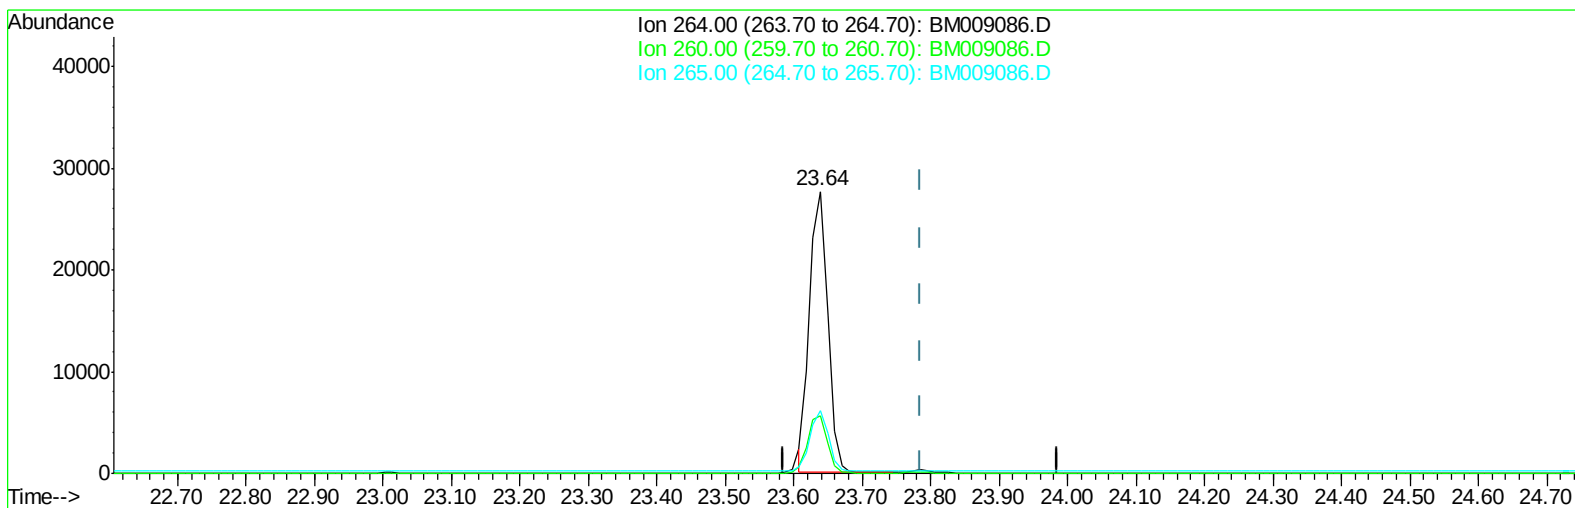

TIC: BM009086.D

(20) Perylene-d12 (I)




23.639min (-0.146) 0.40ng/ul

response 50672

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	20.50#
265.00	103.50	22.28#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030617\
Data File : BM009086.D
Acq On : 06 Mar 2017 18:51
Operator : SJ/MA
Sample : I2064-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Mar 07 03:40:10 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 03:37:41 2017
Response via : Initial Calibration

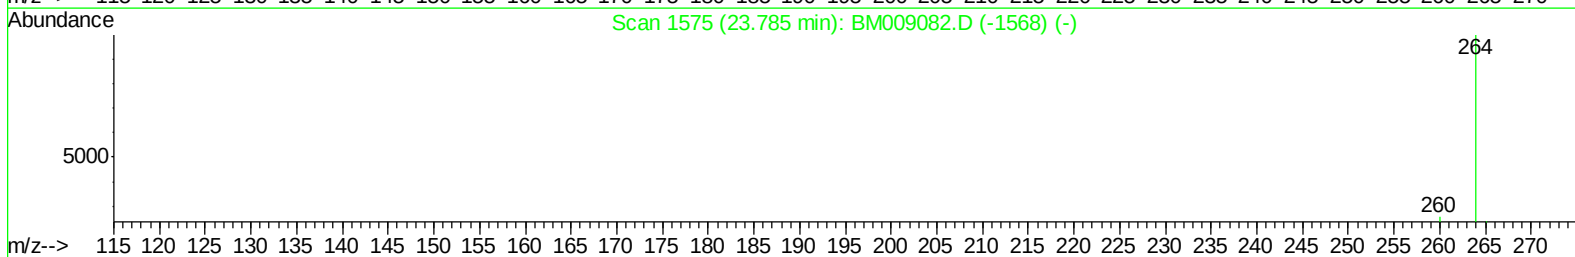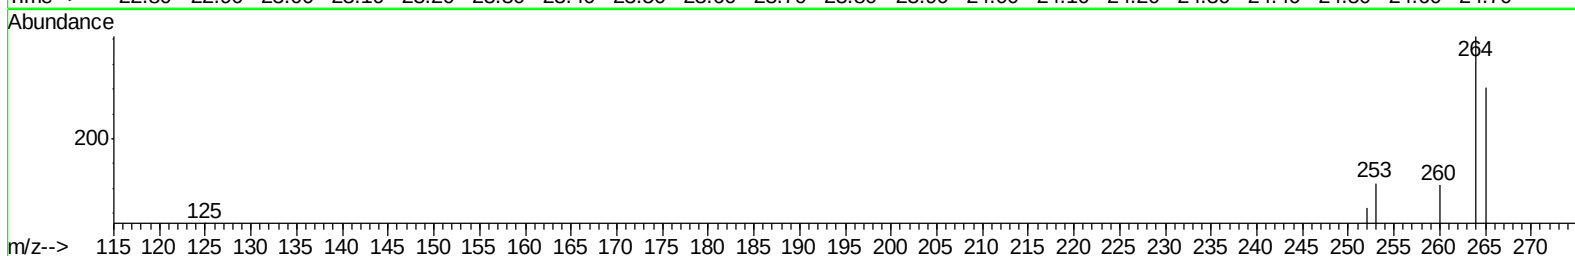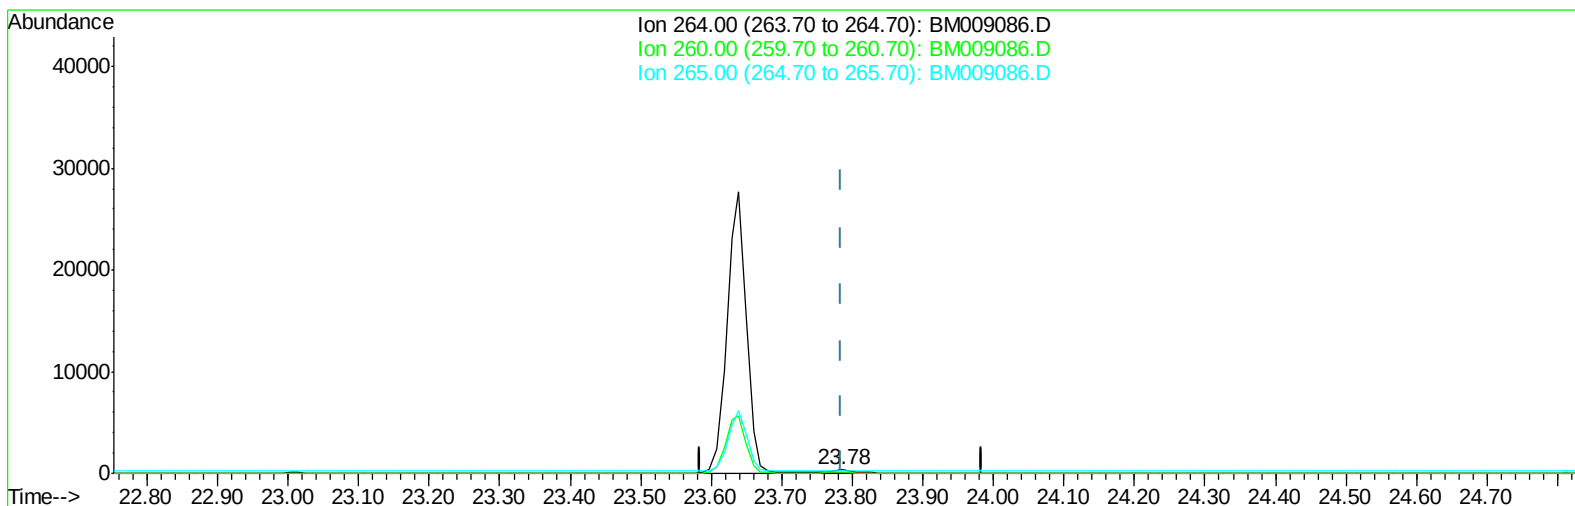

TIC: BM009086.D

(20) Perylene-d12 (I)

23.785min (-0.000) 0.40ng/ul m

response 583

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	34.25
265.00	103.50	77.26#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030617\
 Data File : BM009086.D
 Acq On : 06 Mar 2017 18:51
 Operator : SJ/MA
 Sample : I2064-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Quant Time: Mar 07 04:02:59 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 07 03:37:41 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	153	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	454	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	287	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.28	188	622m	0.40	ng/ul	0.00
16) Chrysene-d12	21.45	240	642	0.40	ng/ul	0.00
20) Perylene-d12	23.78	264	583m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.28	152	235	0.31	ng/ul	0.00
14) Fluoranthene-d10	19.30	212	579	0.30	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030617\
Data File : BM009086.D
Acq On : 06 Mar 2017 18:51
Operator : SJ/MA
Sample : I2064-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Mar 07 04:02:59 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 03:37:41 2017
Response via : Initial Calibration

