




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044543.D
Acq On : 07 Mar 2024 08:07
Operator : MA/JU
Sample : P1676-13
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E06Z9

Manual IntegrationsAPPROVED

Quant Time: Mar 07 08:36:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 05 23:05:11 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/07/2024
Supervised By :mohammad ahmed 03/09/2024

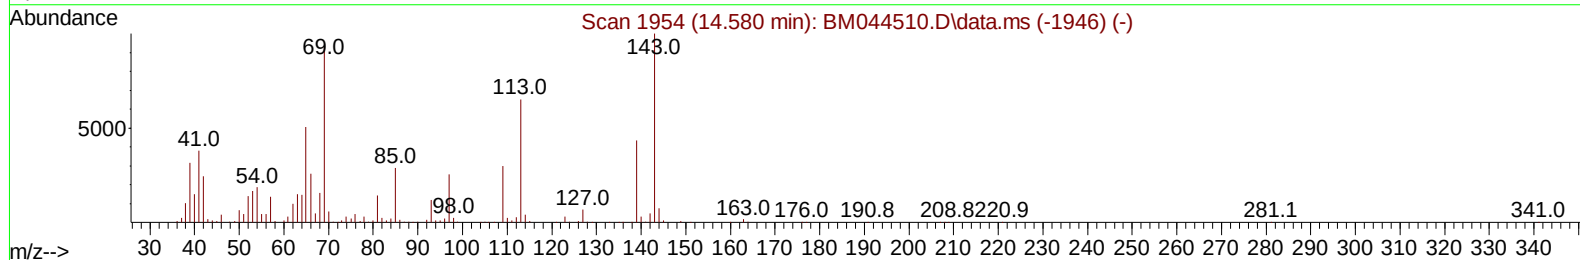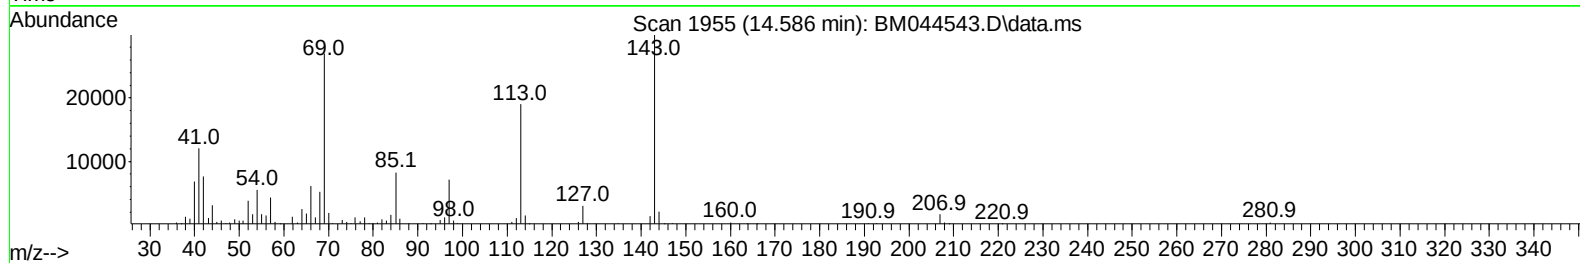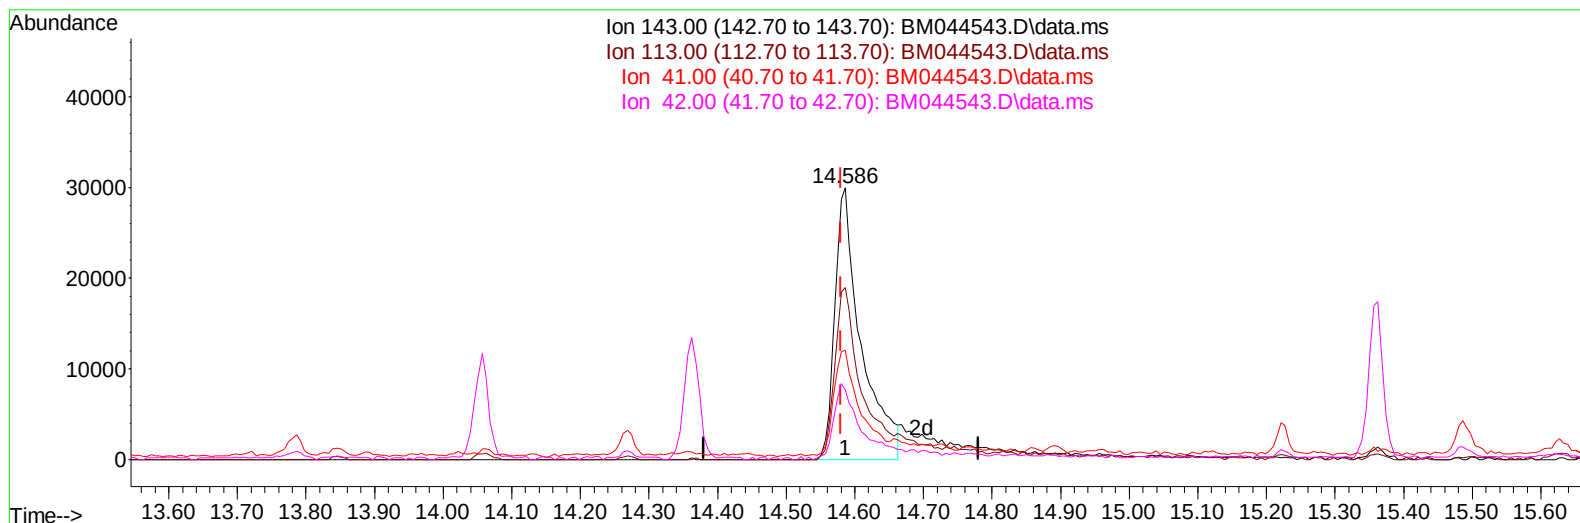

TIC: BM044543.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.586min (+ 0.006) 7.25 ng/ul

response 79655

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	63.70	63.43
41.00	38.40	40.20
42.00	26.60	25.53




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044543.D
Acq On : 07 Mar 2024 08:07
Operator : MA/JU
Sample : P1676-13
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E06Z9

Manual IntegrationsAPPROVED

Quant Time: Mar 07 08:36:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 05 23:05:11 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/07/2024
Supervised By :mohammad ahmed 03/09/2024

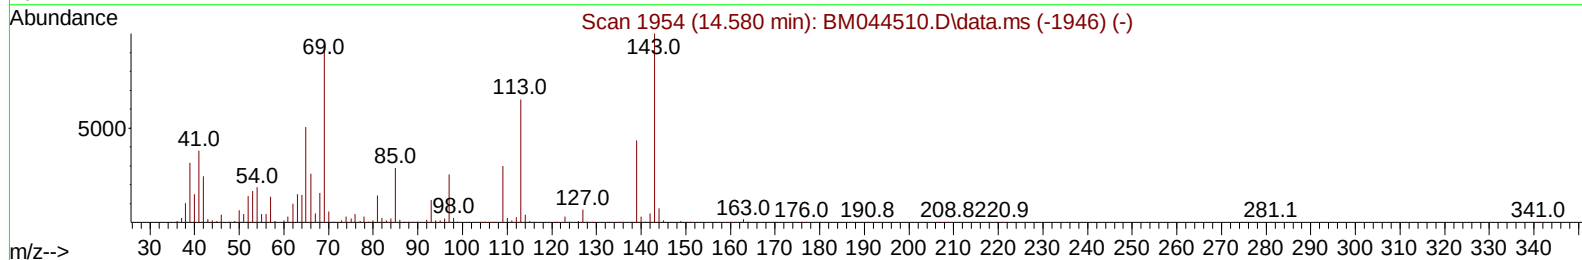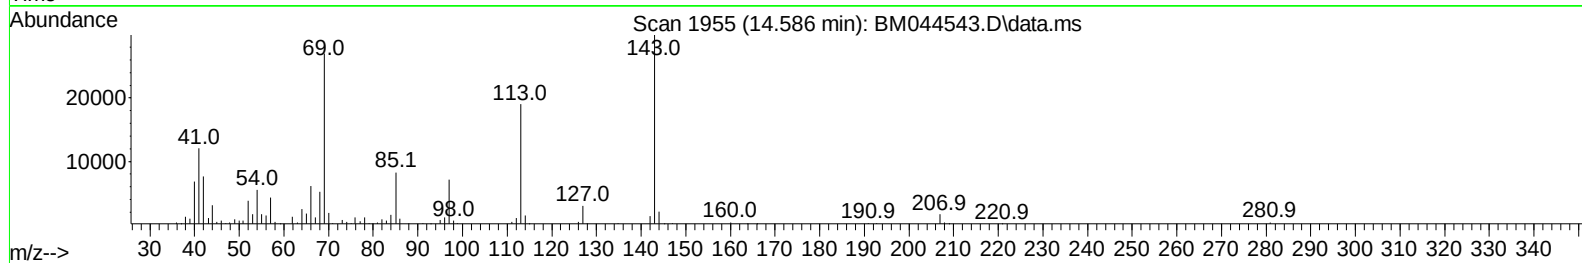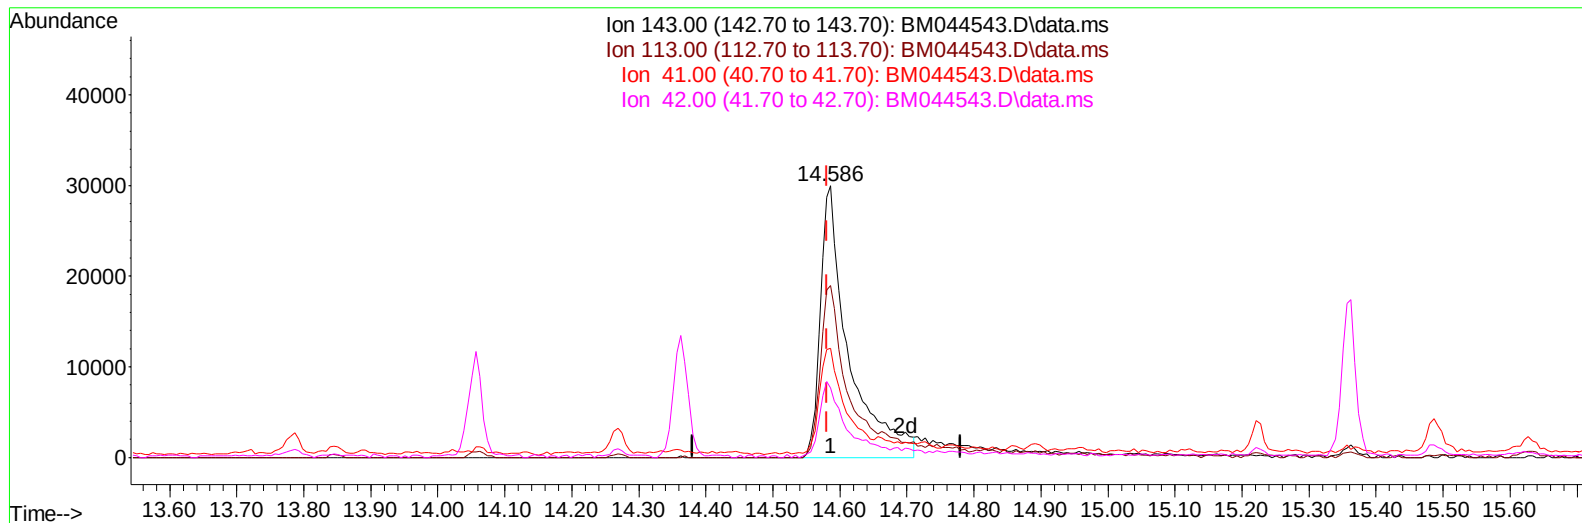

TIC: BM044543.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.586min (+ 0.006) 7.98 ng/ul m

response 87567

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	63.70	63.43
41.00	38.40	40.20
42.00	26.60	25.53

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
 Data File : BM044543.D
 Acq On : 07 Mar 2024 08:07
 Operator : MA/JU
 Sample : P1676-13
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E06Z9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/07/2024
 Supervised By :mohammad ahmed 03/09/2024

Quant Time: Mar 07 08:37:39 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 05 23:05:11 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.728	152	236627	20.000	ng/ul	0.00
20) Naphthalene-d8	10.510	136	1042888	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.363	164	674923	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.115	188	1360454	20.000	ng/ul	0.00
79) Chrysene-d12	21.303	240	1091316	20.000	ng/ul	0.00
88) Perylene-d12	23.550	264	1011651	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.287	96	19573	2.805	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	6.898	99	383495	15.764	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.075	67	280581	18.672	ng/ul	0.00
11) 2-Chlorophenol-d4	7.263	132	303473	16.975	ng/ul	0.00
15) 4-Methylphenol-d8	8.428	113	309649	16.207	ng/ul	-0.01
21) Nitrobenzene-d5	8.886	128	172023	19.589	ng/ul	0.00
24) 2-Nitrophenol-d4	9.598	143	156263	16.506	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.128	165	285043	17.691	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.657	131	390140	14.579	ng/ul	0.00
46) Dimethylphthalate-d6	13.786	166	894156	16.889	ng/ul	0.00
49) Acenaphthylene-d8	14.057	160	1301710	21.498	ng/ul	0.00
54) 4-Nitrophenol-d4	14.586	143	87567m	7.976	ng/ul	0.00
60) Fluorene-d10	15.363	176	1014699	22.807	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.486	200	51662	5.850	ng/ul	0.00
73) Anthracene-d10	17.209	188	1557156	23.946	ng/ul	-0.01
81) Pyrene-d10	19.509	212	1742169	26.028	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.403	264	1276493	24.006	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044543.D
Acq On : 07 Mar 2024 08:07
Operator : MA/JU
Sample : P1676-13
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E06Z9

Manual IntegrationsAPPROVED

Quant Time: Mar 07 08:37:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 05 23:05:11 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/07/2024
Supervised By :mohammad ahmed 03/09/2024

