




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044545.D
Acq On : 07 Mar 2024 09:19
Operator : MA/JU
Sample : P1679-02
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0704

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/07/2024
Supervised By :mohammad ahmed 03/09/2024

Quant Time: Mar 07 10:45:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 05 23:05:11 2024
Response via : Initial Calibration

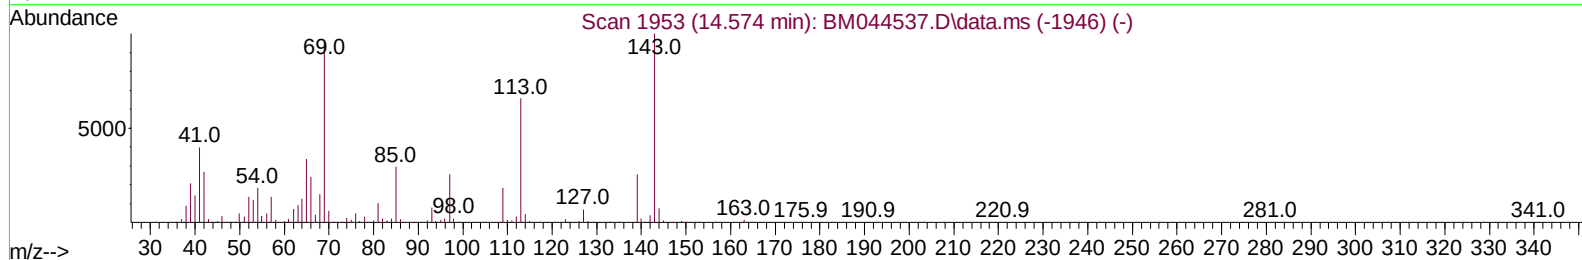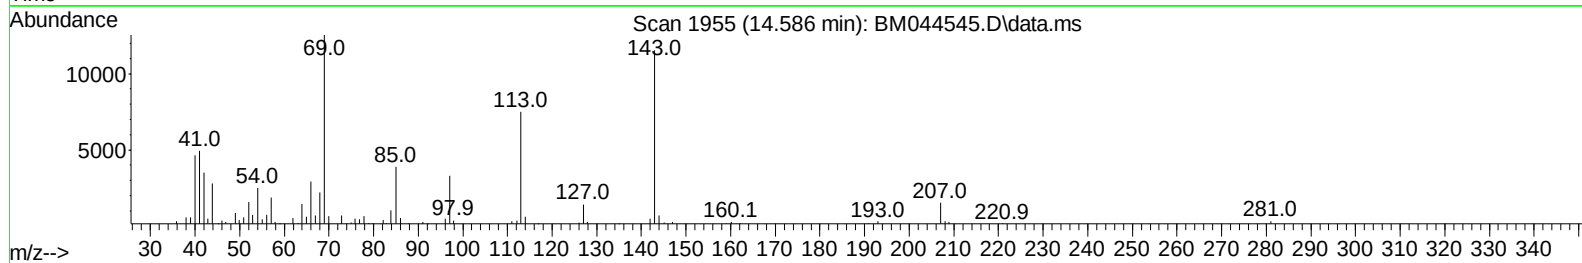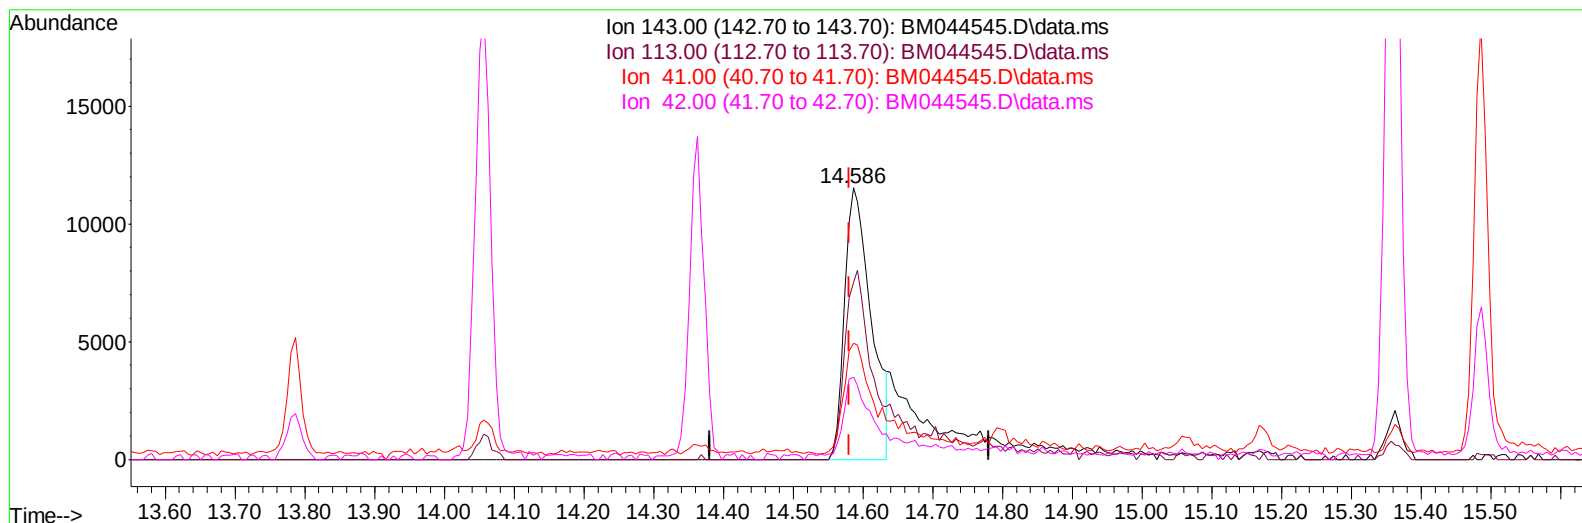

TIC: BM044545.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.586min (+ 0.006) 2.87 ng/ul

response 30466

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	63.70	65.19
41.00	38.40	42.85
42.00	26.60	30.40




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044545.D
Acq On : 07 Mar 2024 09:19
Operator : MA/JU
Sample : P1679-02
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0704

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/07/2024
Supervised By :mohammad ahmed 03/09/2024

Quant Time: Mar 07 10:45:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 05 23:05:11 2024
Response via : Initial Calibration

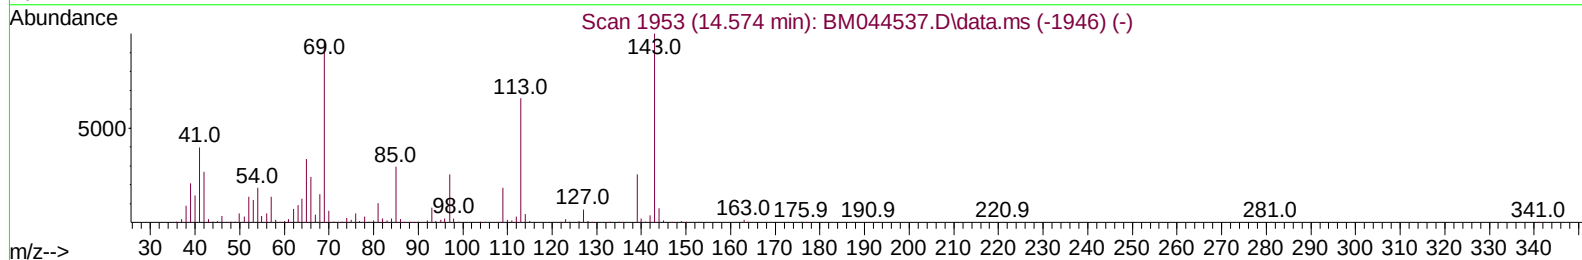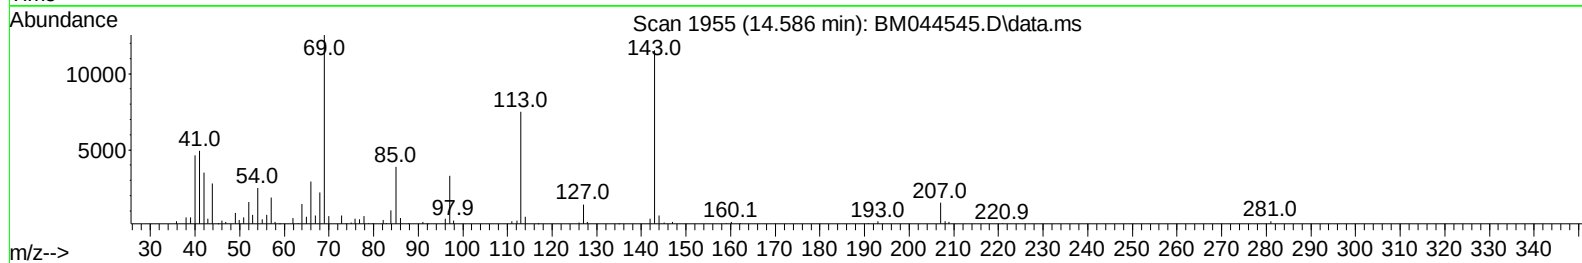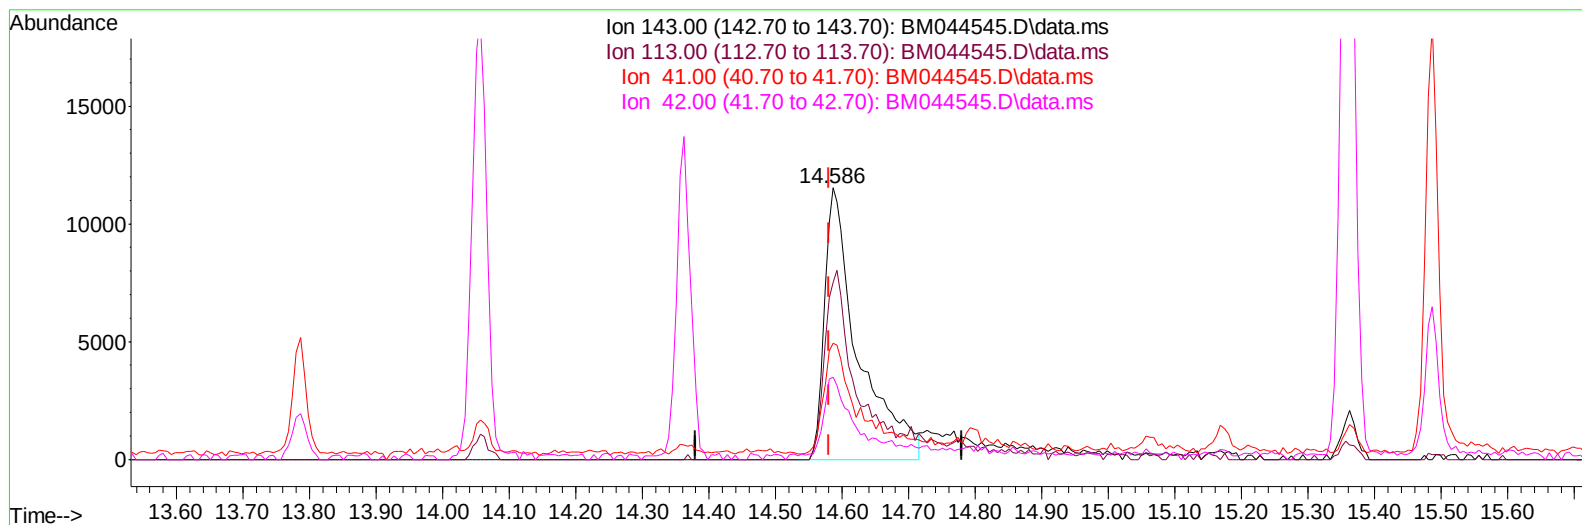

TIC: BM044545.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.586min (+ 0.006) 3.82 ng/ul m

response 40553

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	63.70	65.19
41.00	38.40	42.85
42.00	26.60	30.40

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
 Data File : BM044545.D
 Acq On : 07 Mar 2024 09:19
 Operator : MA/JU
 Sample : P1679-02
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0704

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/07/2024
 Supervised By :mohammad ahmed 03/09/2024

Quant Time: Mar 07 23:41:49 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 05 23:05:11 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.728	152	230380	20.000	ng/ul	0.00
20) Naphthalene-d8	10.504	136	1017627	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.363	164	653071	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.115	188	1277943	20.000	ng/ul	0.00
79) Chrysene-d12	21.297	240	878377	20.000	ng/ul	-0.01
88) Perylene-d12	23.544	264	863518	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	35152	5.175	ng/uL	0.00
4) Pyridine-d5	3.687	84	178470	8.927	ng/ul	0.00
7) Phenol-d5	6.898	99	150385	6.349	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.075	67	557421	38.100	ng/ul	0.00
11) 2-Chlorophenol-d4	7.263	132	474086	27.237	ng/ul	0.00
15) 4-Methylphenol-d8	8.428	113	292467	15.723	ng/ul	-0.01
21) Nitrobenzene-d5	8.886	128	342327	39.949	ng/ul	0.00
24) 2-Nitrophenol-d4	9.598	143	342887	37.118	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.128	165	538078	34.225	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.651	131	829828	31.780	ng/ul	-0.01
46) Dimethylphthalate-d6	13.786	166	2109608	41.180	ng/ul	0.00
49) Acenaphthylene-d8	14.057	160	2400015	40.964	ng/ul	0.00
54) 4-Nitrophenol-d4	14.586	143	40553m	3.817	ng/ul	0.00
60) Fluorene-d10	15.362	176	1834988	42.624	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.486	200	268437	32.360	ng/ul	0.00
73) Anthracene-d10	17.215	188	2789257	45.662	ng/ul	0.00
81) Pyrene-d10	19.509	212	2879579	53.451	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.403	264	2079586	45.818	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044545.D
Acq On : 07 Mar 2024 09:19
Operator : MA/JU
Sample : P1679-02
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0704

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/07/2024
Supervised By :mohammad ahmed 03/09/2024

Quant Time: Mar 07 23:41:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 05 23:05:11 2024
Response via : Initial Calibration

