

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
 Data File : BM044517.D
 Acq On : 06 Mar 2024 15:57
 Operator : MA/JU
 Sample : P1642-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0R33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044517.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	30	34	45	rVB	57115	92299	1.48%	0.167%
2	3.687	99	102	118	rBV	209549	405323	6.49%	0.734%
3	3.993	150	154	159	rVB	17365	26318	0.42%	0.048%
4	6.904	642	649	660	rBV	169432	288293	4.62%	0.522%
5	7.081	672	679	690	rBV	901161	1433084	22.96%	2.594%
6	7.263	703	710	719	rBV	732992	1172763	18.79%	2.123%
7	7.346	722	724	729	rVB5	6550	8900	0.14%	0.016%
8	7.734	783	790	797	rBV	829332	1354821	21.70%	2.452%
9	8.434	902	909	923	rBV	530977	892540	14.30%	1.616%
10	8.892	979	987	1005	rBV	958165	1632061	26.15%	2.954%
11	9.263	1046	1050	1056	rBV2	14270	21891	0.35%	0.040%
12	9.604	1101	1108	1115	rBV2	80367	140805	2.26%	0.255%
13	10.134	1191	1198	1217	rBV	891405	1517452	24.31%	2.747%
14	10.510	1254	1262	1273	rBV	1209163	2017251	32.32%	3.651%
15	10.657	1279	1287	1308	rBV	769188	1426525	22.85%	2.582%
16	11.757	1466	1474	1479	rBV2	12649	21492	0.34%	0.039%
17	12.116	1529	1535	1541	rBV3	16946	36011	0.58%	0.065%
18	13.263	1726	1730	1737	rBV4	17687	29475	0.47%	0.053%
19	13.786	1810	1819	1832	rBV	2254891	3147941	50.43%	5.698%
20	14.057	1858	1865	1874	rBV	2486245	3793481	60.77%	6.866%
21	14.369	1910	1918	1931	rBV	1877154	2780970	44.55%	5.034%
22	15.363	2080	2087	2100	rBV	3328215	4813523	77.11%	8.713%
23	15.604	2123	2128	2134	rBV4	13326	20797	0.33%	0.038%
24	16.157	2216	2222	2226	rVB6	9590	15833	0.25%	0.029%
25	16.804	2327	2332	2334	rBV6	5394	8145	0.13%	0.015%
26	16.904	2345	2349	2355	rBV4	4131	6871	0.11%	0.012%
27	17.115	2378	2385	2396	rBV	2204544	3203207	51.32%	5.798%
28	17.215	2396	2402	2418	rVV	3600774	5186283	83.08%	9.387%
29	18.027	2532	2540	2541	rBV6	9760	16355	0.26%	0.030%
30	18.457	2609	2613	2618	rVB8	6409	9986	0.16%	0.018%
31	19.074	2714	2718	2723	rBV	41504	60364	0.97%	0.109%
32	19.145	2726	2730	2736	rVV	34185	48099	0.77%	0.087%
33	19.309	2755	2758	2762	rBV4	8497	14042	0.22%	0.025%
34	19.509	2786	2792	2808	rBV	4336151	6111610	97.91%	11.062%
35	21.303	3092	3097	3108	rBV	2786081	3517266	56.35%	6.366%
36	23.415	3448	3456	3463	rBV	3312074	6242166	100.00%	11.299%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044517.D
Acq On : 06 Mar 2024 15:57
Operator : MA/JU
Sample : P1642-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0R33

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Title : SVOA CALIBRATION

37 23.556 3473 3480 3492 rVB 1964187 3732860 59.80% 6.757%




Sum of corrected areas: 55247103

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044517.D
Acq On : 06 Mar 2024 15:57
Operator : MA/JU
Sample : P1642-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0R33

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

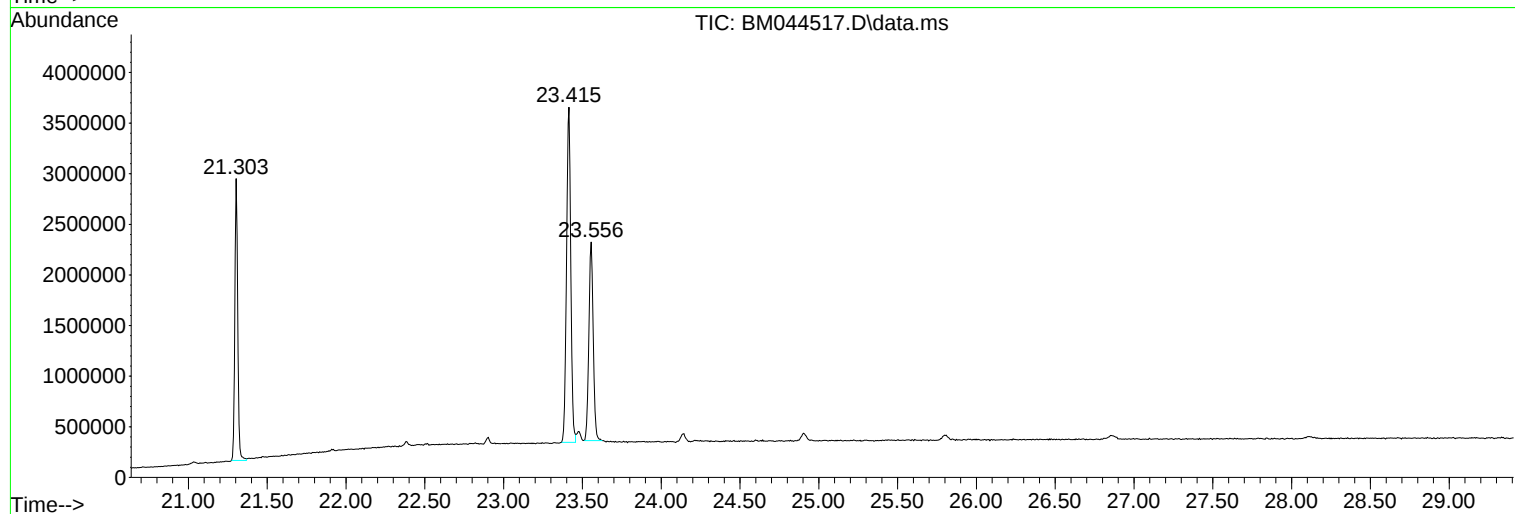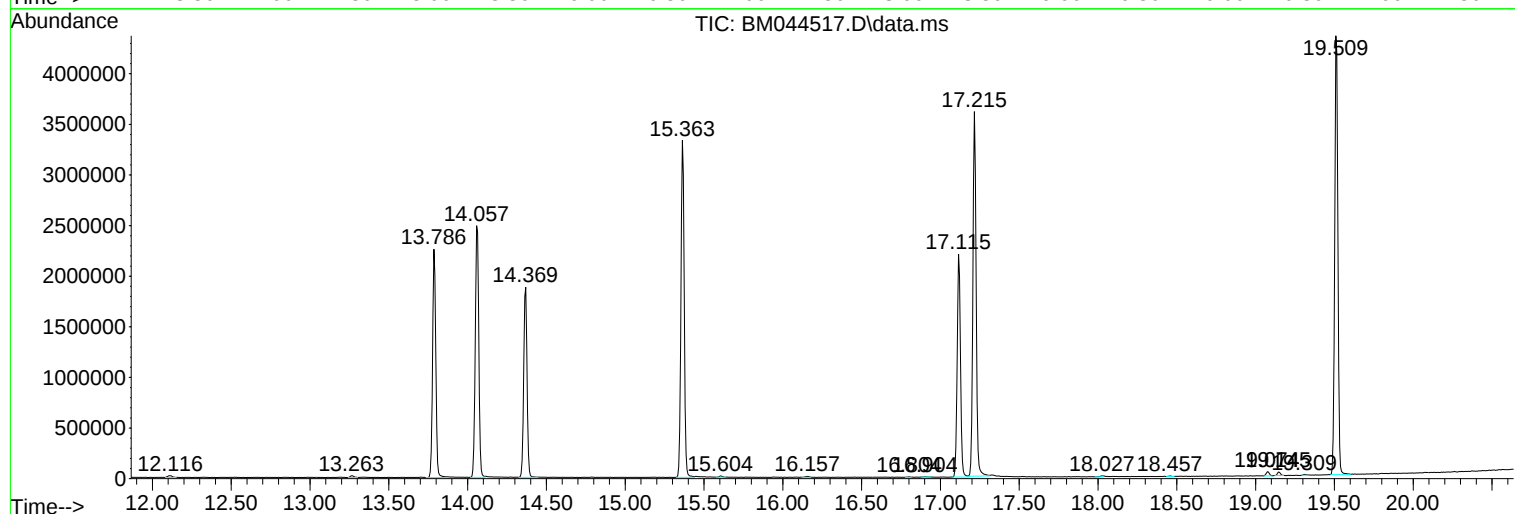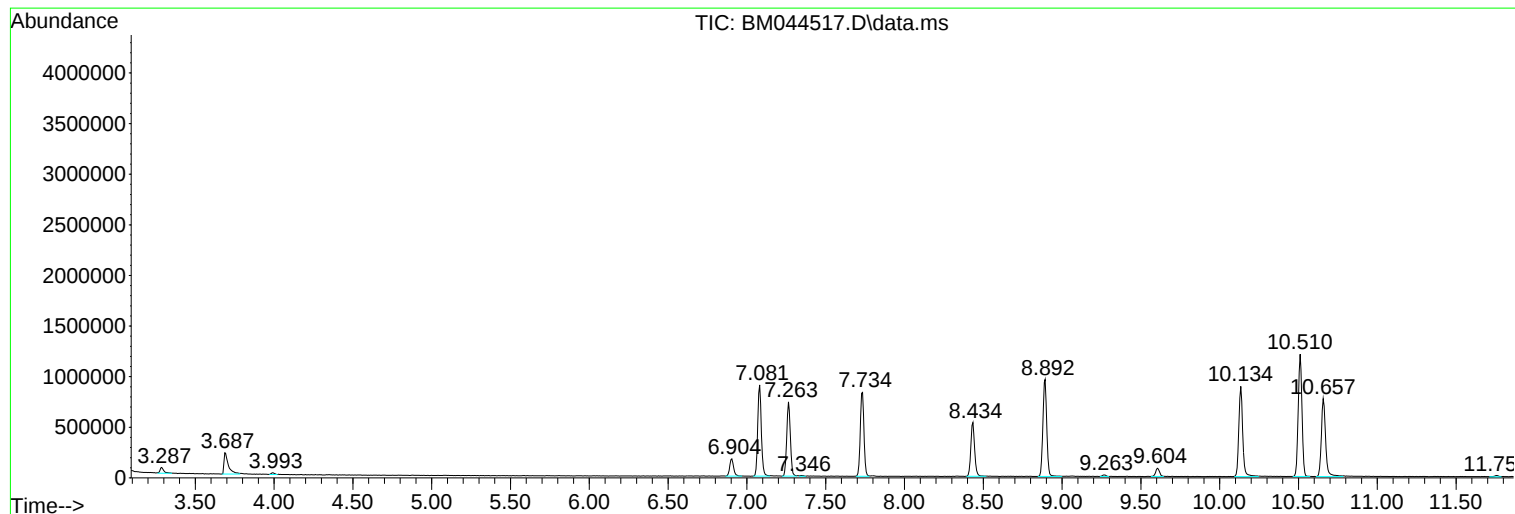

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044517.D
Acq On : 06 Mar 2024 15:57
Operator : MA/JU
Sample : P1642-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0R33

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044517.D
Acq On : 06 Mar 2024 15:57
Operator : MA/JU
Sample : P1642-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0R33

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc