

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
 Data File : BM044520.D
 Acq On : 06 Mar 2024 17:45
 Operator : MA/JU
 Sample : PB159461BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK461

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044520.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	30	34	41	rVB	76773	102354	1.42%	0.136%
2	3.681	98	101	125	rBV	977848	1621075	22.43%	2.159%
3	3.993	150	154	160	rVB	20770	30881	0.43%	0.041%
4	6.904	642	649	659	rBV	1127626	1830944	25.33%	2.438%
5	7.081	672	679	693	rBV	1022494	1617507	22.38%	2.154%
6	7.263	703	710	719	rBV	1158460	1819963	25.18%	2.424%
7	7.734	783	790	799	rVB	966926	1575852	21.80%	2.099%
8	8.434	901	909	922	rBV	1421440	2294973	31.75%	3.056%
9	8.892	978	987	1003	rBV	1107634	1881978	26.04%	2.506%
10	9.604	1101	1108	1121	rBV	929603	1530307	21.17%	2.038%
11	10.133	1191	1198	1216	rBV	1319351	2244532	31.05%	2.989%
12	10.510	1255	1262	1271	rBV	1447362	2403362	33.25%	3.201%
13	10.657	1279	1287	1308	rBV	1397350	2577336	35.66%	3.432%
14	12.110	1528	1534	1541	rVB	22342	40655	0.56%	0.054%
15	13.268	1725	1731	1737	rBV	24575	42918	0.59%	0.057%
16	13.786	1813	1819	1829	rBV	2705968	3860815	53.42%	5.142%
17	14.063	1858	1866	1874	rBV	2909382	4413451	61.06%	5.878%
18	14.368	1909	1918	1927	rBV	2210777	3256849	45.06%	4.337%
19	14.574	1945	1953	1979	rBV	834684	1811714	25.07%	2.413%
20	15.362	2080	2087	2101	rBV	3936800	5543255	76.69%	7.382%
21	15.492	2101	2109	2121	rVV	1340185	1965914	27.20%	2.618%
22	15.604	2124	2128	2133	rVB3	17330	29789	0.41%	0.040%
23	16.151	2216	2221	2226	rVB4	12787	19252	0.27%	0.026%
24	16.792	2328	2330	2336	rBV5	5916	8189	0.11%	0.011%
25	16.909	2346	2350	2355	rBV4	4509	7303	0.10%	0.010%
26	17.115	2379	2385	2395	rBV	2665476	3833610	53.04%	5.106%
27	17.215	2395	2402	2421	rVV	4358544	6216184	86.01%	8.279%
28	18.021	2534	2539	2547	rBV6	16573	39954	0.55%	0.053%
29	19.074	2714	2718	2724	rBV3	51561	76106	1.05%	0.101%
30	19.145	2726	2730	2739	rVV	42811	64306	0.89%	0.086%
31	19.309	2755	2758	2762	rBV6	11816	17602	0.24%	0.023%
32	19.509	2786	2792	2803	rBV	5136506	7227690	100.00%	9.626%
33	21.303	3092	3097	3108	rBV	3082806	3985375	55.14%	5.308%
34	23.415	3448	3456	3463	rBV2	3748310	6972447	96.47%	9.286%
35	23.556	3473	3480	3494	rVB	2103733	4123214	57.05%	5.491%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044520.D
Acq On : 06 Mar 2024 17:45
Operator : MA/JU
Sample : PB159461BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK461

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 75087656

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044520.D
Acq On : 06 Mar 2024 17:45
Operator : MA/JU
Sample : PB159461BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK461

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

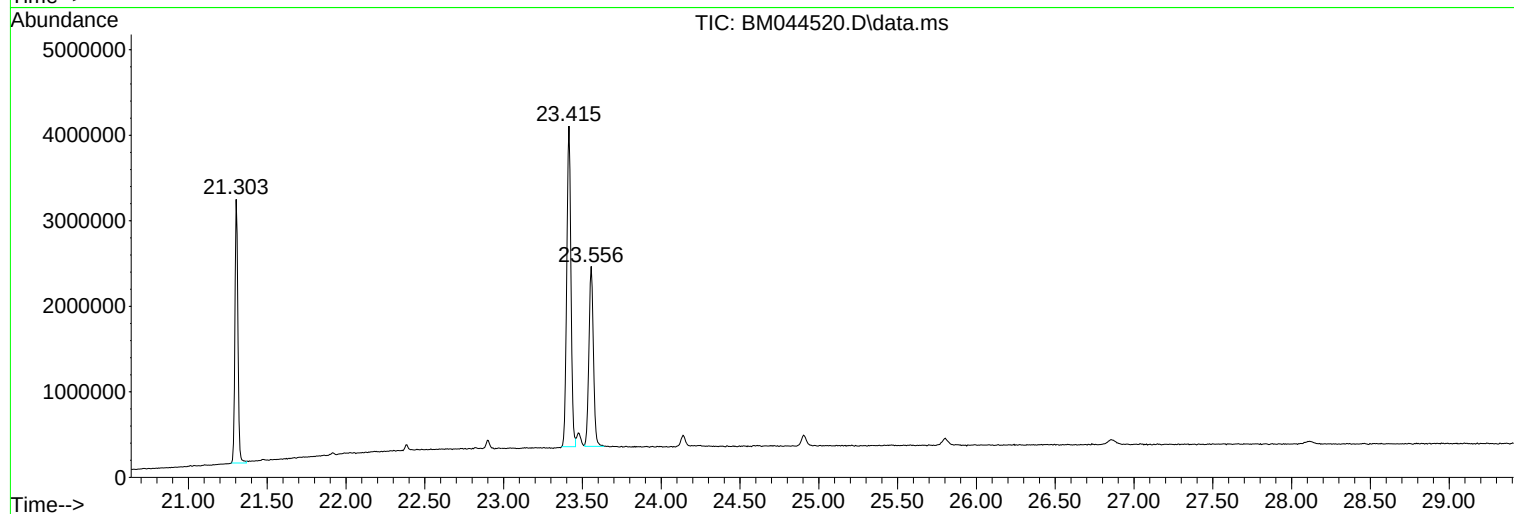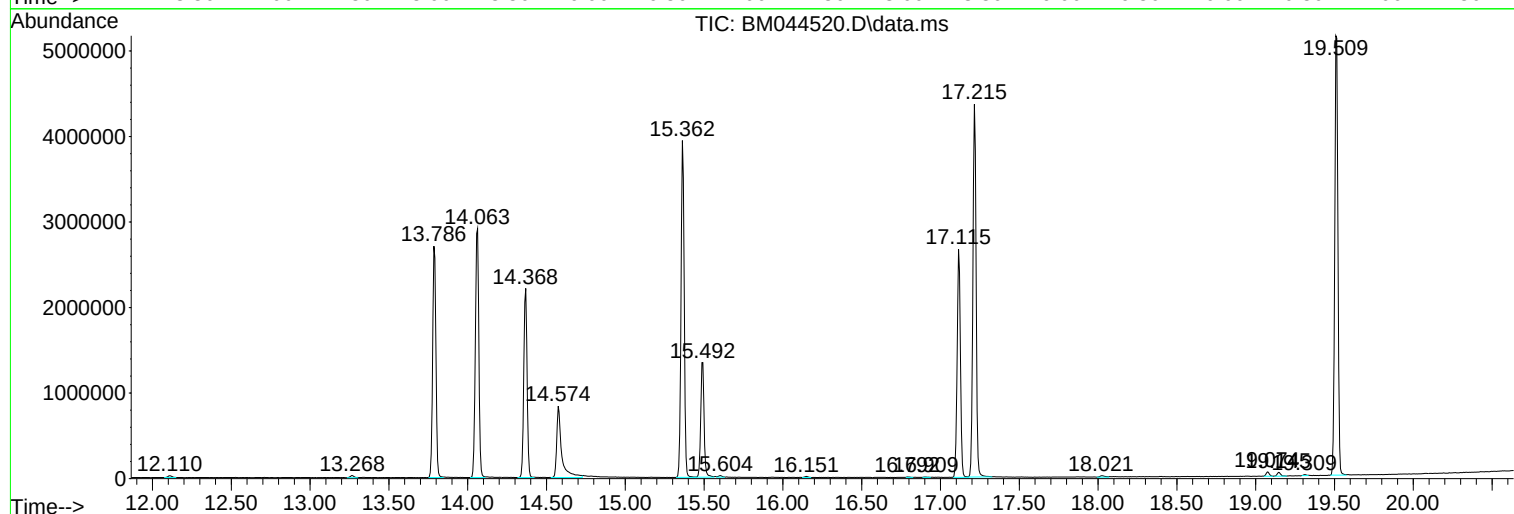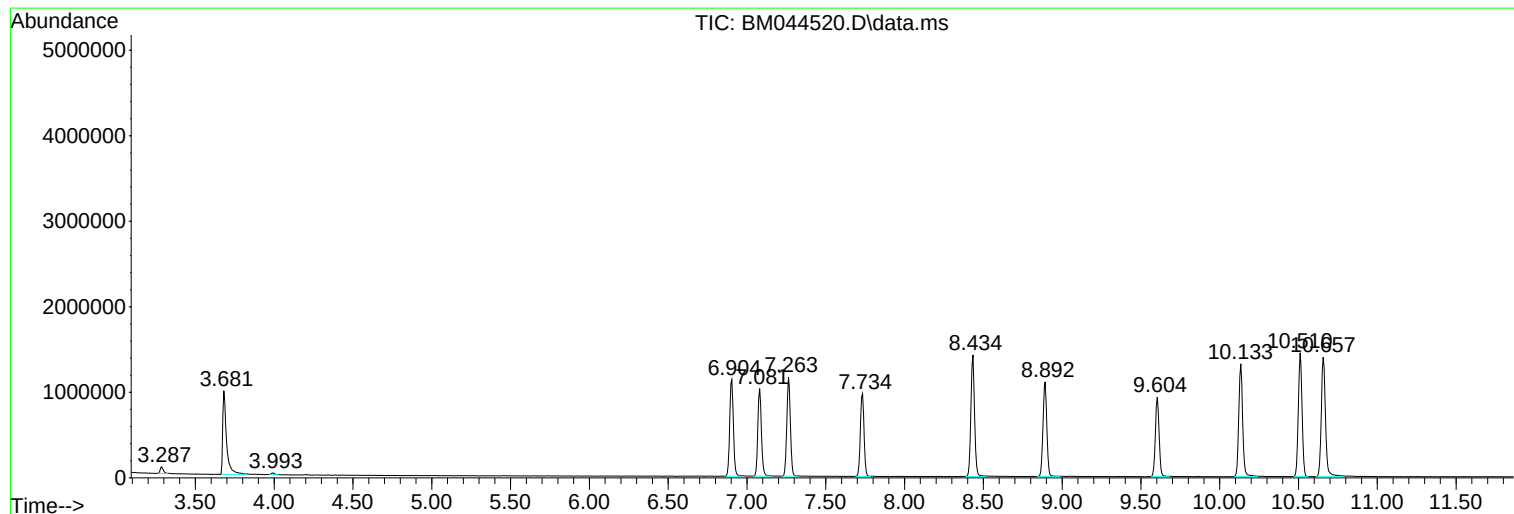

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044520.D
Acq On : 06 Mar 2024 17:45
Operator : MA/JU
Sample : PB159461BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK461

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044520.D
Acq On : 06 Mar 2024 17:45
Operator : MA/JU
Sample : PB159461BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK461

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc