

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
 Data File : BM044521.D
 Acq On : 06 Mar 2024 18:21
 Operator : MA/JU
 Sample : P1642-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0R32

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044521.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	30	34	46	rVB	65655	109428	1.43%	0.160%
2	3.693	99	103	114	rBV	175485	318630	4.16%	0.464%
3	3.993	150	154	159	rVB2	17798	27420	0.36%	0.040%
4	6.904	642	649	661	rBV	247173	415240	5.42%	0.605%
5	7.081	672	679	692	rBV	1171918	1833673	23.93%	2.673%
6	7.263	703	710	721	rBV	984329	1543120	20.13%	2.249%
7	7.345	721	724	732	rVB8	8735	14544	0.19%	0.021%
8	7.734	783	790	797	rBV	836982	1363678	17.79%	1.988%
9	7.792	797	800	807	rVB4	8554	16355	0.21%	0.024%
10	8.345	888	894	897	rBV6	4812	9000	0.12%	0.013%
11	8.434	902	909	921	rBV	750324	1208721	15.77%	1.762%
12	8.892	979	987	999	rBV	1252210	2083102	27.18%	3.037%
13	9.269	1046	1051	1057	rVB	21593	35546	0.46%	0.052%
14	9.604	1100	1108	1120	rBV	976071	1621913	21.16%	2.364%
15	10.133	1190	1198	1215	rBV	1304426	2248903	29.34%	3.278%
16	10.510	1254	1262	1270	rBV	1220638	2043343	26.66%	2.979%
17	10.657	1276	1287	1303	rBV	928568	1703989	22.23%	2.484%
18	11.757	1470	1474	1480	rVB	19626	30395	0.40%	0.044%
19	12.110	1528	1534	1542	rVB	23437	46019	0.60%	0.067%
20	13.186	1713	1717	1723	rBV7	5070	8649	0.11%	0.013%
21	13.263	1725	1730	1738	rVB	24779	38870	0.51%	0.057%
22	13.786	1812	1819	1830	rBV	2790018	4041141	52.73%	5.891%
23	14.063	1858	1866	1875	rBV	3227930	4940940	64.47%	7.203%
24	14.368	1910	1918	1926	rBV	1879691	2766622	36.10%	4.033%
25	14.592	1949	1956	1966	rBV2	66328	203089	2.65%	0.296%
26	15.362	2080	2087	2095	rBV	4148825	6110975	79.74%	8.908%
27	15.492	2102	2109	2124	rBV	1328235	1910239	24.92%	2.785%
28	15.604	2124	2128	2133	rVB3	17545	28029	0.37%	0.041%
29	16.151	2217	2221	2226	rVB3	12659	19455	0.25%	0.028%
30	16.792	2326	2330	2334	rBV7	5909	8612	0.11%	0.013%
31	16.904	2343	2349	2351	rBV6	5551	8995	0.12%	0.013%
32	17.115	2376	2385	2395	rBV	2310519	3235561	42.22%	4.717%
33	17.215	2395	2402	2421	rVV2	4621588	6651804	86.79%	9.697%
34	18.021	2534	2539	2546	rBV2	95294	148729	1.94%	0.217%
35	18.456	2609	2613	2617	rBV5	8408	12717	0.17%	0.019%
36	19.074	2714	2718	2724	rVB2	51166	74162	0.97%	0.108%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044521.D
Acq On : 06 Mar 2024 18:21
Operator : MA/JU
Sample : P1642-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0R32

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Title : SVOA CALIBRATION

37	19.145	2726	2730	2736	rBV	46034	71590	0.93%	0.104%
38	19.303	2753	2757	2767	rBV5	50735	86983	1.13%	0.127%
39	19.515	2786	2793	2802	rBV	5568733	7664045	100.00%	11.172%
40	21.033	3048	3051	3060	rBV6	40082	62808	0.82%	0.092%
41	21.303	3092	3097	3108	rBV	2615529	3336587	43.54%	4.864%
42	23.415	3448	3456	3464	rBV	3766285	7147118	93.26%	10.419%
43	23.550	3473	3479	3495	rVB	1707055	3348224	43.69%	4.881%




Sum of corrected areas: 68598963

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044521.D
Acq On : 06 Mar 2024 18:21
Operator : MA/JU
Sample : P1642-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0R32

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

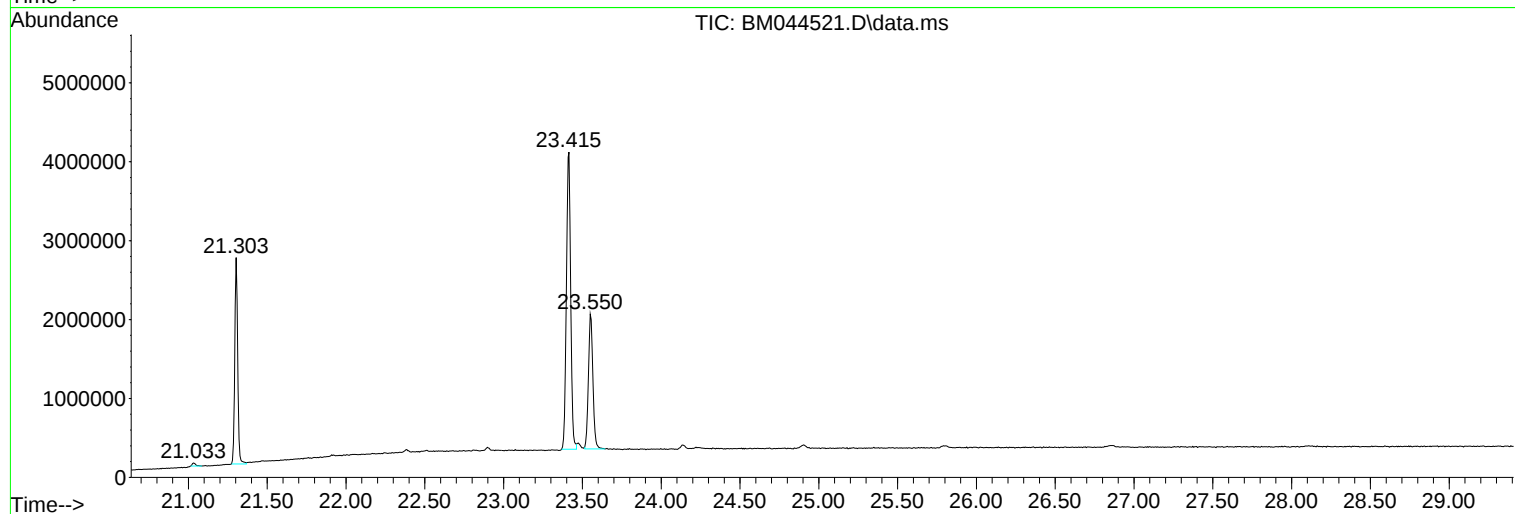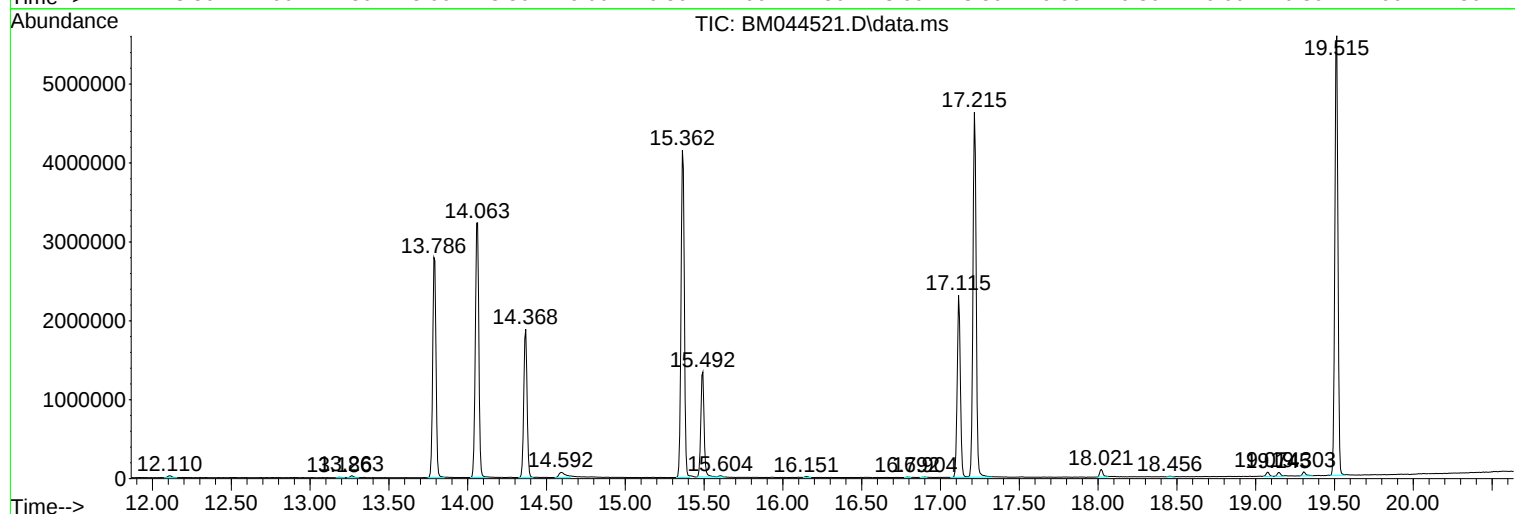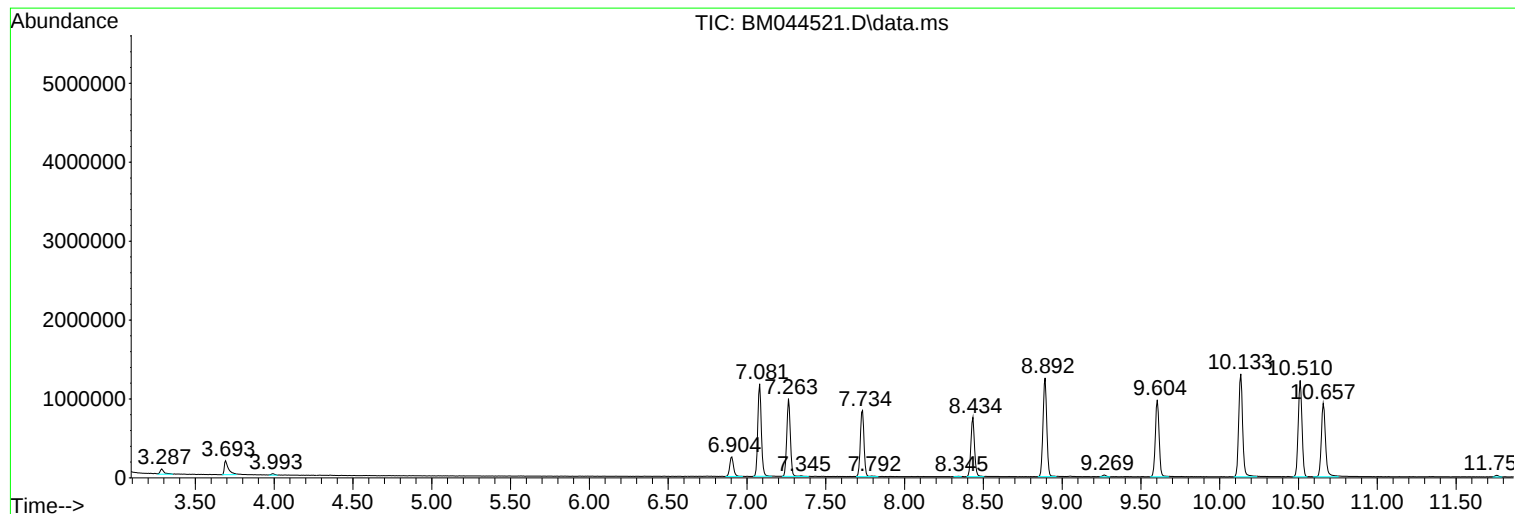

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044521.D
Acq On : 06 Mar 2024 18:21
Operator : MA/JU
Sample : P1642-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0R32

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044521.D
Acq On : 06 Mar 2024 18:21
Operator : MA/JU
Sample : P1642-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0R32

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc