

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
 Data File : BM044528.D
 Acq On : 06 Mar 2024 22:32
 Operator : MA/JU
 Sample : P1676-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E06Y4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044528.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	31	34	40	rVB	38768	51050	1.39%	0.116%
2	3.699	100	104	121	rVB	82282	161144	4.40%	0.365%
3	3.993	151	154	158	rVB	14848	20428	0.56%	0.046%
4	6.898	642	648	663	rBV	592794	988216	26.96%	2.239%
5	7.081	672	679	689	rBV	552244	897137	24.48%	2.032%
6	7.263	703	710	721	rBV	617224	972137	26.53%	2.202%
7	7.728	782	789	797	rBV	906859	1459418	39.82%	3.306%
8	7.793	797	800	804	rVB5	5890	8030	0.22%	0.018%
9	8.434	901	909	919	rBV	729485	1230327	33.57%	2.787%
10	8.887	979	986	997	rBV	606108	1036103	28.27%	2.347%
11	9.051	1010	1014	1018	rVB6	5512	6281	0.17%	0.014%
12	9.263	1046	1050	1056	rVB8	5175	8959	0.24%	0.020%
13	9.604	1097	1108	1118	rBV	465720	789817	21.55%	1.789%
14	9.822	1141	1145	1150	rVB6	3117	4742	0.13%	0.011%
15	10.134	1191	1198	1209	rBV	676792	1188595	32.43%	2.692%
16	10.510	1253	1262	1275	rBV	1334989	2209870	60.30%	5.006%
17	10.657	1279	1287	1307	rBV	729565	1346537	36.74%	3.050%
18	11.933	1501	1504	1510	rVB7	6523	11946	0.33%	0.027%
19	12.110	1528	1534	1540	rBV2	14012	24780	0.68%	0.056%
20	12.763	1641	1645	1649	rVB6	3972	5401	0.15%	0.012%
21	12.898	1663	1668	1673	rBV6	6451	9575	0.26%	0.022%
22	13.186	1713	1717	1724	rBV3	16095	23500	0.64%	0.053%
23	13.263	1724	1730	1737	rVV	45274	74523	2.03%	0.169%
24	13.345	1740	1744	1749	rVB6	3931	5732	0.16%	0.013%
25	13.786	1811	1819	1828	rBV	1422419	2042395	55.73%	4.626%
26	13.974	1848	1851	1854	rVB5	3866	4785	0.13%	0.011%
27	14.057	1858	1865	1876	rVV	1727175	2552018	69.63%	5.781%
28	14.274	1897	1902	1905	rVB2	16072	21047	0.57%	0.048%
29	14.363	1910	1917	1925	rBV	1990773	2950220	80.50%	6.683%
30	14.586	1948	1955	1970	rBV	190727	556811	15.19%	1.261%
31	14.892	2004	2007	2011	rVB6	5309	7163	0.20%	0.016%
32	14.969	2016	2020	2025	rBV6	3407	5122	0.14%	0.012%
33	15.157	2049	2052	2053	rBV3	3408	3726	0.10%	0.008%
34	15.174	2053	2055	2058	rVV4	3616	4563	0.12%	0.010%
35	15.227	2060	2064	2068	rVV	17199	21508	0.59%	0.049%
36	15.363	2079	2087	2101	rBV	2207546	3236981	88.32%	7.332%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
 Data File : BM044528.D
 Acq On : 06 Mar 2024 22:32
 Operator : MA/JU
 Sample : P1676-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E06Y4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Title : SVOA CALIBRATION

37	15.486	2102	2108	2121	rBV	356077	532091	14.52%	1.205%
38	15.604	2124	2128	2130	rBV4	10151	12804	0.35%	0.029%
39	15.792	2158	2160	2163	rVV3	4197	4687	0.13%	0.011%
40	15.839	2167	2168	2173	rVB5	4581	4811	0.13%	0.011%
41	16.092	2206	2211	2213	rBV3	20816	32079	0.88%	0.073%
42	16.157	2217	2222	2227	rVB7	7655	13882	0.38%	0.031%
43	16.421	2264	2267	2269	rBV4	2780	3711	0.10%	0.008%
44	16.668	2304	2309	2311	rBV6	3986	6215	0.17%	0.014%
45	16.798	2328	2331	2333	rVB4	4812	4608	0.13%	0.010%
46	16.886	2342	2346	2350	rBV3	16422	27925	0.76%	0.063%
47	16.933	2352	2354	2358	rVB4	8473	10478	0.29%	0.024%
48	17.115	2378	2385	2395	rBV	2299693	3285524	89.65%	7.442%
49	17.215	2395	2402	2416	rVV	2336660	3333555	90.96%	7.551%
50	17.415	2433	2436	2441	rVB6	6982	8367	0.23%	0.019%
51	17.621	2467	2471	2476	rBV3	15746	21354	0.58%	0.048%
52	17.768	2493	2496	2498	rBV4	4260	4392	0.12%	0.010%
53	17.798	2499	2501	2504	rVV4	5860	5789	0.16%	0.013%
54	17.904	2514	2519	2522	rBV7	3710	6442	0.18%	0.015%
55	18.015	2534	2538	2546	rBV2	52568	82506	2.25%	0.187%
56	18.098	2550	2552	2554	rVB3	5471	4655	0.13%	0.011%
57	18.315	2585	2589	2594	rBV2	15896	22773	0.62%	0.052%
58	18.957	2695	2698	2702	rVB	16028	14962	0.41%	0.034%
59	19.074	2714	2718	2722	rBV4	28593	40039	1.09%	0.091%
60	19.145	2727	2730	2734	rVV	24216	36918	1.01%	0.084%
61	19.186	2735	2737	2746	rVB10	11085	19469	0.53%	0.044%
62	19.304	2754	2757	2762	rBV6	22695	31464	0.86%	0.071%
63	19.509	2786	2792	2800	rBV	2722445	3664897	100.00%	8.302%
64	20.074	2885	2888	2892	rVB3	30588	33355	0.91%	0.076%
65	20.568	2969	2972	2977	rBV3	40024	46336	1.26%	0.105%
66	21.033	3047	3051	3056	rBV	213729	314395	8.58%	0.712%
67	21.303	3091	3097	3105	rBV	2220457	2869634	78.30%	6.500%
68	23.409	3448	3455	3463	rBV	1532506	2916680	79.58%	6.607%
69	23.550	3473	3479	3493	rVB	1422993	2788585	76.09%	6.317%




Sum of corrected areas: 44145969

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044528.D
Acq On : 06 Mar 2024 22:32
Operator : MA/JU
Sample : P1676-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E06Y4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

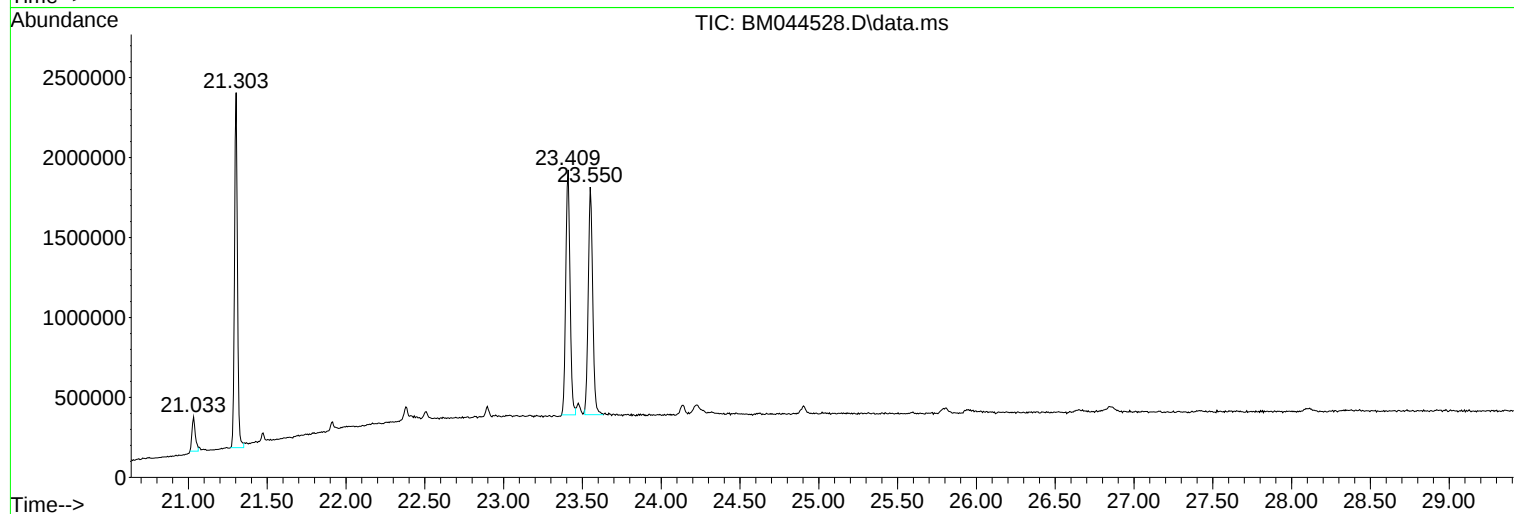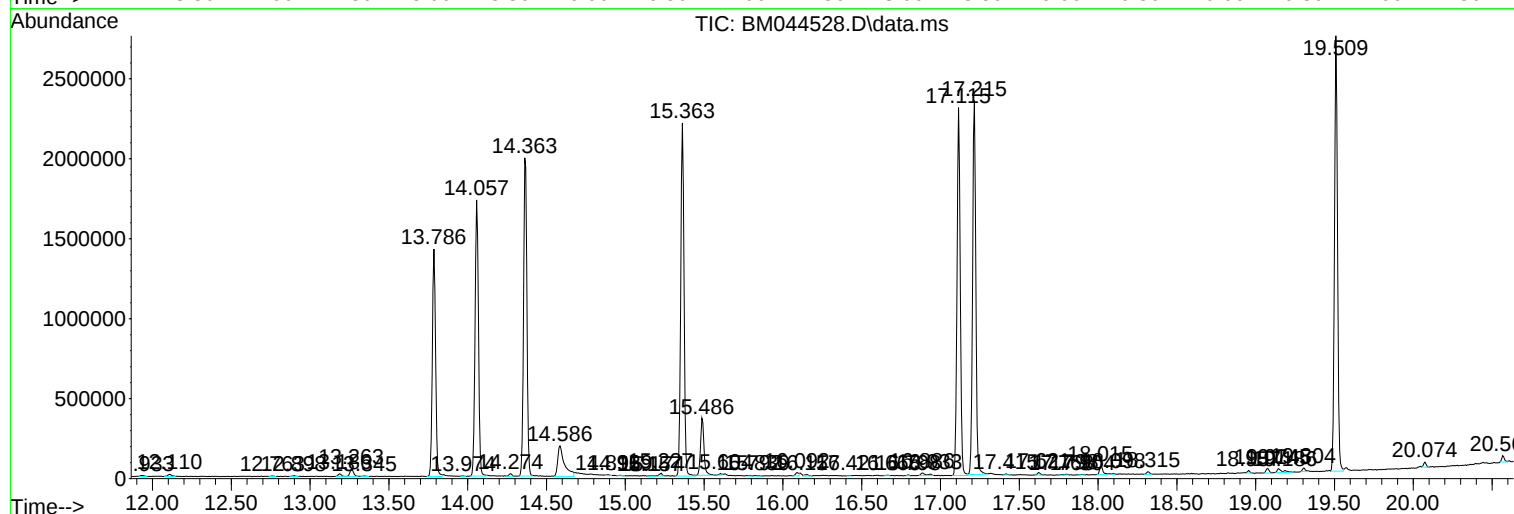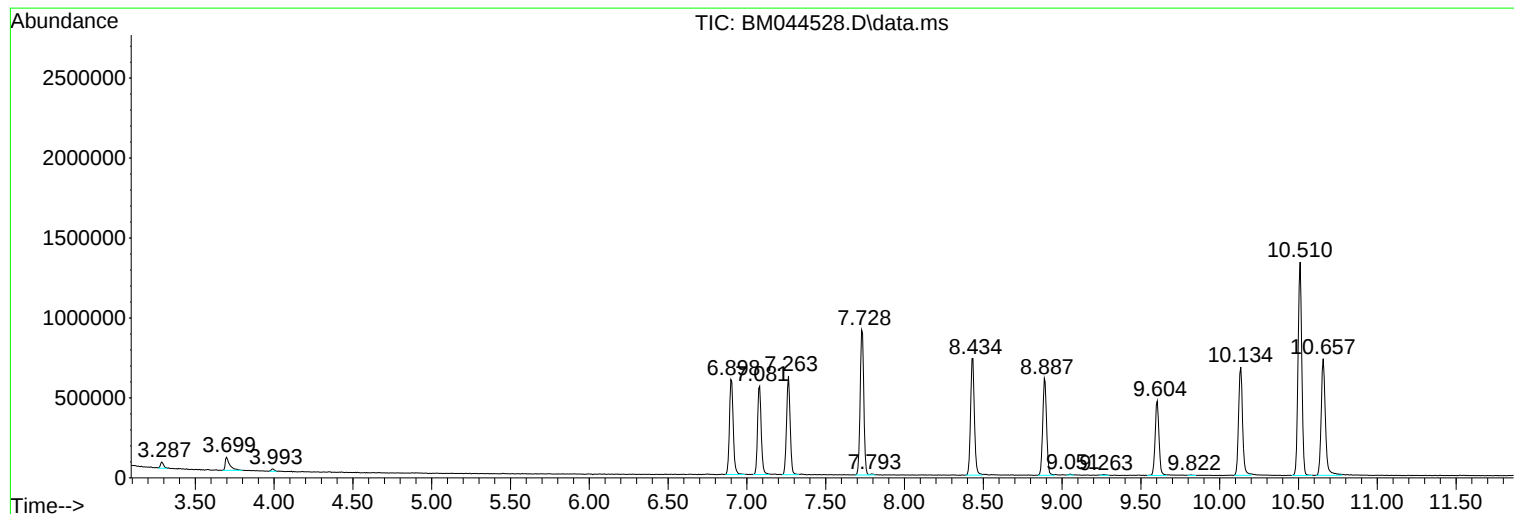

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044528.D
Acq On : 06 Mar 2024 22:32
Operator : MA/JU
Sample : P1676-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E06Y4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.033	2.19 ng/ul	314395	Chrysene-d12	21.303

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		5-Octadecene, (E)-	252	C18H36	007206-21-5	96
2		3-Eicosene, (E)-	280	C20H40	074685-33-9	95
3		Pentadecafluorooctanoic acid, oc...	666	C26H37F15O2	1000406-04-8	94
4		5-Eicosene, (E)-	280	C20H40	074685-30-6	92
5		Ethanol, 2-(tetradecyloxy)-	258	C16H34O2	002136-70-1	91

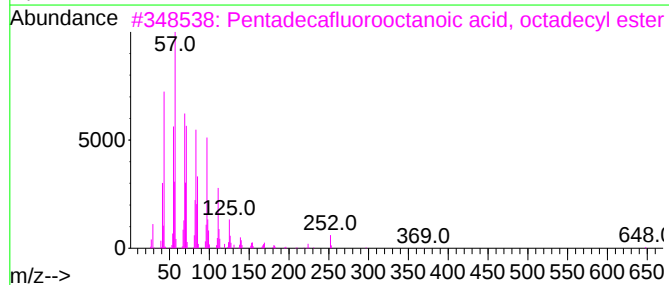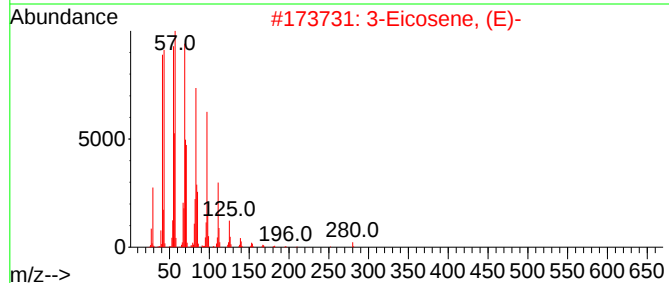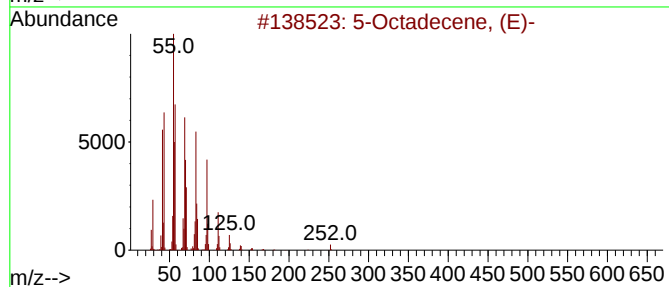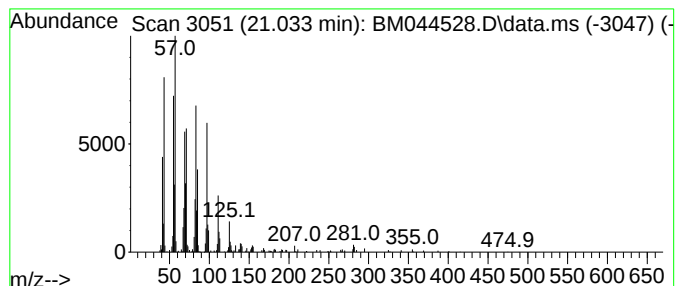

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044528.D
Acq On : 06 Mar 2024 22:32
Operator : MA/JU
Sample : P1676-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E06Y4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.033	2.2	ng/u1	314395	5	21.303	2869630	20.0