

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
 Data File : BM044530.D
 Acq On : 06 Mar 2024 23:44
 Operator : MA/JU
 Sample : P1676-07
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E06Y6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044530.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	30	34	39	rVB	29522	39221	0.76%	0.076%
2	3.699	101	104	115	rBV	51686	104740	2.04%	0.202%
3	3.993	150	154	159	rVB	15839	23935	0.47%	0.046%
4	6.899	641	648	663	rBV	632672	1044446	20.30%	2.018%
5	7.081	672	679	689	rBV	633396	1022929	19.88%	1.977%
6	7.263	702	710	720	rBV	639385	1012153	19.67%	1.956%
7	7.728	782	789	796	rBV	870338	1377076	26.76%	2.661%
8	8.434	902	909	922	rBV	790243	1328579	25.82%	2.568%
9	8.887	979	986	1004	rBV	707418	1226538	23.84%	2.370%
10	9.051	1008	1014	1021	rVB8	10853	17878	0.35%	0.035%
11	9.269	1047	1051	1057	rVB5	5632	8299	0.16%	0.016%
12	9.604	1101	1108	1124	rBV	353871	624576	12.14%	1.207%
13	9.822	1137	1145	1149	rBV3	16423	27079	0.53%	0.052%
14	10.134	1191	1198	1215	rBV	718205	1262622	24.54%	2.440%
15	10.510	1251	1262	1271	rBV	1262796	2118444	41.17%	4.094%
16	10.657	1276	1287	1304	rBV	570237	1071943	20.83%	2.072%
17	11.428	1412	1418	1422	rVB9	5613	8514	0.17%	0.016%
18	11.528	1428	1435	1440	rBV4	13411	21573	0.42%	0.042%
19	11.787	1475	1479	1483	rBV7	3744	5975	0.12%	0.012%
20	11.934	1495	1504	1510	rBV	41308	67828	1.32%	0.131%
21	12.110	1529	1534	1539	rVV3	13330	24542	0.48%	0.047%
22	12.151	1539	1541	1548	rVB7	6871	11466	0.22%	0.022%
23	12.575	1606	1613	1617	rBV8	6327	14190	0.28%	0.027%
24	12.681	1627	1631	1633	rBV4	5330	6320	0.12%	0.012%
25	12.763	1639	1645	1648	rBV6	7289	12740	0.25%	0.025%
26	12.839	1653	1658	1663	rBV6	8308	13052	0.25%	0.025%
27	12.892	1663	1667	1672	rVV2	21257	28994	0.56%	0.056%
28	13.187	1708	1717	1724	rBV	81841	136314	2.65%	0.263%
29	13.263	1725	1730	1737	rVV3	36757	63715	1.24%	0.123%
30	13.345	1742	1744	1749	rVB6	10020	14891	0.29%	0.029%
31	13.498	1764	1770	1773	rBV6	3468	5801	0.11%	0.011%
32	13.710	1801	1806	1811	rBV7	3923	8876	0.17%	0.017%
33	13.786	1811	1819	1826	rBV	1228259	1780826	34.61%	3.442%
34	13.851	1826	1830	1834	rVB2	44836	66310	1.29%	0.128%
35	13.892	1834	1837	1843	rVB3	13691	22228	0.43%	0.043%
36	13.969	1846	1850	1856	rBV6	8889	13571	0.26%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
 Data File : BM044530.D
 Acq On : 06 Mar 2024 23:44
 Operator : MA/JU
 Sample : P1676-07
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E06Y6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Title : SVOA CALIBRATION

37	14.057	1856	1865	1874	rBV	2176433	3228856	62.75%	6.240%
38	14.210	1885	1891	1893	rBV7	4881	8941	0.17%	0.017%
39	14.269	1896	1901	1908	rVB	109230	143658	2.79%	0.278%
40	14.363	1910	1917	1925	rBV	1883531	2860284	55.59%	5.528%
41	14.463	1932	1934	1938	rVB5	4595	5598	0.11%	0.011%
42	14.592	1950	1956	1971	rBV3	82581	275146	5.35%	0.532%
43	14.775	1984	1987	1993	rVB7	11754	18721	0.36%	0.036%
44	14.892	2000	2007	2013	rVV4	25317	40252	0.78%	0.078%
45	14.957	2016	2018	2022	rVB3	6476	8568	0.17%	0.017%
46	15.122	2042	2046	2050	rVB4	6539	9588	0.19%	0.019%
47	15.228	2059	2064	2068	rVB	107129	131650	2.56%	0.254%
48	15.322	2077	2080	2081	rBV3	5028	5571	0.11%	0.011%
49	15.363	2081	2087	2099	rVV	2847791	4113937	79.95%	7.951%
50	15.492	2103	2109	2118	rVB	103746	172534	3.35%	0.333%
51	15.628	2124	2132	2138	rBV2	63734	124359	2.42%	0.240%
52	15.722	2147	2148	2154	rVB6	8839	11714	0.23%	0.023%
53	15.780	2155	2158	2164	rBV8	11003	21097	0.41%	0.041%
54	15.845	2166	2169	2173	rVB6	14249	18433	0.36%	0.036%
55	15.963	2186	2189	2192	rVB4	6643	8079	0.16%	0.016%
56	16.092	2206	2211	2212	rBV	127838	160055	3.11%	0.309%
57	16.151	2219	2221	2227	rVB6	18221	23111	0.45%	0.045%
58	16.204	2227	2230	2234	rBV4	10790	18741	0.36%	0.036%
59	16.427	2265	2268	2272	rBV3	12792	21458	0.42%	0.041%
60	16.492	2276	2279	2283	rVB5	11359	16274	0.32%	0.031%
61	16.598	2293	2297	2300	rBV2	13606	16195	0.31%	0.031%
62	16.639	2302	2304	2306	rVV3	6507	6272	0.12%	0.012%
63	16.663	2306	2308	2311	rVV4	12960	15367	0.30%	0.030%
64	16.692	2311	2313	2316	rVB4	7310	7400	0.14%	0.014%
65	16.886	2341	2346	2350	rBV	107823	143465	2.79%	0.277%
66	16.933	2350	2354	2358	rVB	55647	78599	1.53%	0.152%
67	17.116	2379	2385	2395	rBV	2303453	3313928	64.40%	6.404%
68	17.216	2395	2402	2414	rVV2	3026744	4405645	85.62%	8.514%
69	17.416	2433	2436	2441	rVB3	22443	33574	0.65%	0.065%
70	17.474	2444	2446	2449	rBV4	7314	10053	0.20%	0.019%
71	17.622	2467	2471	2475	rBV	109036	128168	2.49%	0.248%
72	18.021	2534	2539	2544	rBV3	44898	70163	1.36%	0.136%
73	18.321	2585	2590	2596	rBV	96485	125362	2.44%	0.242%
74	18.957	2694	2698	2704	rVB	101047	122755	2.39%	0.237%
75	19.074	2714	2718	2722	rVB	43461	57696	1.12%	0.112%
76	19.145	2727	2730	2734	rVV	34592	47920	0.93%	0.093%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
 Data File : BM044530.D
 Acq On : 06 Mar 2024 23:44
 Operator : MA/JU
 Sample : P1676-07
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E06Y6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Title : SVOA CALIBRATION

77	19.186	2734	2737	2746	rVB4	32023	57424	1.12%	0.111%
78	19.304	2755	2757	2760	rVB3	14663	11816	0.23%	0.023%
79	19.510	2786	2792	2800	rBV	3732250	5145460	100.00%	9.944%
80	19.574	2800	2803	2810	rVB3	46471	65393	1.27%	0.126%
81	20.074	2884	2888	2892	rVB	155204	168781	3.28%	0.326%
82	20.568	2969	2972	2976	rBV	173866	190188	3.70%	0.368%
83	21.033	3046	3051	3060	rBV	508190	761839	14.81%	1.472%
84	21.304	3092	3097	3105	rBV	2402832	3079571	59.85%	5.952%
85	21.474	3122	3126	3131	rBV	206363	244724	4.76%	0.473%
86	21.909	3197	3200	3207	rBV	182739	228088	4.43%	0.441%
87	22.380	3277	3280	3287	rVB2	186084	244336	4.75%	0.472%
88	22.898	3364	3368	3373	rVB	162477	222971	4.33%	0.431%
89	23.409	3448	3455	3462	rBV2	2020776	3854141	74.90%	7.449%
90	23.551	3473	3479	3491	rVB	1449313	2801659	54.45%	5.414%



Sum of corrected areas: 51743762

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044530.D
Acq On : 06 Mar 2024 23:44
Operator : MA/JU
Sample : P1676-07
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E06Y6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

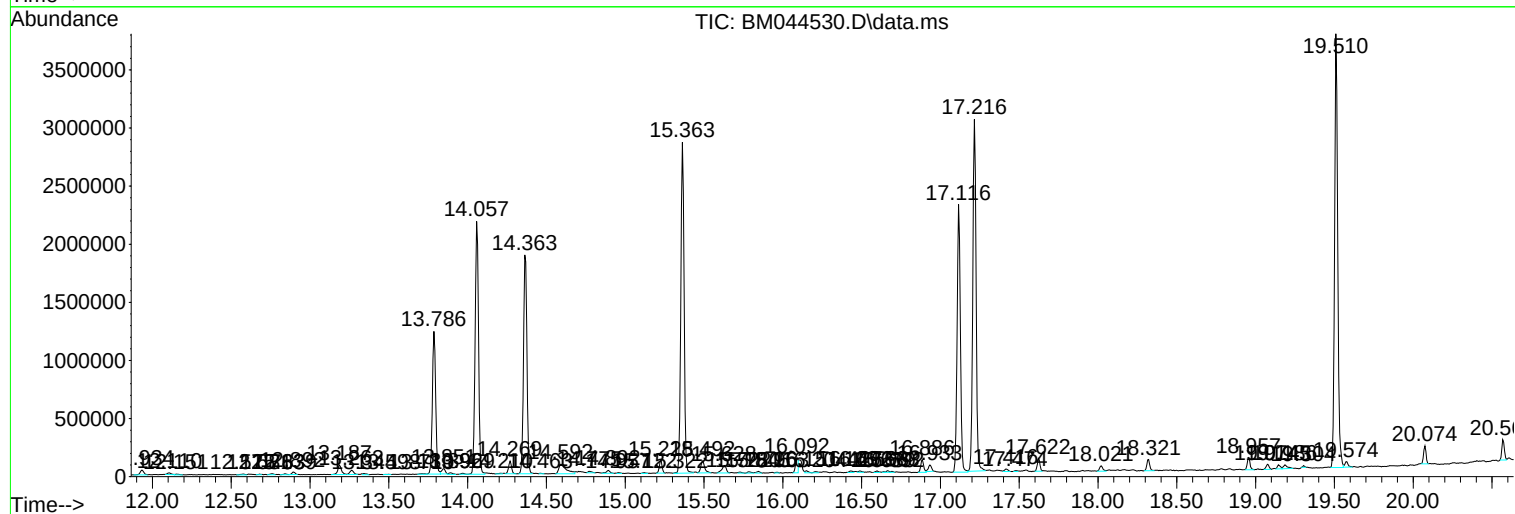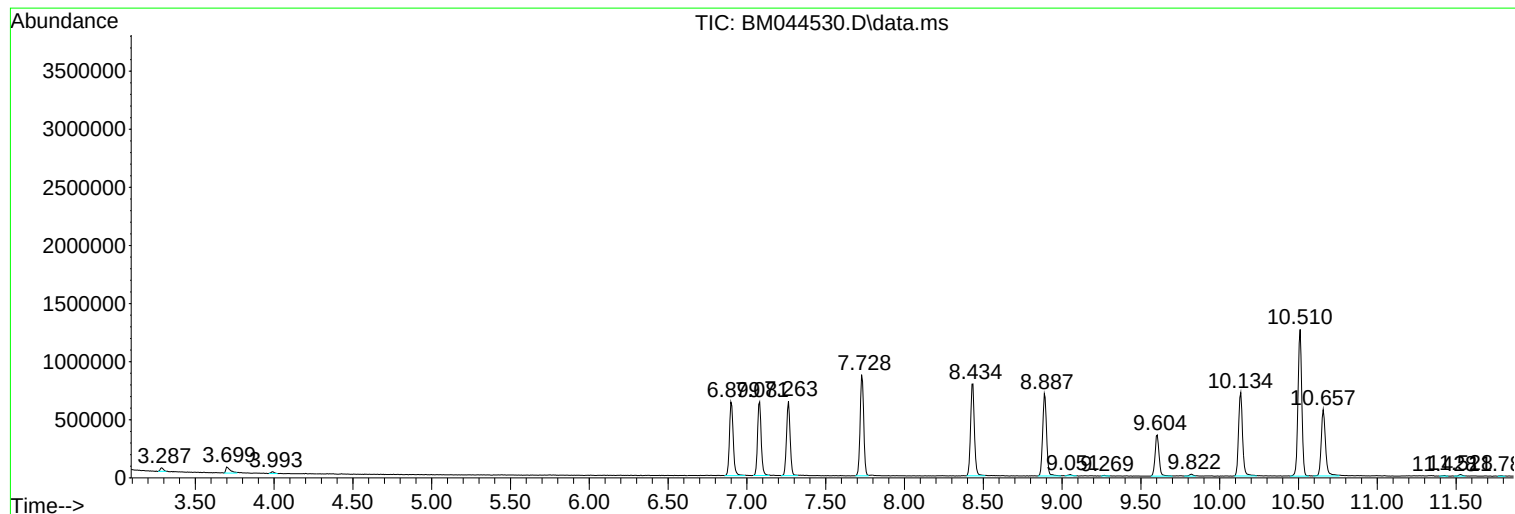

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044530.D
Acq On : 06 Mar 2024 23:44
Operator : MA/JU
Sample : P1676-07
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E06Y6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1-Dodecanol, 2-hexyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.033	4.95 ng/ul	761839	Chrysene-d12	21.304

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Dodecanol, 2-hexyl-			270	C18H38O	110225-00-8	91
2	Carbonic acid, octadecyl prop-1-...			354	C22H42O3	1000383-11-5	90
3	Oxalic acid, isobutyl hexadecyl ...			370	C22H42O4	1000309-38-1	81
4	Pentadecafluorooctanoic acid, oc...			666	C26H37F15O2	1000406-04-8	76
5	Carbonic acid, eicosyl vinyl ester			368	C23H44O3	1000382-54-3	74

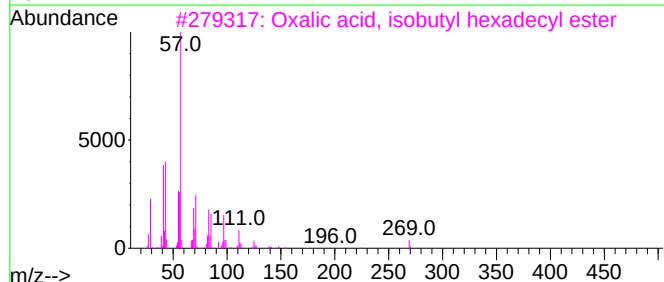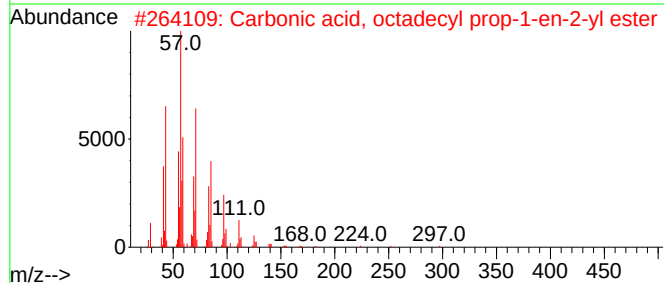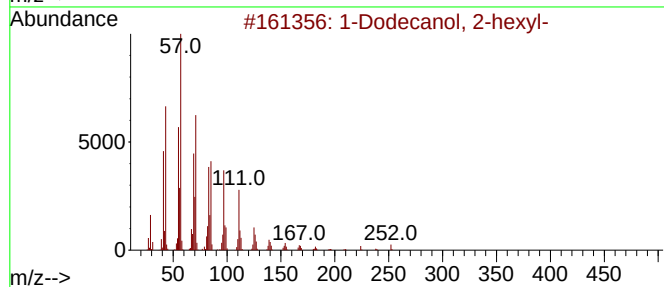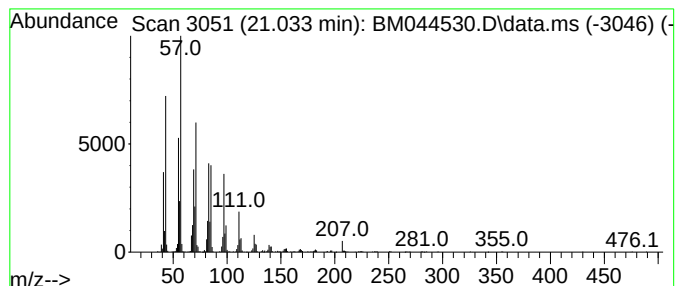

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044530.D
Acq On : 06 Mar 2024 23:44
Operator : MA/JU
Sample : P1676-07
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E06Y6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Dodecanol, 2-...	21.033	5.0	ng/ul	761839	5	21.304	3079570	20.0