

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
 Data File : BM044538.D
 Acq On : 07 Mar 2024 05:07
 Operator : MA/JU
 Sample : PB159484BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK484

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044538.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	30	34	43	rVB	71772	104628	1.80%	0.167%
2	3.681	98	101	127	rBV	885865	1458423	25.11%	2.321%
3	3.993	151	154	161	rVB	15299	20452	0.35%	0.033%
4	6.898	641	648	665	rBV	1040933	1663518	28.64%	2.647%
5	7.075	671	678	691	rBV	897010	1455501	25.06%	2.316%
6	7.263	702	710	723	rBV	1021900	1647634	28.36%	2.622%
7	7.728	782	789	796	rBV	897504	1422843	24.49%	2.264%
8	8.428	901	908	921	rBV	1272472	2068952	35.62%	3.292%
9	8.887	978	986	997	rBV	983720	1668786	28.73%	2.656%
10	9.045	1010	1013	1018	rVB7	5940	9626	0.17%	0.015%
11	9.598	1098	1107	1120	rBV	805112	1383364	23.81%	2.201%
12	10.128	1190	1197	1213	rBV	1152002	2024357	34.85%	3.222%
13	10.510	1253	1262	1273	rBV	1245665	2161783	37.21%	3.440%
14	10.657	1279	1287	1312	rBV	1229028	2275337	39.17%	3.621%
15	12.110	1527	1534	1539	rBV	20160	36496	0.63%	0.058%
16	12.322	1565	1570	1574	rVB7	3917	5943	0.10%	0.009%
17	13.263	1723	1730	1735	rBV2	31211	51713	0.89%	0.082%
18	13.786	1812	1819	1831	rBV	2348164	3299260	56.79%	5.250%
19	14.057	1857	1865	1875	rBV	2725128	3959979	68.17%	6.302%
20	14.363	1906	1917	1929	rBV	2021617	2990431	51.48%	4.759%
21	14.574	1946	1953	1986	rBV	657512	1565308	26.95%	2.491%
22	15.363	2080	2087	2095	rBV	3383312	4868800	83.81%	7.748%
23	15.486	2102	2108	2124	rBV	1096944	1575900	27.13%	2.508%
24	15.604	2124	2128	2133	rVB6	15345	23992	0.41%	0.038%
25	16.145	2216	2220	2225	rBV4	10716	15336	0.26%	0.024%
26	16.798	2327	2331	2334	rVB6	4259	6246	0.11%	0.010%
27	16.904	2345	2349	2352	rBV5	4814	6272	0.11%	0.010%
28	17.115	2378	2385	2395	rBV	2421825	3478391	59.88%	5.535%
29	17.215	2395	2402	2418	rVV	3617002	5230510	90.04%	8.324%
30	18.021	2534	2539	2544	rBV5	20030	38784	0.67%	0.062%
31	19.074	2713	2718	2723	rBV2	44565	60906	1.05%	0.097%
32	19.145	2726	2730	2736	rBV	39048	54273	0.93%	0.086%
33	19.309	2754	2758	2762	rBV4	22894	37114	0.64%	0.059%
34	19.509	2786	2792	2802	rBV	4299153	5809146	100.00%	9.245%
35	21.303	3091	3097	3108	rBV	2324664	3163693	54.46%	5.035%
36	23.403	3447	3454	3463	rBV2	2206550	4435711	76.36%	7.059%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044538.D
Acq On : 07 Mar 2024 05:07
Operator : MA/JU
Sample : PB159484BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK484

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Title : SVOA CALIBRATION

37	23.550	3472	3479	3491	rVB	1406764	2758946	47.49%	4.391%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 62838354

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044538.D
Acq On : 07 Mar 2024 05:07
Operator : MA/JU
Sample : PB159484BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK484

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

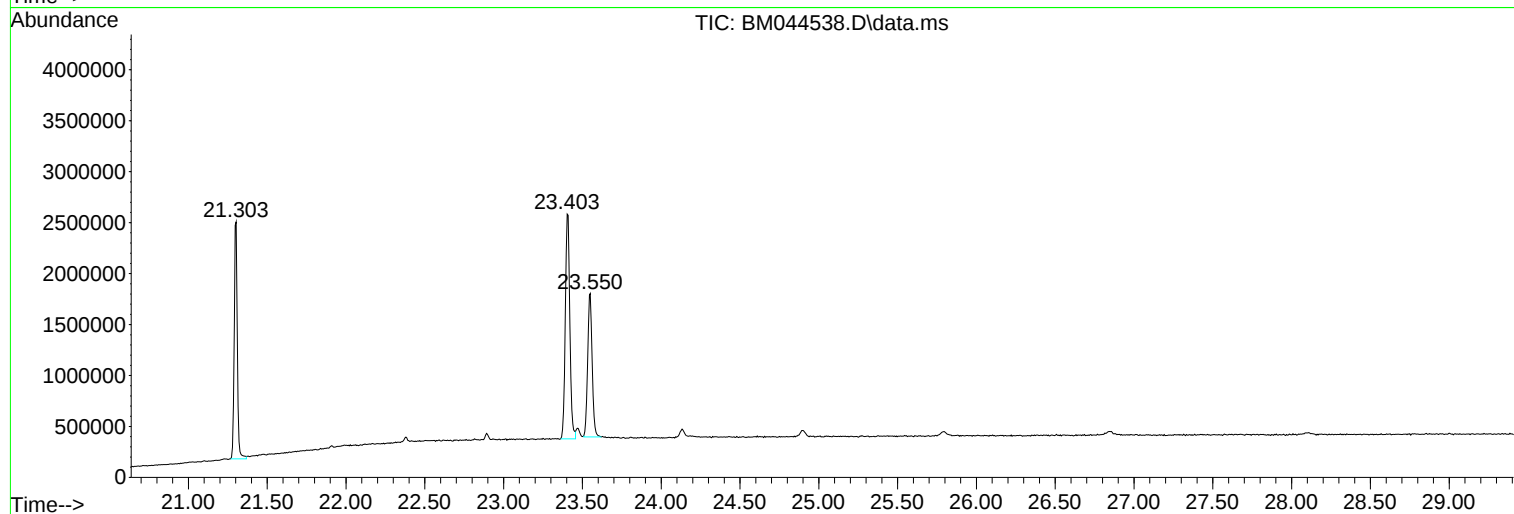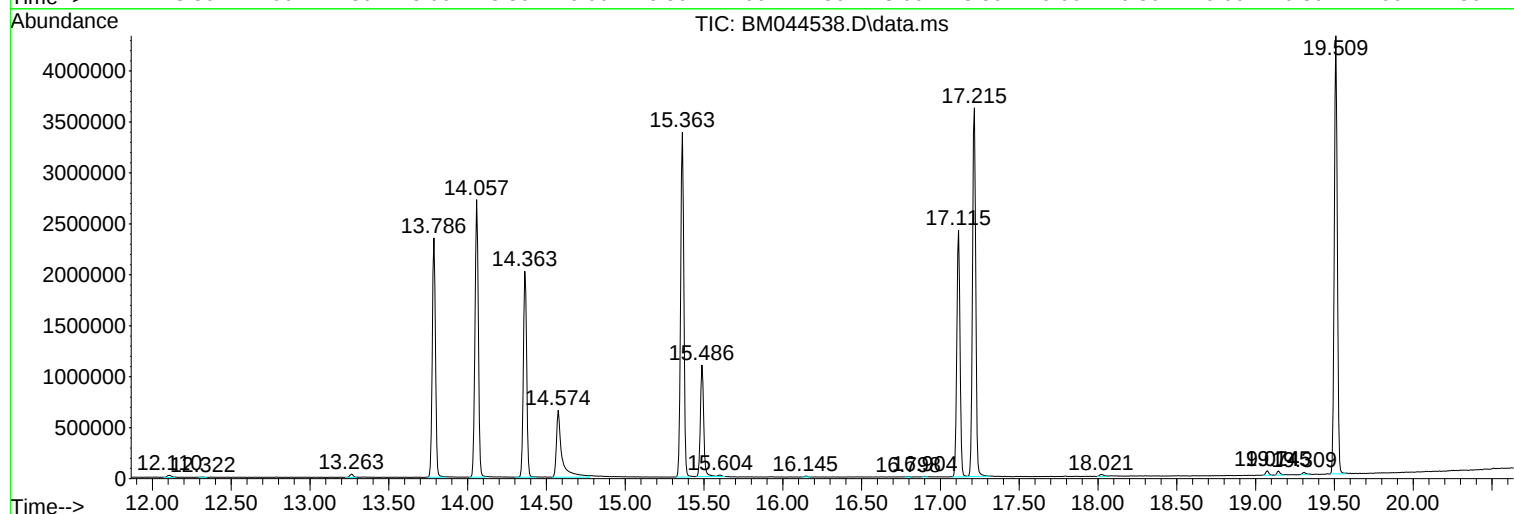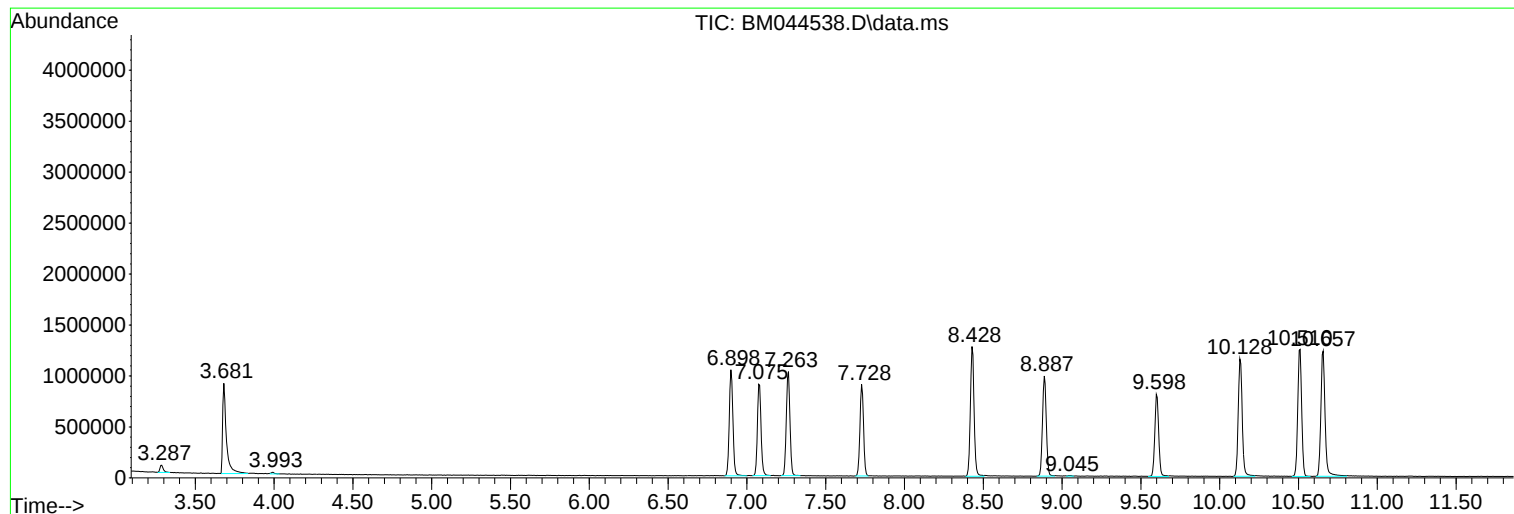

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044538.D
Acq On : 07 Mar 2024 05:07
Operator : MA/JU
Sample : PB159484BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK484

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044538.D
Acq On : 07 Mar 2024 05:07
Operator : MA/JU
Sample : PB159484BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK484

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------