

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
 Data File : BM044545.D
 Acq On : 07 Mar 2024 09:19
 Operator : MA/JU
 Sample : P1679-02
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0704

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044545.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	30	33	43	rVB	74557	108489	1.44%	0.156%
2	3.687	99	102	120	rBV	270560	494189	6.55%	0.709%
3	3.993	150	154	157	rBV	20208	24777	0.33%	0.036%
4	4.446	229	231	237	rVB6	7410	10376	0.14%	0.015%
5	6.898	641	648	658	rBV	281491	463249	6.14%	0.665%
6	7.075	670	678	690	rBV	1206278	1953077	25.88%	2.803%
7	7.263	703	710	720	rBV	986406	1614411	21.39%	2.317%
8	7.339	720	723	726	rVB5	8996	10340	0.14%	0.015%
9	7.728	782	789	797	rBV	859874	1355986	17.97%	1.946%
10	8.428	901	908	920	rBV	776016	1259628	16.69%	1.808%
11	8.622	935	941	948	rVB2	9141	14839	0.20%	0.021%
12	8.886	978	986	998	rBV	1357703	2257172	29.91%	3.240%
13	8.992	1000	1004	1008	rVV2	19377	35656	0.47%	0.051%
14	9.045	1008	1013	1024	rVB2	56605	97590	1.29%	0.140%
15	9.598	1100	1107	1116	rBV	1057111	1739721	23.05%	2.497%
16	10.128	1189	1197	1207	rBV	1457023	2443165	32.37%	3.507%
17	10.504	1254	1261	1270	rBV	1202146	2059143	27.28%	2.955%
18	10.651	1278	1286	1302	rBV	1464169	2609925	34.58%	3.746%
19	11.316	1396	1399	1405	rBV7	7982	17572	0.23%	0.025%
20	11.751	1468	1473	1477	rBV3	7650	12138	0.16%	0.017%
21	12.051	1516	1524	1528	rBV10	5854	15796	0.21%	0.023%
22	12.104	1528	1533	1539	rVB2	30123	52506	0.70%	0.075%
23	12.721	1632	1638	1644	rVB7	5167	11650	0.15%	0.017%
24	12.969	1676	1680	1685	rBV7	5945	9424	0.12%	0.014%
25	13.263	1725	1730	1736	rBV5	11702	20265	0.27%	0.029%
26	13.333	1738	1742	1746	rBV6	6434	9568	0.13%	0.014%
27	13.786	1810	1819	1831	rBV	3264039	4502249	59.65%	6.462%
28	14.057	1857	1865	1881	rBV	3635428	5485246	72.68%	7.873%
29	14.363	1910	1917	1925	rBV	1906335	2778913	36.82%	3.989%
30	14.586	1948	1955	1970	rBV3	78241	257925	3.42%	0.370%
31	14.798	1985	1991	2002	rVB3	15793	43335	0.57%	0.062%
32	15.057	2031	2035	2039	rVB4	7477	10062	0.13%	0.014%
33	15.168	2050	2054	2066	rVB2	22555	39883	0.53%	0.057%
34	15.362	2079	2087	2099	rBV	4663630	6795448	90.03%	9.754%
35	15.486	2102	2108	2124	rVV	1369573	1963966	26.02%	2.819%
36	15.598	2124	2127	2137	rVB3	25036	51317	0.68%	0.074%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044545.D
Acq On : 07 Mar 2024 09:19
Operator : MA/JU
Sample : P1679-02
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0704

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Title : SVOA CALIBRATION

37	16.086	2206	2210	2217	rVB4	8307	14693	0.19%	0.021%
38	16.145	2217	2220	2224	rVB2	14323	19601	0.26%	0.028%
39	16.792	2327	2330	2333	rBV5	7695	8223	0.11%	0.012%
40	16.904	2343	2349	2354	rVB5	5533	10381	0.14%	0.015%
41	17.115	2378	2385	2395	rBV	2183301	3109240	41.20%	4.463%
42	17.215	2395	2402	2415	rVV	4981558	7199213	95.38%	10.333%
43	17.415	2432	2436	2440	rVB4	6715	10524	0.14%	0.015%
44	17.509	2448	2452	2458	rVB8	4603	7885	0.10%	0.011%
45	17.792	2496	2500	2506	rBV8	8080	13172	0.17%	0.019%
46	17.956	2524	2528	2533	rBV6	8346	12913	0.17%	0.019%
47	18.015	2533	2538	2546	rBV	144206	228024	3.02%	0.327%
48	18.092	2549	2551	2557	rVB3	16964	22652	0.30%	0.033%
49	18.456	2609	2613	2616	rVB6	9435	11829	0.16%	0.017%
50	18.880	2682	2685	2690	rBV6	9749	12600	0.17%	0.018%
51	19.003	2703	2706	2713	rBV5	11872	21857	0.29%	0.031%
52	19.074	2713	2718	2723	rBV	58272	82597	1.09%	0.119%
53	19.145	2726	2730	2736	rBV	45601	73155	0.97%	0.105%
54	19.303	2753	2757	2767	rBV2	113520	183800	2.44%	0.264%
55	19.509	2786	2792	2803	rBV	5609247	7547586	100.00%	10.833%
56	21.297	3091	3096	3104	rBV	1949073	2531868	33.55%	3.634%
57	23.403	3447	3454	3463	rBV2	2977821	5635011	74.66%	8.088%
58	23.544	3472	3478	3491	rVB	1167619	2286049	30.29%	3.281%




Sum of corrected areas: 69671869

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044545.D
Acq On : 07 Mar 2024 09:19
Operator : MA/JU
Sample : P1679-02
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0704

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

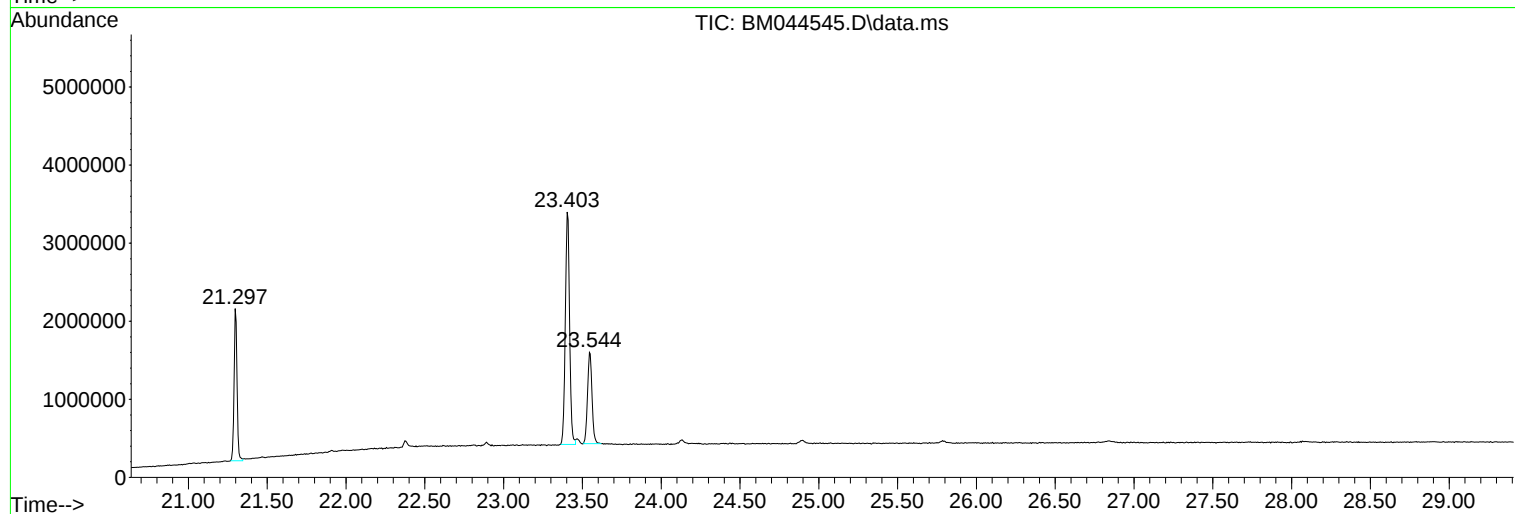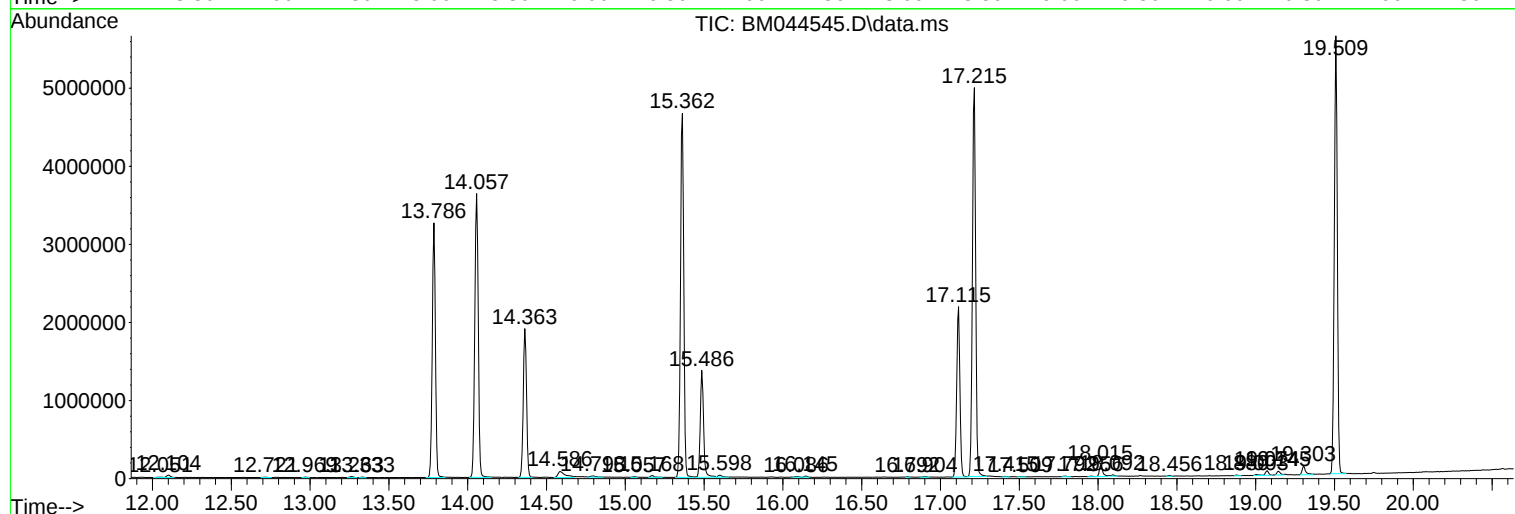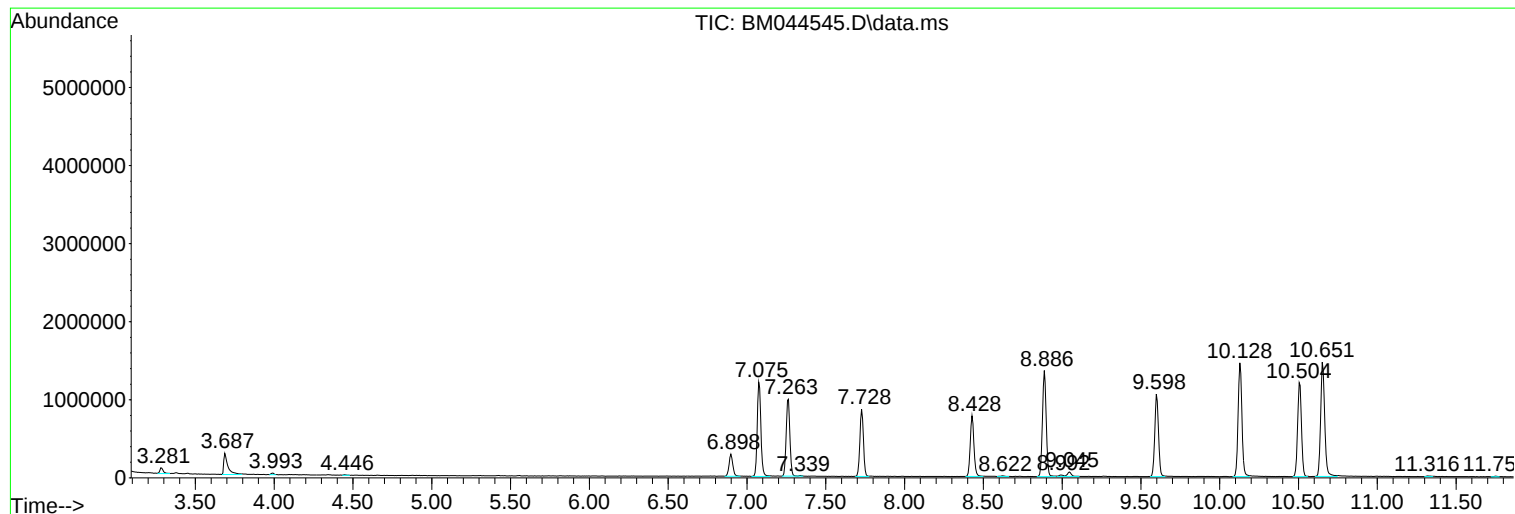

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044545.D
Acq On : 07 Mar 2024 09:19
Operator : MA/JU
Sample : P1679-02
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0704

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044545.D
Acq On : 07 Mar 2024 09:19
Operator : MA/JU
Sample : P1679-02
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0704

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------