

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
 Data File : BM044549.D
 Acq On : 07 Mar 2024 14:00
 Operator : MA/JU
 Sample : PB159425BL
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK425

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044549.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	42	rVB	77854	117700	1.80%	0.172%
2	3.669	96	99	120	rBV	911966	1567004	23.98%	2.292%
3	3.981	148	152	156	rVB3	12793	19085	0.29%	0.028%
4	6.892	640	647	658	rBV	1132596	1808619	27.68%	2.645%
5	7.069	670	677	696	rVB	987125	1570514	24.04%	2.297%
6	7.251	701	708	717	rBV	1101597	1768100	27.06%	2.586%
7	7.722	781	788	797	rBV	854833	1337259	20.47%	1.956%
8	8.422	900	907	920	rBV	1406179	2249731	34.43%	3.290%
9	8.881	977	985	994	rBV	1098251	1810018	27.70%	2.647%
10	9.592	1099	1106	1117	rBV	885913	1499238	22.95%	2.193%
11	10.122	1189	1196	1218	rBV	1296083	2231876	34.16%	3.264%
12	10.504	1253	1261	1269	rBV	1218477	2036311	31.17%	2.978%
13	10.651	1278	1286	1305	rBV	1408366	2521586	38.59%	3.688%
14	12.104	1527	1533	1541	rBV	21490	41346	0.63%	0.060%
15	13.263	1724	1730	1739	rVB4	13366	24386	0.37%	0.036%
16	13.786	1812	1819	1833	rBV	2437076	3434742	52.57%	5.023%
17	14.057	1858	1865	1877	rBV	2876265	4205628	64.37%	6.151%
18	14.363	1911	1917	1925	rBV	1883720	2805031	42.93%	4.102%
19	14.574	1946	1953	1973	rBV	1139424	1824288	27.92%	2.668%
20	15.362	2078	2087	2096	rBV	3547471	5172179	79.16%	7.564%
21	15.492	2102	2109	2122	rBV	1167124	1679722	25.71%	2.457%
22	15.604	2124	2128	2134	rVB4	14906	23258	0.36%	0.034%
23	16.151	2217	2221	2225	rVB5	11312	13995	0.21%	0.020%
24	16.804	2328	2332	2337	rBV7	6199	9595	0.15%	0.014%
25	17.121	2379	2386	2395	rBV	2374469	3353994	51.33%	4.905%
26	17.221	2396	2403	2415	rVV2	3801059	5596386	85.65%	8.185%
27	18.033	2537	2541	2546	rBV7	10233	15011	0.23%	0.022%
28	19.080	2715	2719	2725	rBV	48459	65940	1.01%	0.096%
29	19.150	2727	2731	2740	rBV	43631	64672	0.99%	0.095%
30	19.315	2757	2759	2763	rBV5	9118	14223	0.22%	0.021%
31	19.521	2787	2794	2802	rBV	4708213	6533743	100.00%	9.555%
32	21.315	3094	3099	3107	rBV	2824079	3532102	54.06%	5.166%
33	23.427	3451	3458	3467	rBV2	3206535	6037564	92.41%	8.830%
34	23.574	3476	3483	3493	rVB	1771168	3392761	51.93%	4.962%

Sum of corrected areas: 68377607

Instrument :

BNA_M

ClientSampleId :




SBLK425

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044549.D
Acq On : 07 Mar 2024 14:00
Operator : MA/JU
Sample : PB159425BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

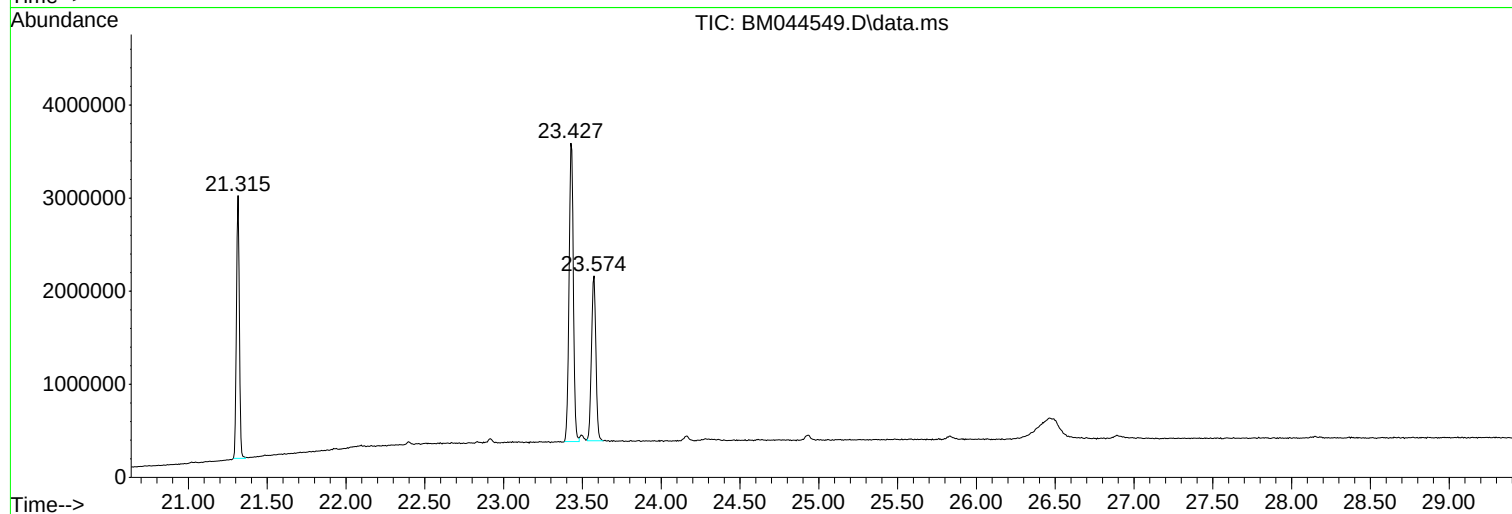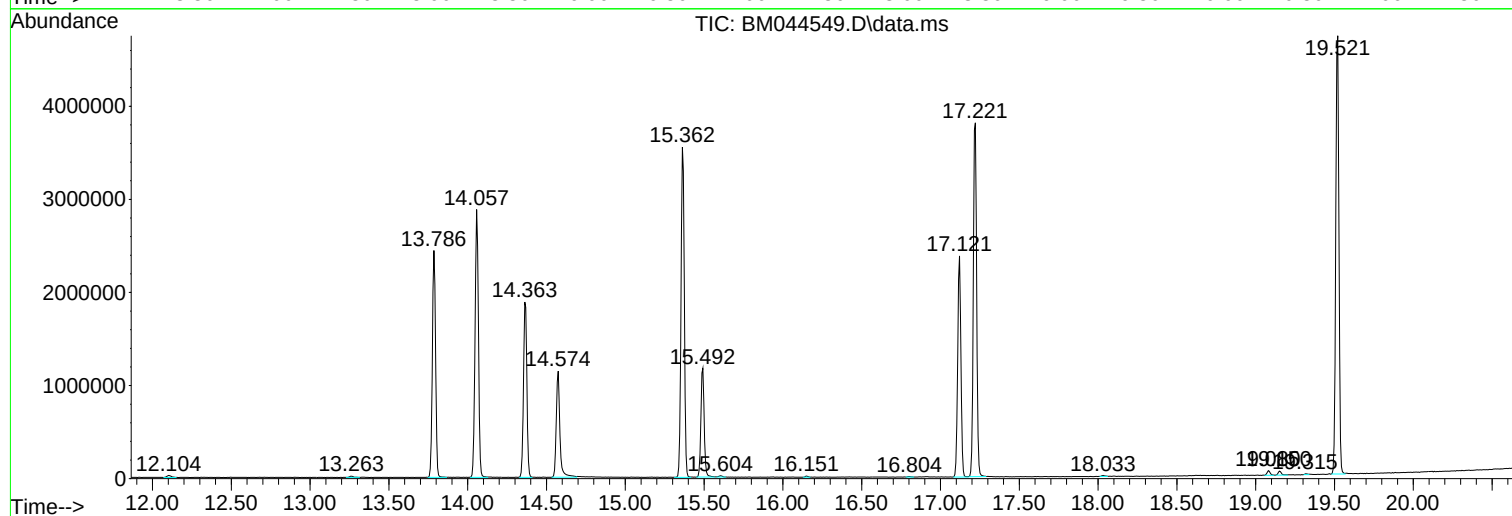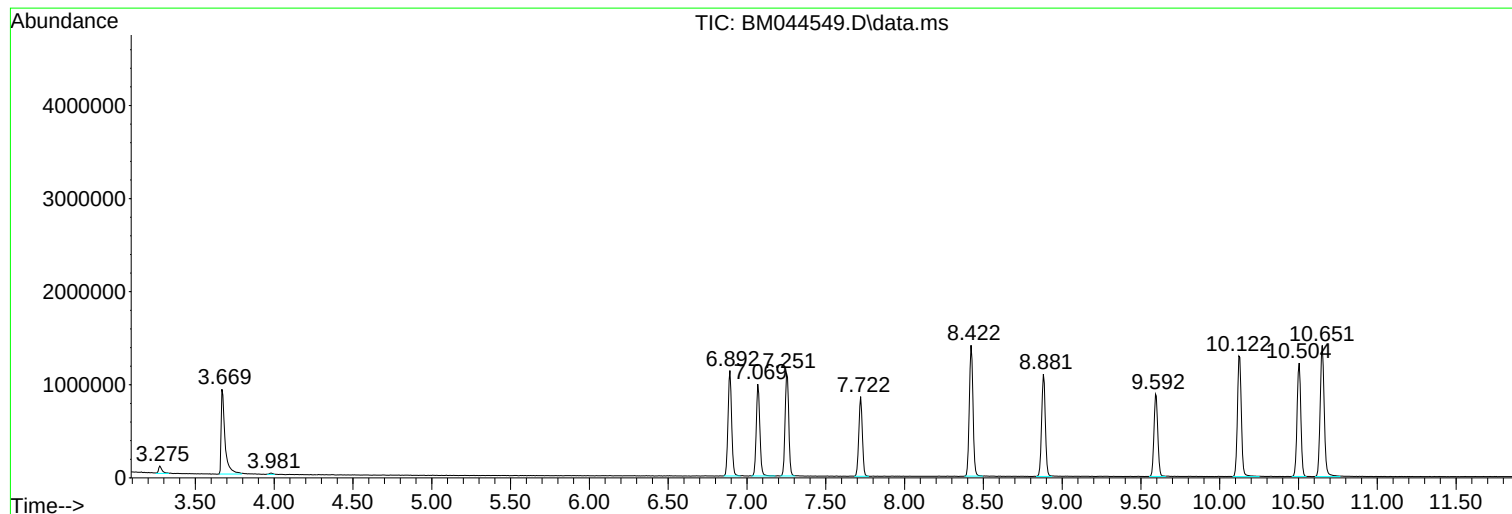

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044549.D
Acq On : 07 Mar 2024 14:00
Operator : MA/JU
Sample : PB159425BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030624\
Data File : BM044549.D
Acq On : 07 Mar 2024 14:00
Operator : MA/JU
Sample : PB159425BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc