

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030717\
 Data File : BM009101.D
 Acq On : 07 Mar 2017 18:14
 Operator : SJ/MA
 Sample : I2064-11
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AE2

Quant Time: Mar 08 03:13:43 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 08 03:12:37 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	141	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	406	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	249	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.36	188	36411	0.40	ng/ul	0.09
16) Chrysene-d12	21.45	240	563	0.40	ng/ul	0.00
20) Perylene-d12	23.63	264	35278	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	159	0.24	ng/ul	0.00
14) Fluoranthene-d10	19.30	212	425	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.66	202	95	0.05	ng/ul#	Qvalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030717\
Data File : BM009101.D
Acq On : 07 Mar 2017 18:14
Operator : SJ/MA
Sample : I2064-11
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE2

Quant Time: Mar 08 03:13:43 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 08 03:12:37 2017
Response via : Initial Calibration

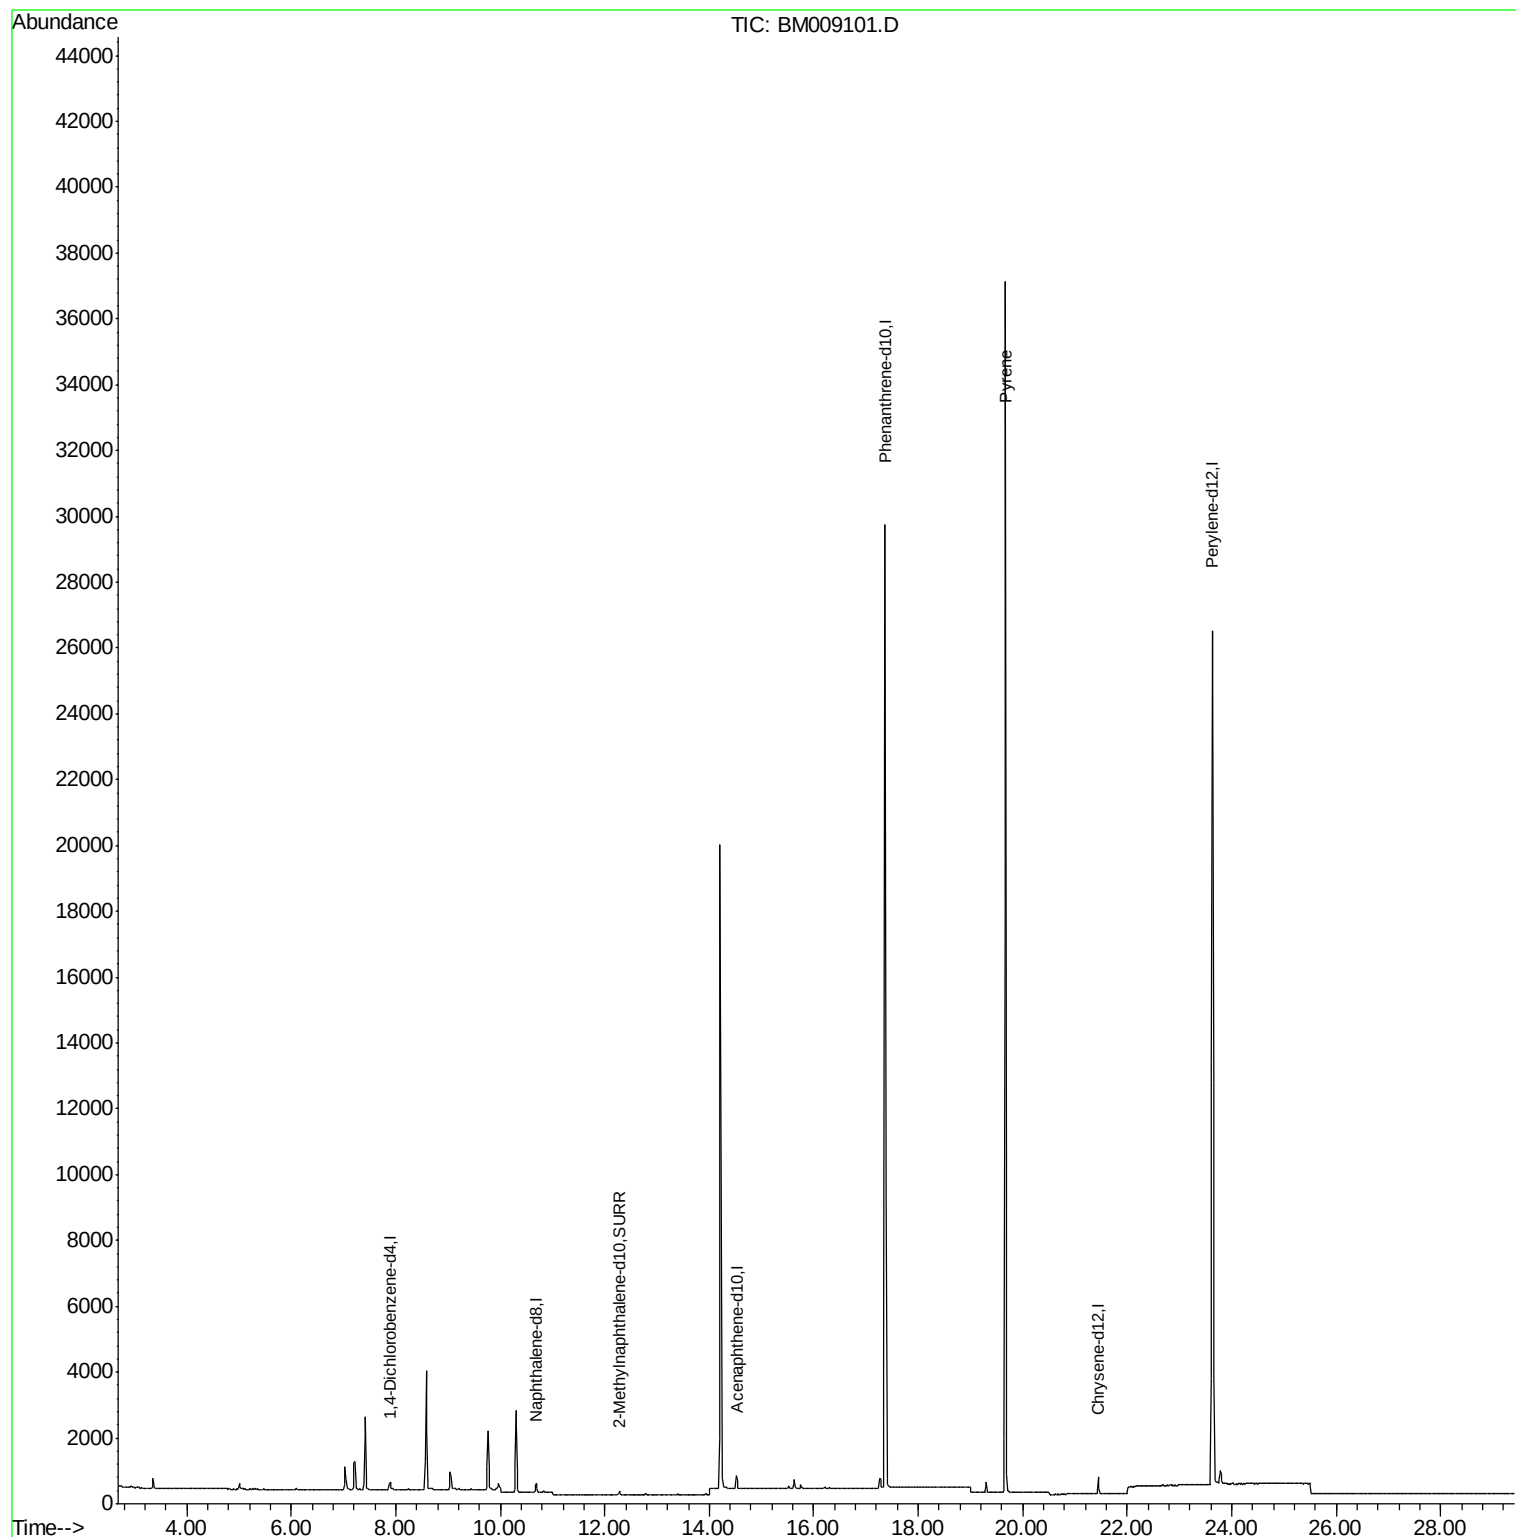

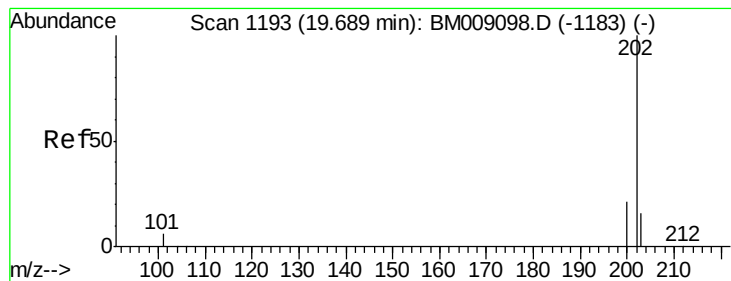

#17

Pyrene

Concen: 0.05 ng/ul

RT: 19.66 min Scan# 1191

Delta R.T. -0.02 min

Lab File: BM009101.D


Acq: 07 Mar 2017 18:14

Instrument :

BNA_M

ClientSampleId :

C0AE2

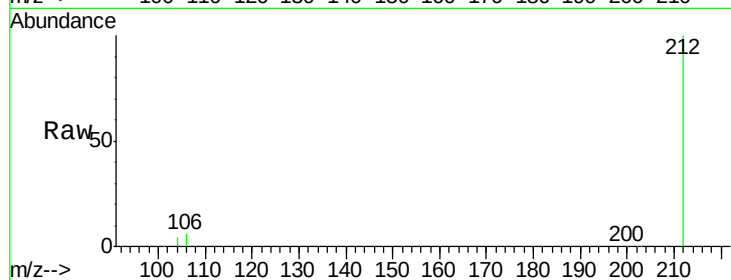

Tgt Ion	Ratio	Lower	Upper
202	100		
200	47.5	18.2	27.4#
203	156.4	15.6	23.4#

