

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030717\
 Data File : BM009103.D
 Acq On : 07 Mar 2017 19:27
 Operator : SJ/MA
 Sample : I2064-13
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AL4

Quant Time: Mar 08 03:13:51 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 08 03:12:37 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	135	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	398	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	259	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.36	188	46000	0.40	ng/ul	0.09
16) Chrysene-d12	21.44	240	696	0.40	ng/ul	0.00
20) Perylene-d12	23.63	264	60368	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	177	0.27	ng/ul	0.00
14) Fluoranthene-d10	19.30	212	584	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.66	202	123	0.05	ng/ul#	Qvalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030717\
Data File : BM009103.D
Acq On : 07 Mar 2017 19:27
Operator : SJ/MA
Sample : I2064-13
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AL4

Quant Time: Mar 08 03:13:51 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 08 03:12:37 2017
Response via : Initial Calibration

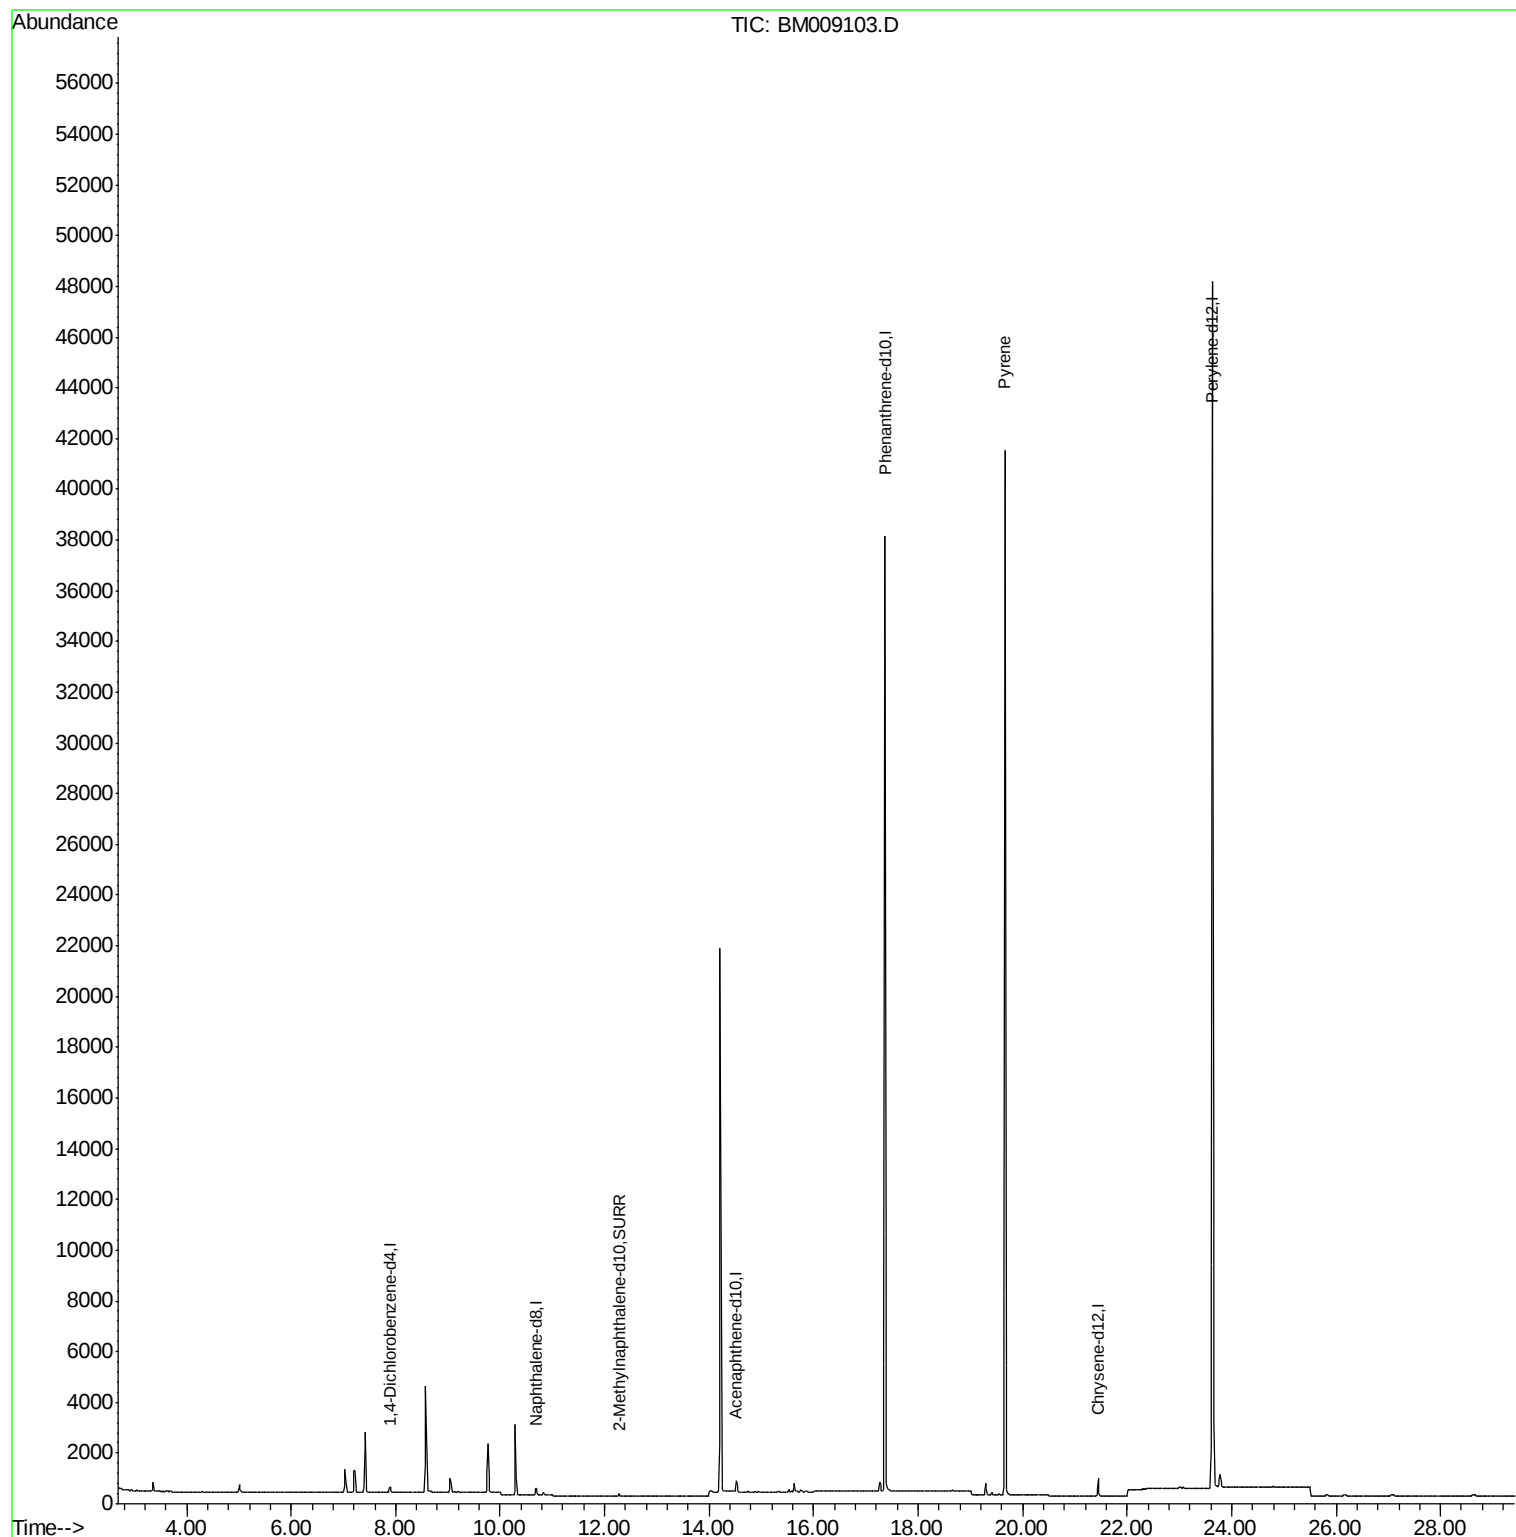


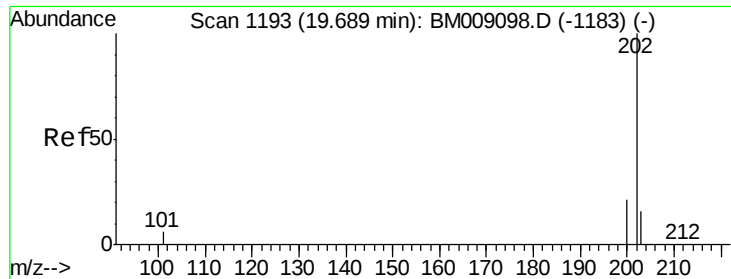

#17
 Pyrene
 Concen: 0.05 ng/ul
 RT: 19.66 min Scan# 1190
 Delta R.T. -0.03 min
 Lab File: BM009103.D
 Acq: 07 Mar 2017 19:27

Instrument :
 BNA_M
 ClientSampleId :
 C0AL4

Tgt Ion	Ratio	Lower	Upper
202	100		
200	41.7	18.2	27.4#
203	122.5	15.6	23.4#

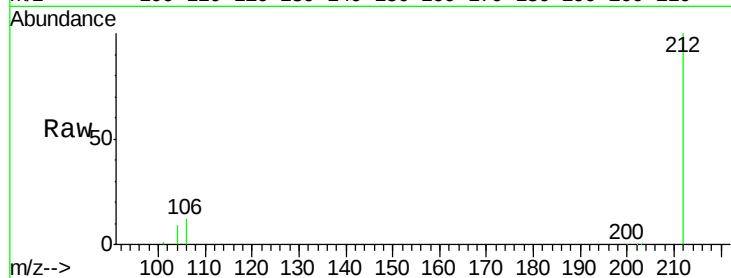

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 200.00 (199.70 to 200.70): E
 Ion 203.00 (202.70 to 203.70): E

