


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA M\Data\BM030718\
 Data File : BM014499.D
 Acq On : 06 Mar 2018 14:21
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM020718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 07 17:16:49 2018

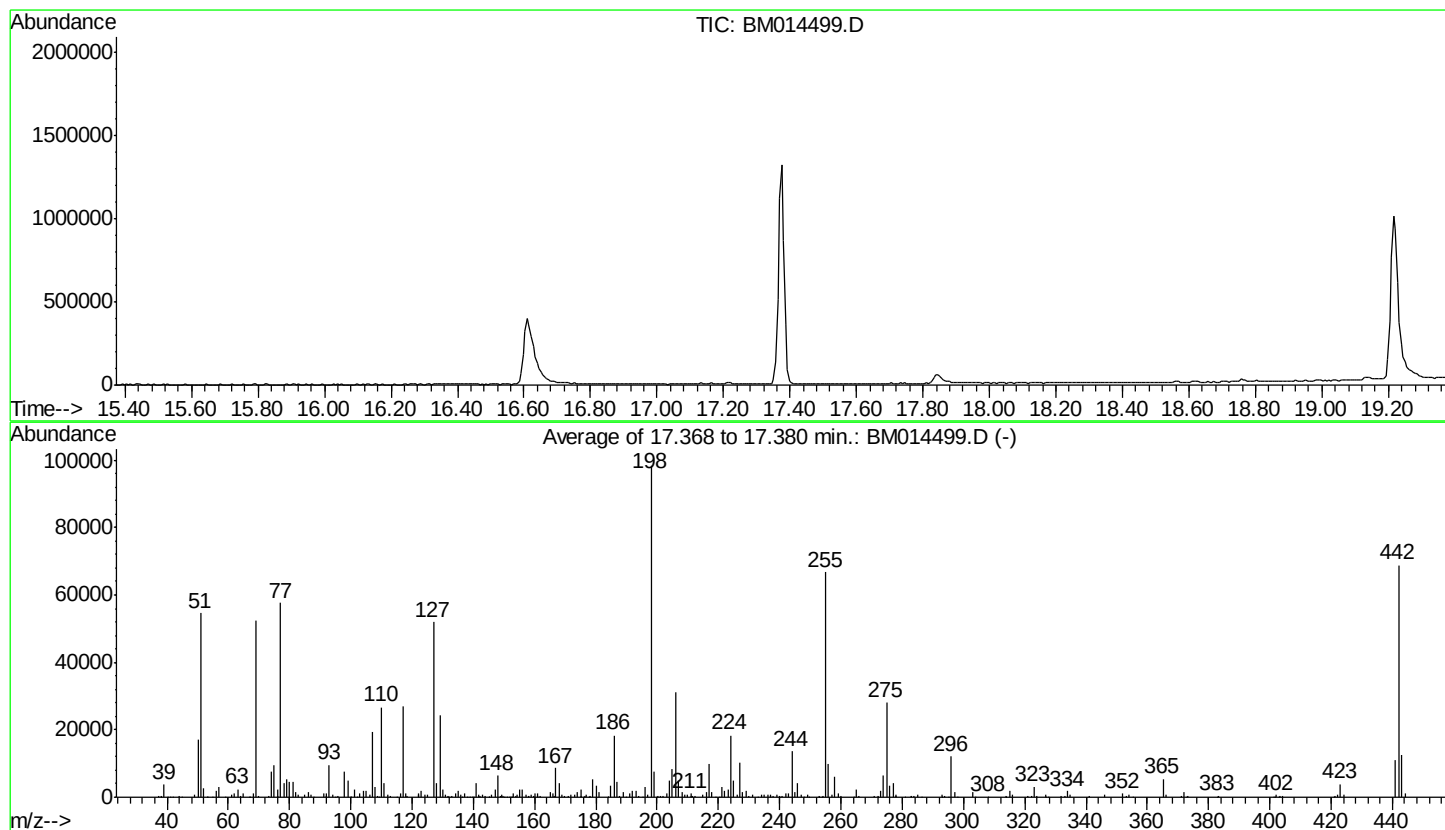

AutoFind: Scans 2445, 2446, 2447; Background Corrected with Scan 2439

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.6	54645	PASS
68	69	0.00	2	2.0	1061	PASS
69	198	0.00	100	53.5	52577	PASS
70	69	0.00	2	0.9	487	PASS
127	198	10	80	52.8	51917	PASS
197	198	0.00	2	0.7	719	PASS
198	198	100	100	100.0	98333	PASS
199	198	5	9	7.6	7489	PASS
275	198	10	60	28.5	28013	PASS
365	198	1	100	5.5	5457	PASS
441	443	0.01	100	88.1	11116	PASS
442	198	50	100	70.0	68786	PASS
443	442	15	24	18.3	12619	PASS