

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
 Data File : BM038873.D
 Acq On : 06 Mar 2023 16:06
 Operator : CG/JU
 Sample : PB151195BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK195

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038873.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	12	16	30	rVB	81595	125234	1.87%	0.176%
2	3.799	84	87	114	rBV	923582	1546962	23.12%	2.173%
3	4.146	142	146	152	rVB2	19198	29472	0.44%	0.041%
4	7.151	649	657	665	rBV	1193185	1853593	27.71%	2.603%
5	7.328	680	687	697	rBV	1015357	1582765	23.66%	2.223%
6	7.528	714	721	734	rBV	1165260	1863293	27.85%	2.617%
7	8.004	794	802	811	rVB	1066883	1653083	24.71%	2.322%
8	8.710	914	922	936	rBV	1436908	2280178	34.08%	3.202%
9	9.169	991	1000	1009	rBV	1119625	1762542	26.35%	2.475%
10	9.898	1115	1124	1136	rBV	781282	1284301	19.20%	1.804%
11	10.433	1207	1215	1227	rBV	1367040	2263674	33.84%	3.179%
12	10.822	1272	1281	1290	rBV	1490709	2476641	37.02%	3.478%
13	10.951	1296	1303	1315	rBV	1516656	2494850	37.29%	3.504%
14	12.404	1544	1550	1555	rBV2	23554	36255	0.54%	0.051%
15	14.051	1824	1830	1845	rBV	2569675	3400487	50.83%	4.776%
16	14.333	1871	1878	1893	rBV	2898189	4125205	61.66%	5.794%
17	14.639	1923	1930	1940	rBV	2332028	3284668	49.10%	4.613%
18	14.815	1954	1960	1984	rBV	1179161	1643098	24.56%	2.308%
19	15.051	1996	2000	2003	rVB6	5851	7763	0.12%	0.011%
20	15.627	2092	2098	2111	rBV	3680165	5184124	77.49%	7.281%
21	15.739	2111	2117	2127	rBV	878220	1177773	17.60%	1.654%
22	15.868	2135	2139	2145	rVB3	16947	22840	0.34%	0.032%
23	17.380	2390	2396	2404	rBV	2693124	3778896	56.48%	5.307%
24	17.480	2407	2413	2431	rVV	4084931	5607099	83.81%	7.875%
25	19.333	2725	2728	2735	rVB4	38772	53285	0.80%	0.075%
26	19.403	2736	2740	2746	rVB2	37244	50706	0.76%	0.071%
27	19.768	2796	2802	2811	rBV	4959673	6496841	97.11%	9.124%
28	21.562	3101	3107	3118	rBV	2972331	3988945	59.62%	5.602%
29	23.856	3489	3497	3507	rBV2	3495680	6690153	100.00%	9.396%
30	24.015	3516	3524	3537	rVB2	2140546	4438558	66.34%	6.234%




Sum of corrected areas: 71203284

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038873.D
Acq On : 06 Mar 2023 16:06
Operator : CG/JU
Sample : PB151195BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK195

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

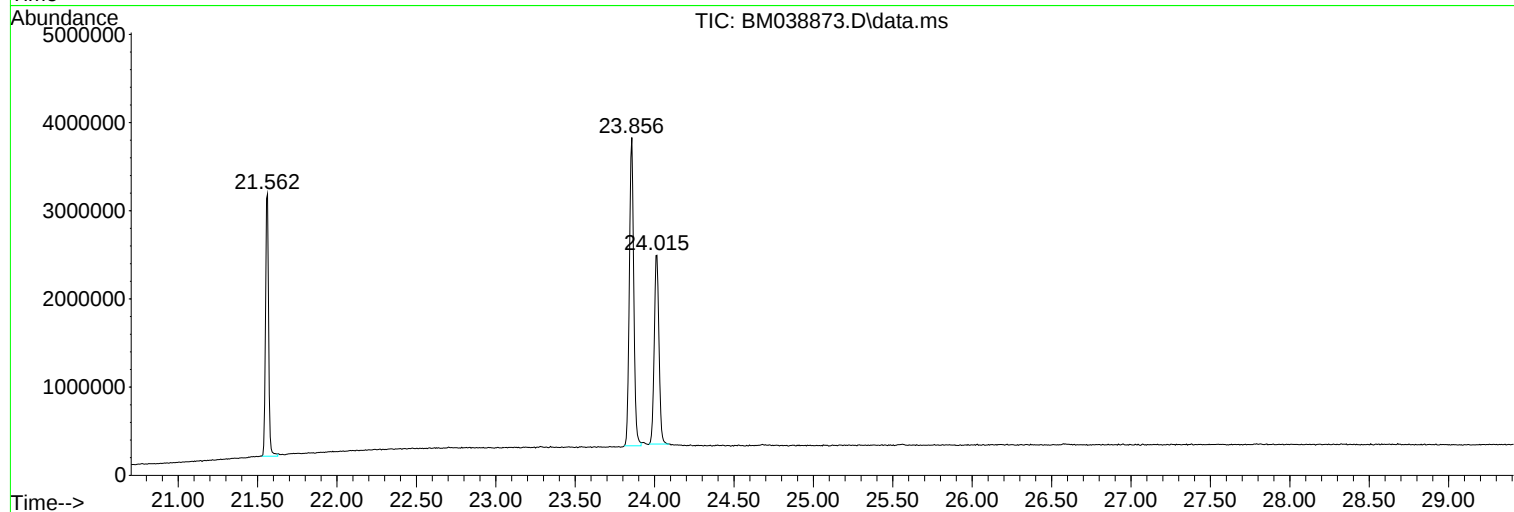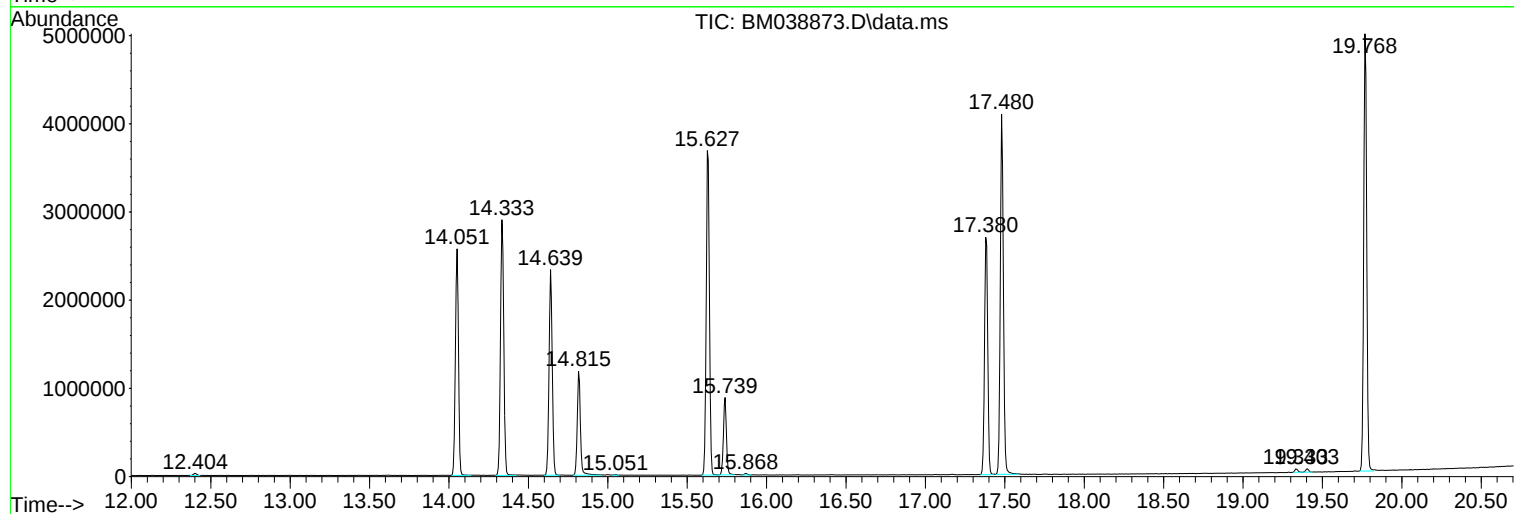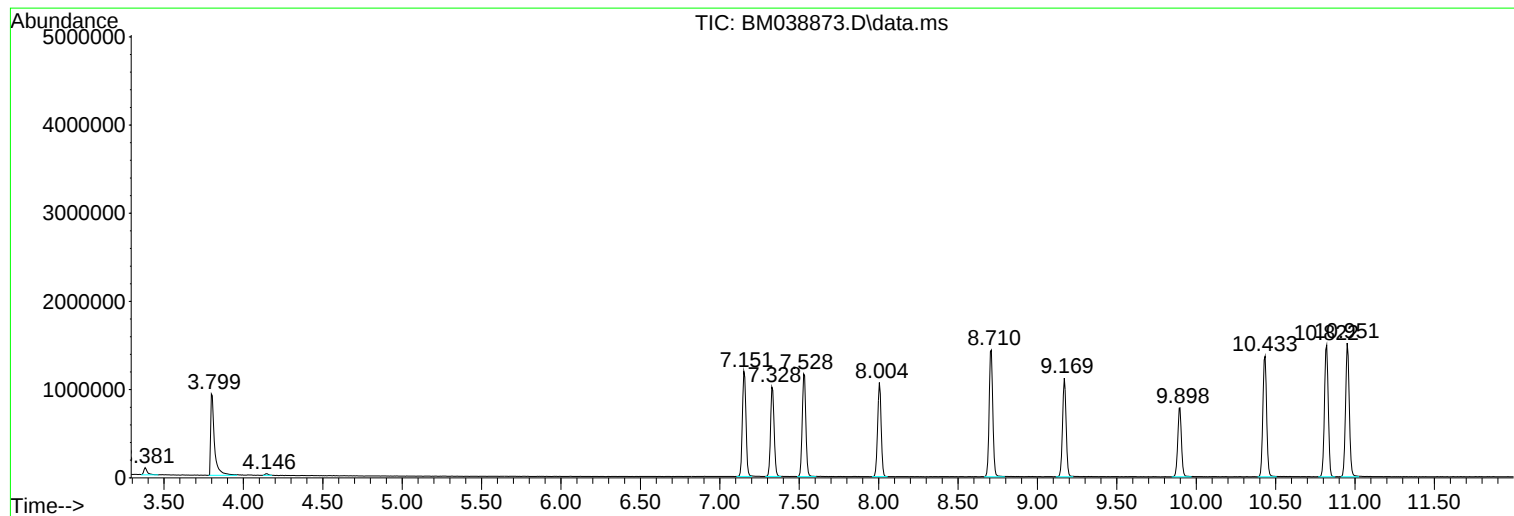

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038873.D
Acq On : 06 Mar 2023 16:06
Operator : CG/JU
Sample : PB151195BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK195

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038873.D
Acq On : 06 Mar 2023 16:06
Operator : CG/JU
Sample : PB151195BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK195

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc