

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
 Data File : BM038874.D
 Acq On : 06 Mar 2023 16:43
 Operator : CG/JU
 Sample : PB151197BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK197

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038874.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	12	16	27	rVB	87247	129061	1.88%	0.172%
2	3.799	85	87	108	rBV	1017377	1629173	23.70%	2.176%
3	4.146	142	146	155	rVB	22749	38464	0.56%	0.051%
4	7.151	650	657	670	rBV	1288089	1959475	28.50%	2.617%
5	7.334	681	688	696	rBV	1069006	1682811	24.48%	2.247%
6	7.528	714	721	731	rBV	1263615	1975388	28.73%	2.638%
7	8.004	795	802	813	rVB	1130703	1753864	25.51%	2.342%
8	8.710	913	922	937	rBV	1517185	2433942	35.40%	3.250%
9	9.169	991	1000	1008	rBV	1209282	1871839	27.23%	2.500%
10	9.898	1115	1124	1135	rBV	837777	1354280	19.70%	1.809%
11	10.434	1206	1215	1225	rBV	1491088	2390990	34.78%	3.193%
12	10.822	1272	1281	1289	rBV	1600292	2611668	37.99%	3.488%
13	10.951	1296	1303	1316	rBV	1619511	2628083	38.23%	3.510%
14	12.398	1544	1549	1556	rBV	25325	42210	0.61%	0.056%
15	14.051	1824	1830	1842	rBV	2741257	3595330	52.29%	4.801%
16	14.333	1872	1878	1893	rBV	3112120	4395578	63.93%	5.870%
17	14.639	1923	1930	1939	rBV	2404699	3457469	50.29%	4.617%
18	14.816	1954	1960	1982	rBV	1211414	1739166	25.30%	2.323%
19	15.051	1997	2000	2005	rVB7	5649	7730	0.11%	0.010%
20	15.627	2091	2098	2109	rBV	3905098	5507077	80.10%	7.354%
21	15.739	2111	2117	2128	rBV	930395	1252451	18.22%	1.673%
22	15.869	2134	2139	2144	rVB2	17890	26040	0.38%	0.035%
23	17.380	2390	2396	2406	rBV	2881620	3968485	57.72%	5.300%
24	17.480	2407	2413	2429	rVV	4372865	5920511	86.11%	7.906%
25	19.333	2724	2728	2734	rBV2	43531	59750	0.87%	0.080%
26	19.404	2736	2740	2744	rBV	43306	55458	0.81%	0.074%
27	19.768	2796	2802	2813	rBV	5164504	6812741	99.09%	9.098%
28	21.562	3102	3107	3118	rBV	3170611	4075239	59.27%	5.442%
29	23.856	3490	3497	3507	rBV2	3504598	6875265	100.00%	9.181%
30	24.015	3517	3524	3541	rVB	2248638	4632244	67.38%	6.186%




Sum of corrected areas: 74881782

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038874.D
Acq On : 06 Mar 2023 16:43
Operator : CG/JU
Sample : PB151197BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK197

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

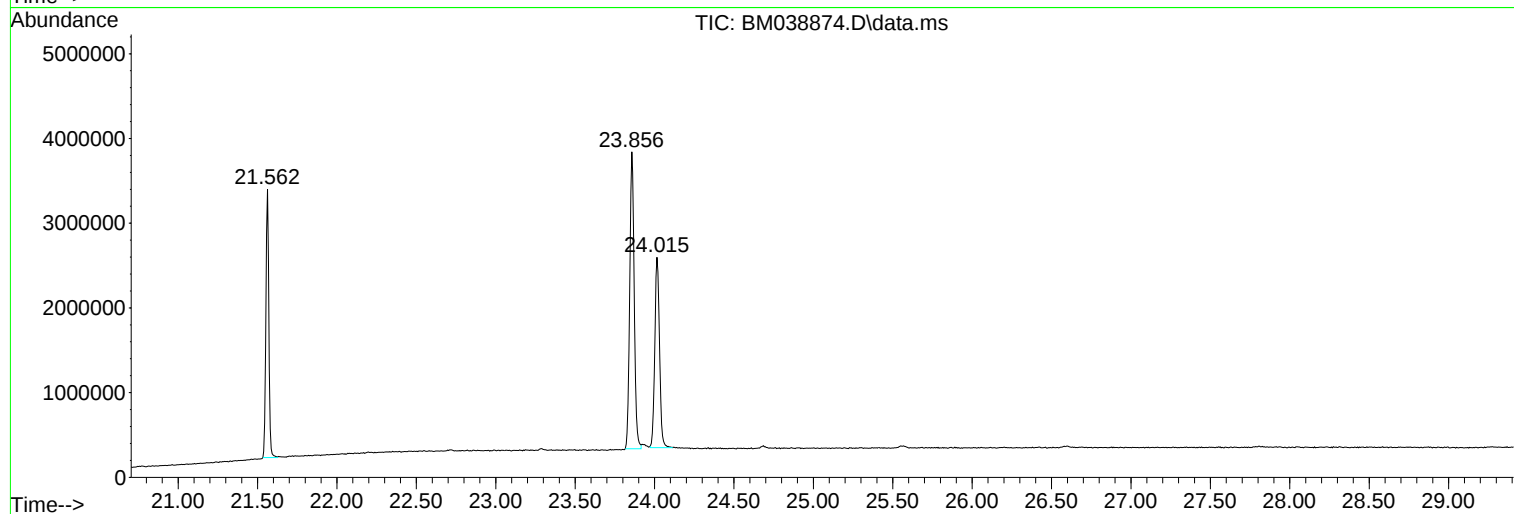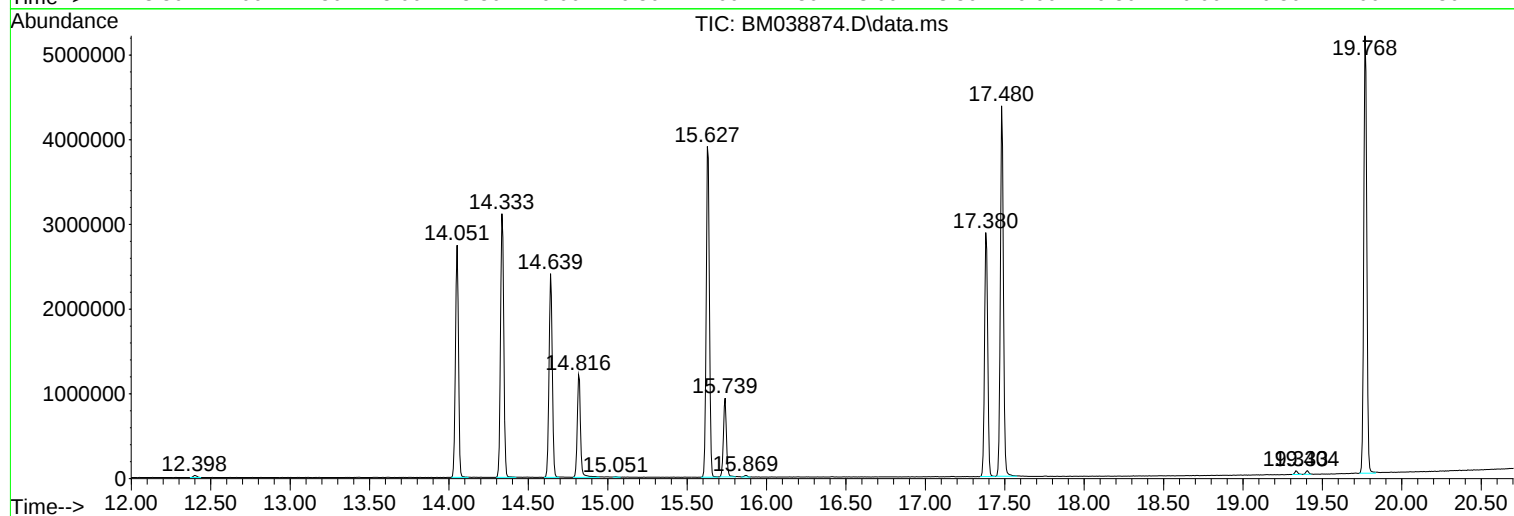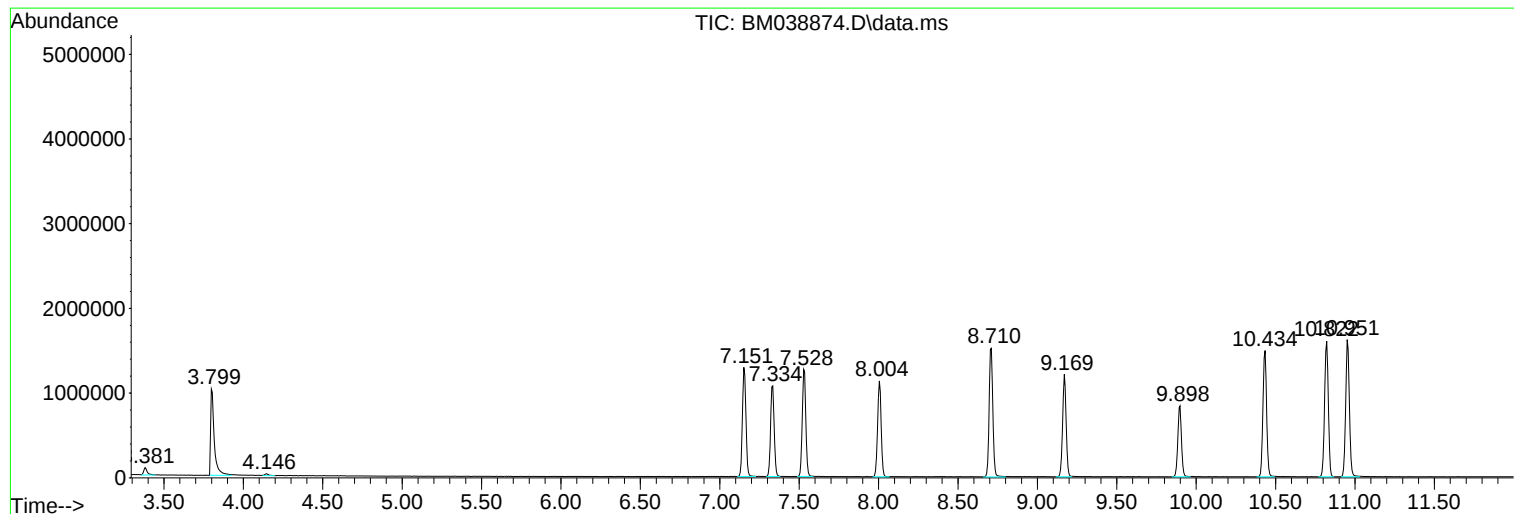

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038874.D
Acq On : 06 Mar 2023 16:43
Operator : CG/JU
Sample : PB151197BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK197

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038874.D
Acq On : 06 Mar 2023 16:43
Operator : CG/JU
Sample : PB151197BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK197

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc