

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
 Data File : BM038884.D
 Acq On : 06 Mar 2023 22:54
 Operator : CG/JU
 Sample : 01746-15
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCAF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038884.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	12	16	28	rVB	57575	93807	0.99%	0.126%
2	3.675	62	66	70	rBV5	6989	14275	0.15%	0.019%
3	3.810	86	89	108	rBV	121836	230414	2.44%	0.311%
4	4.046	124	129	137	rVV2	27326	46650	0.49%	0.063%
5	4.146	141	146	152	rBV2	18216	28556	0.30%	0.038%
6	4.246	158	163	168	rBV3	18132	24307	0.26%	0.033%
7	4.516	207	209	218	rBV10	5067	9512	0.10%	0.013%
8	5.075	297	304	311	rBV	14649	25451	0.27%	0.034%
9	6.381	521	526	529	rVB3	15954	21418	0.23%	0.029%
10	7.151	651	657	669	rVB	239367	371403	3.93%	0.501%
11	7.328	680	687	697	rBV	1039293	1595909	16.90%	2.151%
12	7.528	714	721	730	rBV	893648	1413592	14.97%	1.906%
13	8.004	794	802	809	rBV	963804	1521410	16.11%	2.051%
14	8.704	914	921	932	rBV	705430	1092112	11.56%	1.472%
15	9.169	992	1000	1009	rBV	1172485	1875066	19.85%	2.528%
16	9.275	1012	1018	1027	rBV	59401	103110	1.09%	0.139%
17	9.604	1069	1074	1079	rVB3	8183	13076	0.14%	0.018%
18	9.892	1115	1123	1133	rBV	870478	1387701	14.69%	1.871%
19	10.428	1204	1214	1226	rBV	1297855	2097092	22.20%	2.827%
20	10.816	1273	1280	1289	rVB	1383972	2319040	24.55%	3.126%
21	10.951	1294	1303	1318	rBV	1222055	2072369	21.94%	2.794%
22	11.598	1410	1413	1416	rBV3	9504	15498	0.16%	0.021%
23	12.104	1495	1499	1502	rBV3	10425	16260	0.17%	0.022%
24	12.398	1545	1549	1555	rVB	26274	40005	0.42%	0.054%
25	13.533	1738	1742	1748	rBV9	6829	12154	0.13%	0.016%
26	14.051	1823	1830	1842	rBV	2716988	3819356	40.44%	5.149%
27	14.333	1871	1878	1887	rBV	3218945	4547193	48.15%	6.130%
28	14.639	1923	1930	1938	rBV	2133489	3113932	32.97%	4.198%
29	14.816	1953	1960	1976	rBV	227979	356671	3.78%	0.481%
30	15.004	1986	1992	1996	rBV4	7204	14019	0.15%	0.019%
31	15.051	1996	2000	2006	rVB6	17862	26450	0.28%	0.036%
32	15.457	2062	2069	2072	rBV2	7437	15397	0.16%	0.021%
33	15.627	2091	2098	2110	rBV	4247182	5933655	62.83%	7.999%
34	15.733	2110	2116	2129	rBV	1207392	1614263	17.09%	2.176%
35	15.868	2134	2139	2144	rVB3	19593	31343	0.33%	0.042%
36	15.992	2152	2160	2166	rBV	218293	293270	3.11%	0.395%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
 Data File : BM038884.D
 Acq On : 06 Mar 2023 22:54
 Operator : CG/JU
 Sample : 01746-15
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCAF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Title : SVOA CALIBRATION

37	17.380	2390	2396	2406	rBV	2705799	3672897	38.89%	4.951%
38	17.480	2406	2413	2424	rBV	5013340	6924089	73.31%	9.334%
39	18.057	2507	2511	2515	rBV5	8631	11649	0.12%	0.016%
40	18.274	2544	2548	2555	rBV2	53211	75767	0.80%	0.102%
41	18.351	2558	2561	2568	rVB	21976	24863	0.26%	0.034%
42	18.709	2618	2622	2626	rBV7	11776	18571	0.20%	0.025%
43	19.333	2724	2728	2734	rBV	63123	82794	0.88%	0.112%
44	19.404	2735	2740	2744	rBV2	56148	86165	0.91%	0.116%
45	19.545	2761	2764	2770	rBV7	30894	45104	0.48%	0.061%
46	19.768	2796	2802	2810	rBV	6605018	8346592	88.38%	11.252%
47	21.268	3054	3057	3063	rBV5	61300	71345	0.76%	0.096%
48	21.556	3101	3106	3117	rBV	3244111	4261245	45.12%	5.745%
49	23.850	3489	3496	3506	rBV2	4731992	9444441	100.00%	12.732%
50	24.009	3516	3523	3536	rVB2	2425663	4906752	51.95%	6.615%




Sum of corrected areas: 74178010

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038884.D
Acq On : 06 Mar 2023 22:54
Operator : CG/JU
Sample : 01746-15
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCAF1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

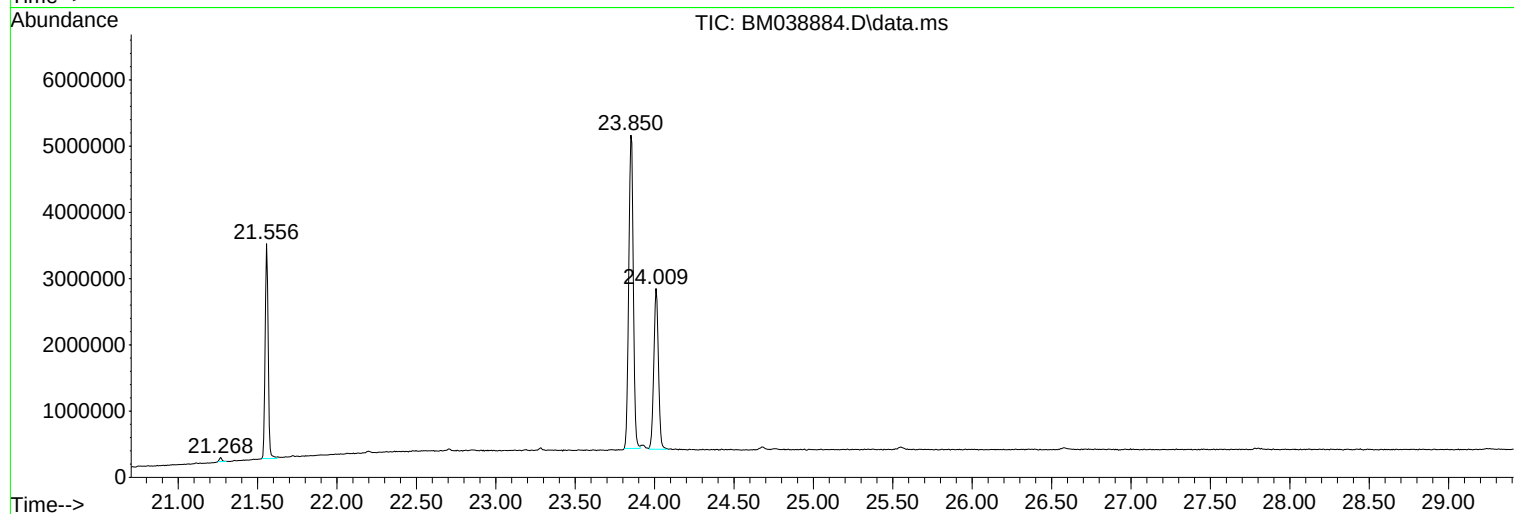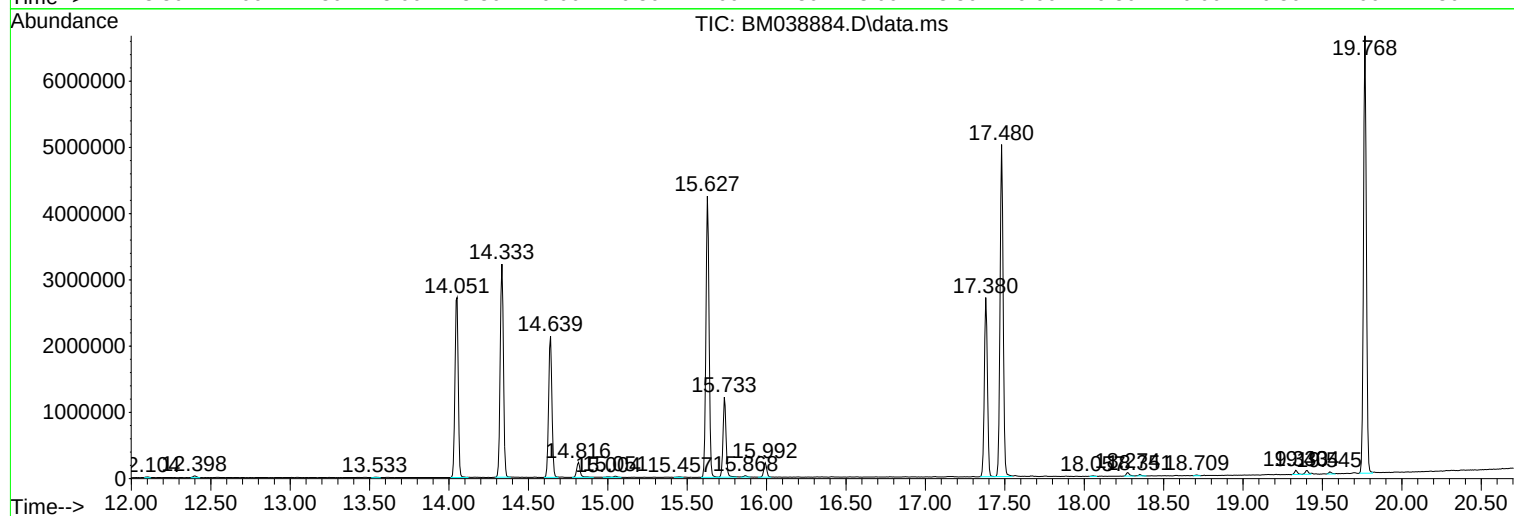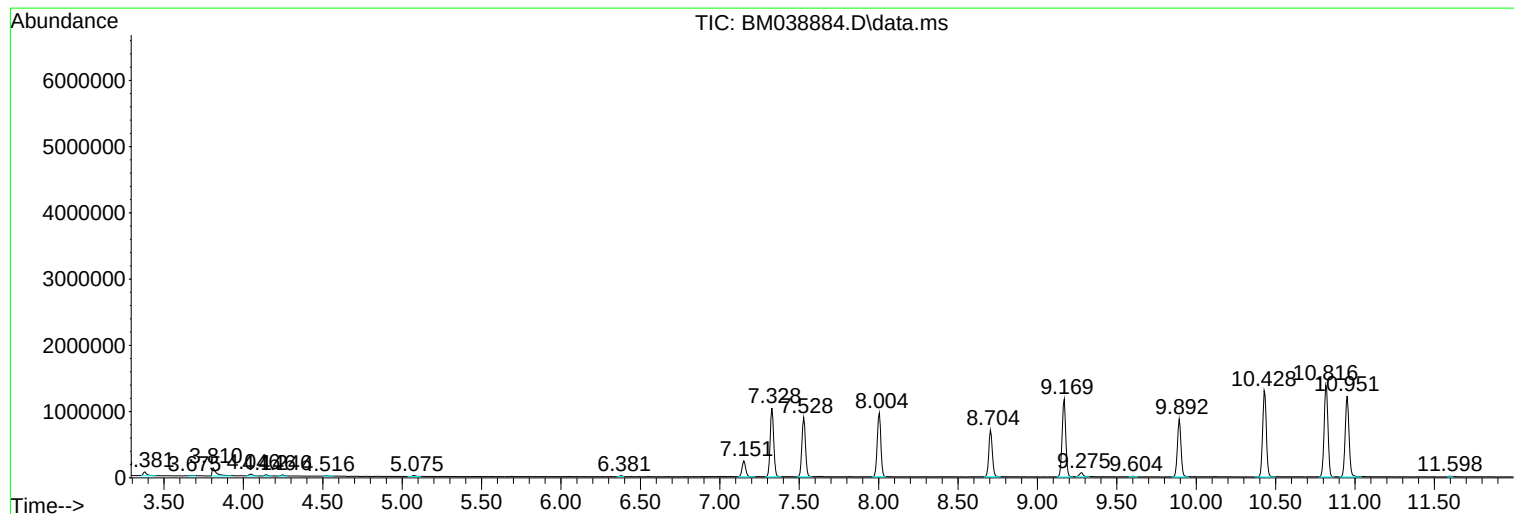

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038884.D
Acq On : 06 Mar 2023 22:54
Operator : CG/JU
Sample : 01746-15
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCAF1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038884.D
Acq On : 06 Mar 2023 22:54
Operator : CG/JU
Sample : 01746-15
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCAF1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc