

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
 Data File : BM038885.D
 Acq On : 06 Mar 2023 23:31
 Operator : CG/JU
 Sample : 01746-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCAC8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038885.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	12	16	25	rVB	64286	89897	0.94%	0.105%
2	3.681	63	67	71	rVB7	5665	10137	0.11%	0.012%
3	3.805	85	88	107	rBV	275034	457871	4.77%	0.536%
4	4.052	124	130	135	rBV	28322	46092	0.48%	0.054%
5	4.140	142	145	152	rVB	23720	33922	0.35%	0.040%
6	4.246	159	163	169	rVB3	17392	26926	0.28%	0.032%
7	5.075	300	304	311	rVB	17306	31417	0.33%	0.037%
8	6.381	520	526	533	rVB3	17542	27347	0.29%	0.032%
9	7.151	651	657	665	rVB	269872	421215	4.39%	0.493%
10	7.328	680	687	697	rBV	1249389	1886158	19.66%	2.207%
11	7.528	714	721	731	rBV	1079059	1682148	17.53%	1.968%
12	8.004	792	802	809	rBV	1250696	1946247	20.29%	2.277%
13	8.704	914	921	929	rBV	833964	1286982	13.41%	1.506%
14	9.169	992	1000	1012	rBV	1412315	2221771	23.16%	2.599%
15	9.275	1012	1018	1025	rBV	44595	72029	0.75%	0.084%
16	9.604	1070	1074	1079	rVB2	8282	11969	0.12%	0.014%
17	9.892	1114	1123	1132	rBV	1044597	1684066	17.55%	1.970%
18	10.428	1207	1214	1224	rBV	1556023	2536806	26.44%	2.968%
19	10.816	1272	1280	1292	rBV	1808835	2971199	30.97%	3.476%
20	10.951	1295	1303	1314	rBV	1568237	2600610	27.11%	3.043%
21	11.604	1410	1414	1419	rBV6	5216	11190	0.12%	0.013%
22	12.398	1544	1549	1555	rVB	29209	47788	0.50%	0.056%
23	12.539	1569	1573	1581	rVB3	19014	27440	0.29%	0.032%
24	13.539	1739	1743	1749	rVV3	16774	25568	0.27%	0.030%
25	14.051	1823	1830	1840	rBV	3158112	4362192	45.47%	5.104%
26	14.333	1870	1878	1886	rBV	3937825	5399644	56.28%	6.317%
27	14.639	1923	1930	1939	rBV	2803579	3996630	41.66%	4.676%
28	14.816	1953	1960	1973	rBV	237948	374224	3.90%	0.438%
29	15.051	1996	2000	2004	rBV4	19781	26591	0.28%	0.031%
30	15.439	2061	2066	2071	rBV4	9159	14837	0.15%	0.017%
31	15.627	2091	2098	2107	rBV	4799197	6859622	71.50%	8.026%
32	15.739	2109	2117	2129	rBV	1412045	1906285	19.87%	2.230%
33	15.869	2135	2139	2146	rVB3	24188	35029	0.37%	0.041%
34	16.180	2188	2192	2198	rVB7	12906	23984	0.25%	0.028%
35	17.015	2330	2334	2339	rBV2	38643	57017	0.59%	0.067%
36	17.051	2339	2340	2346	rVB6	7660	9646	0.10%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
 Data File : BM038885.D
 Acq On : 06 Mar 2023 23:31
 Operator : CG/JU
 Sample : 01746-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCAC8

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Title : SVOA CALIBRATION

37	17.380	2390	2396	2405	rBV	3325495	4646975	48.44%	5.437%
38	17.480	2406	2413	2423	rBV	5816362	7946143	82.82%	9.297%
39	18.274	2544	2548	2552	rBV4	35477	48741	0.51%	0.057%
40	18.351	2556	2561	2565	rVV2	15259	21164	0.22%	0.025%
41	18.710	2619	2622	2626	rVB5	14610	17224	0.18%	0.020%
42	19.333	2724	2728	2735	rVB	66190	91216	0.95%	0.107%
43	19.404	2735	2740	2744	rBV	67834	95752	1.00%	0.112%
44	19.551	2761	2765	2769	rBV4	29653	42962	0.45%	0.050%
45	19.768	2796	2802	2816	rBV	7262262	9269640	96.62%	10.845%
46	21.556	3101	3106	3116	rBV	3785807	4970793	51.81%	5.816%
47	23.856	3489	3497	3507	rBV2	4791045	9593996	100.00%	11.225%
48	24.015	3516	3524	3537	rVB2	2677096	5504141	57.37%	6.440%




Sum of corrected areas: 85471243

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038885.D
Acq On : 06 Mar 2023 23:31
Operator : CG/JU
Sample : 01746-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCAC8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

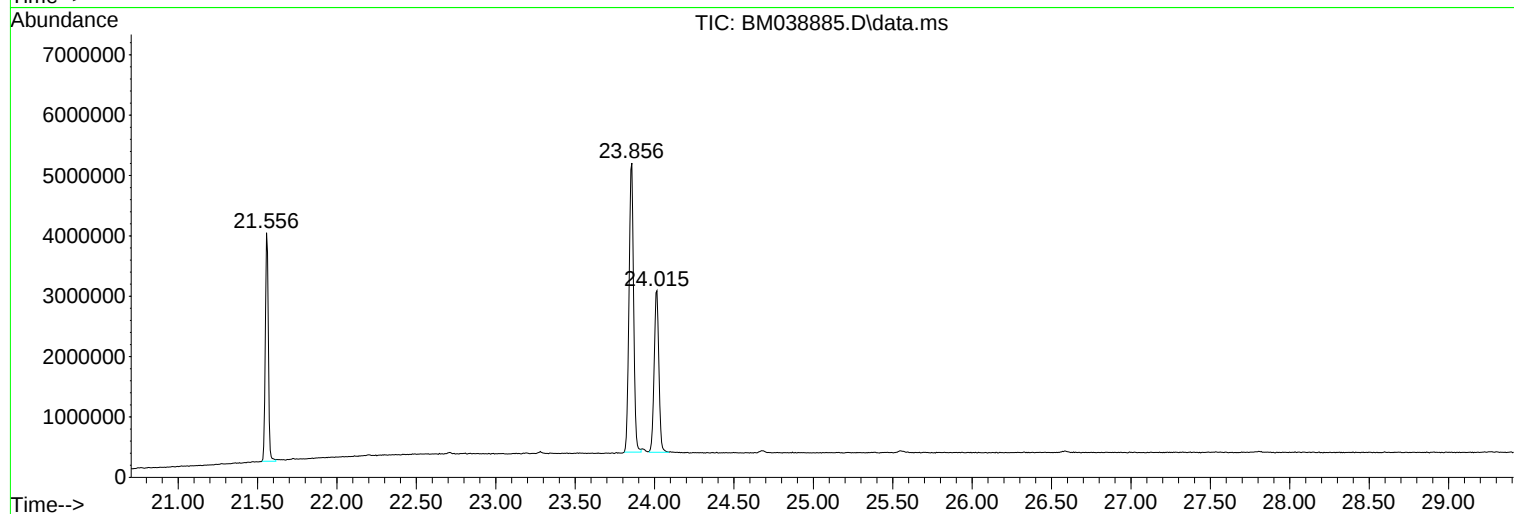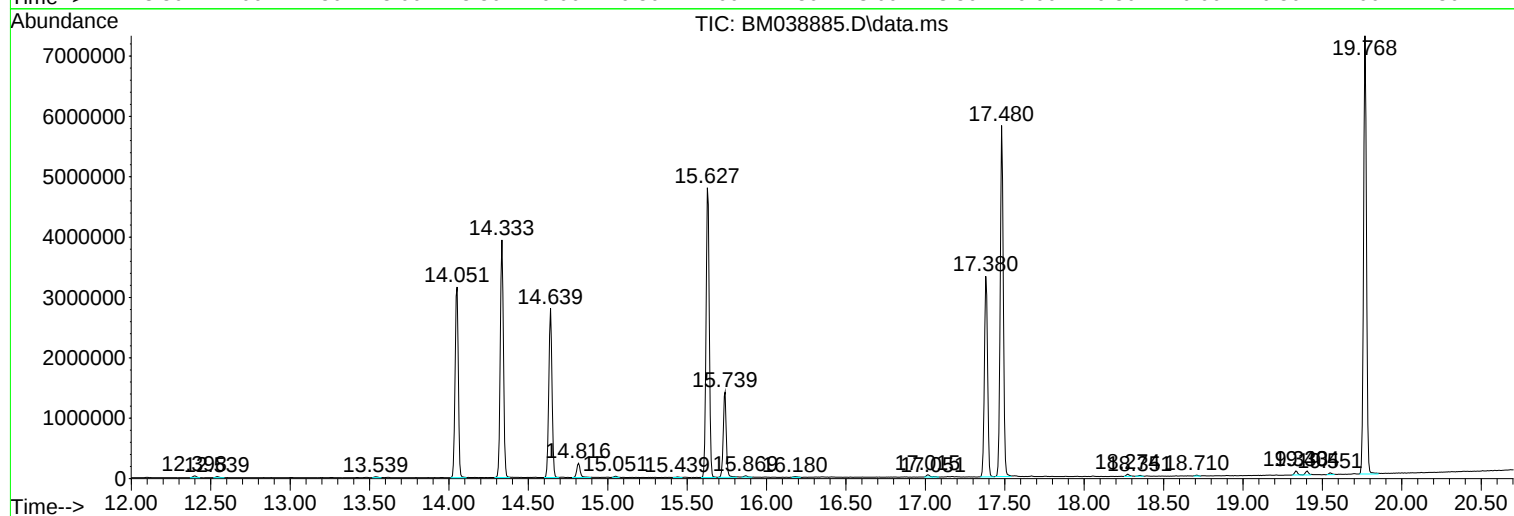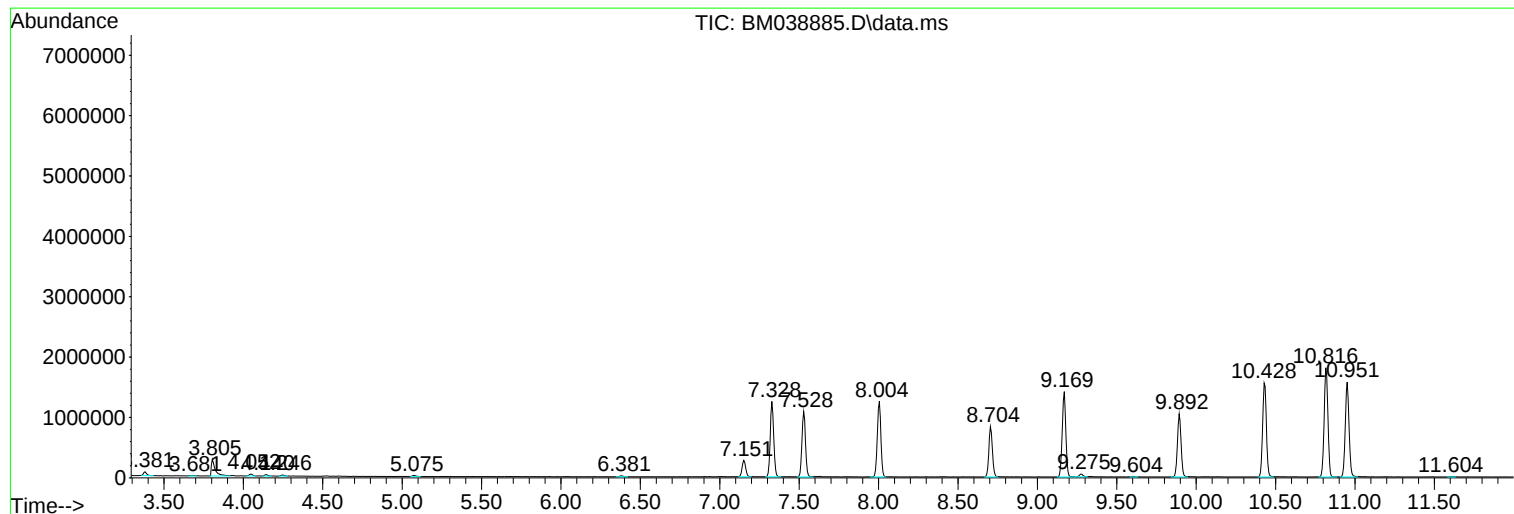

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038885.D
Acq On : 06 Mar 2023 23:31
Operator : CG/JU
Sample : 01746-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCAC8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038885.D
Acq On : 06 Mar 2023 23:31
Operator : CG/JU
Sample : 01746-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCAC8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc