

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM030723\  
 Data File : BM038890.D  
 Acq On : 07 Mar 2023 11:04  
 Operator : CG/JU  
 Sample : PB151234BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 SBLK234

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM022823.M  
 Title : SVOA CALIBRATION

Signal : TIC: BM038890.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 3.381       | 12            | 16          | 27           | rVB      | 79061          | 123698        | 1.40%           | 0.151%        |
| 2         | 3.799       | 85            | 87          | 111          | rBV      | 1074411        | 1680992       | 19.00%          | 2.051%        |
| 3         | 4.146       | 142           | 146         | 153          | rVB      | 19956          | 28692         | 0.32%           | 0.035%        |
| 4         | 7.151       | 650           | 657         | 666          | rBV      | 1393250        | 2084572       | 23.57%          | 2.543%        |
| 5         | 7.328       | 680           | 687         | 698          | rVB      | 1155150        | 1758186       | 19.88%          | 2.145%        |
| 6         | 7.528       | 713           | 721         | 734          | rBV      | 1345744        | 2094863       | 23.68%          | 2.556%        |
| 7         | 8.004       | 795           | 802         | 812          | rVB      | 1035675        | 1594495       | 18.03%          | 1.945%        |
| 8         | 8.704       | 914           | 921         | 935          | rBV      | 1688340        | 2607499       | 29.48%          | 3.181%        |
| 9         | 9.169       | 993           | 1000        | 1013         | rBV      | 1267643        | 2055403       | 23.24%          | 2.508%        |
| 10        | 9.892       | 1115          | 1123        | 1131         | rBV      | 1004658        | 1591473       | 17.99%          | 1.942%        |
| 11        | 10.428      | 1207          | 1214        | 1229         | rBV      | 1610023        | 2612364       | 29.53%          | 3.187%        |
| 12        | 10.816      | 1272          | 1280        | 1293         | rVB      | 1456599        | 2453246       | 27.74%          | 2.993%        |
| 13        | 10.951      | 1295          | 1303        | 1319         | rBV      | 1698919        | 2842825       | 32.14%          | 3.468%        |
| 14        | 12.398      | 1544          | 1549        | 1556         | rVB      | 29333          | 47395         | 0.54%           | 0.058%        |
| 15        | 14.051      | 1823          | 1830        | 1840         | rBV      | 2949321        | 3970651       | 44.89%          | 4.845%        |
| 16        | 14.333      | 1871          | 1878        | 1886         | rBV      | 3353493        | 4753262       | 53.74%          | 5.799%        |
| 17        | 14.639      | 1922          | 1930        | 1938         | rBV      | 2304503        | 3275865       | 37.04%          | 3.997%        |
| 18        | 14.815      | 1954          | 1960        | 1979         | rBV      | 1452073        | 2112661       | 23.88%          | 2.578%        |
| 19        | 15.051      | 1995          | 2000        | 2007         | rVB7     | 8369           | 13414         | 0.15%           | 0.016%        |
| 20        | 15.627      | 2090          | 2098        | 2106         | rBV      | 4190681        | 5964104       | 67.43%          | 7.277%        |
| 21        | 15.739      | 2110          | 2117        | 2132         | rVV      | 1218667        | 1604025       | 18.13%          | 1.957%        |
| 22        | 15.868      | 2135          | 2139        | 2145         | rVB4     | 19215          | 31665         | 0.36%           | 0.039%        |
| 23        | 16.415      | 2228          | 2232        | 2235         | rBV5     | 5347           | 10023         | 0.11%           | 0.012%        |
| 24        | 17.380      | 2389          | 2396        | 2406         | rBV      | 2750866        | 3863487       | 43.68%          | 4.714%        |
| 25        | 17.480      | 2406          | 2413        | 2427         | rBV      | 4876182        | 6646467       | 75.14%          | 8.109%        |
| 26        | 19.333      | 2724          | 2728        | 2732         | rBV2     | 50041          | 67405         | 0.76%           | 0.082%        |
| 27        | 19.403      | 2736          | 2740        | 2746         | rVV2     | 50926          | 68058         | 0.77%           | 0.083%        |
| 28        | 19.768      | 2796          | 2802        | 2812         | rBV      | 6054630        | 7915731       | 89.49%          | 9.658%        |
| 29        | 21.562      | 3101          | 3107        | 3115         | rBV      | 3403530        | 4369278       | 49.40%          | 5.331%        |
| 30        | 23.856      | 3489          | 3497        | 3507         | rBV      | 4579001        | 8845149       | 100.00%         | 10.792%       |
| 31        | 24.015      | 3517          | 3524        | 3535         | rVB2     | 2413233        | 4874574       | 55.11%          | 5.947%        |




Sum of corrected areas: 81961522

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM030723\  
Data File : BM038890.D  
Acq On : 07 Mar 2023 11:04  
Operator : CG/JU  
Sample : PB151234BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
SBLK234

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM022823.M  
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

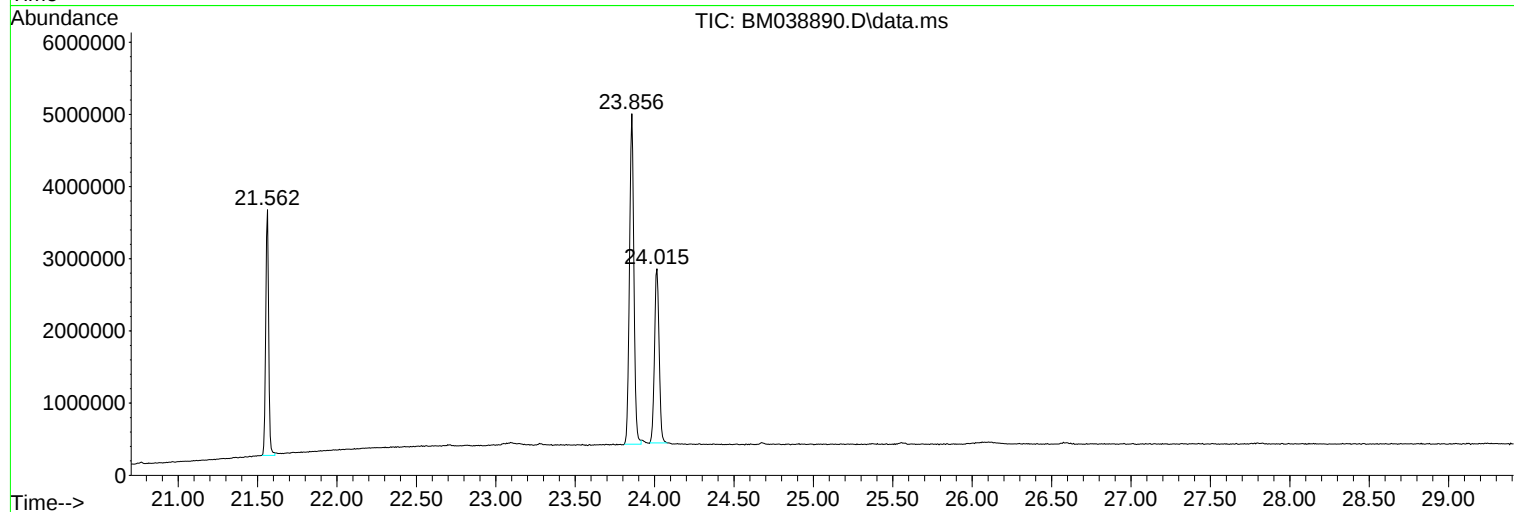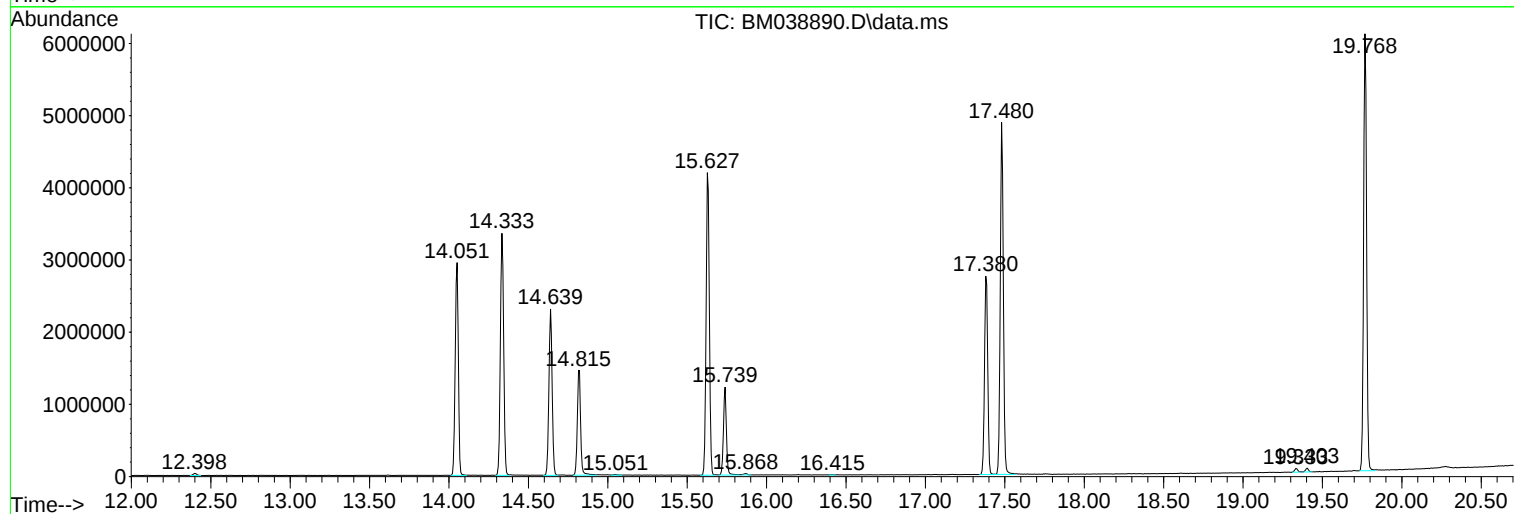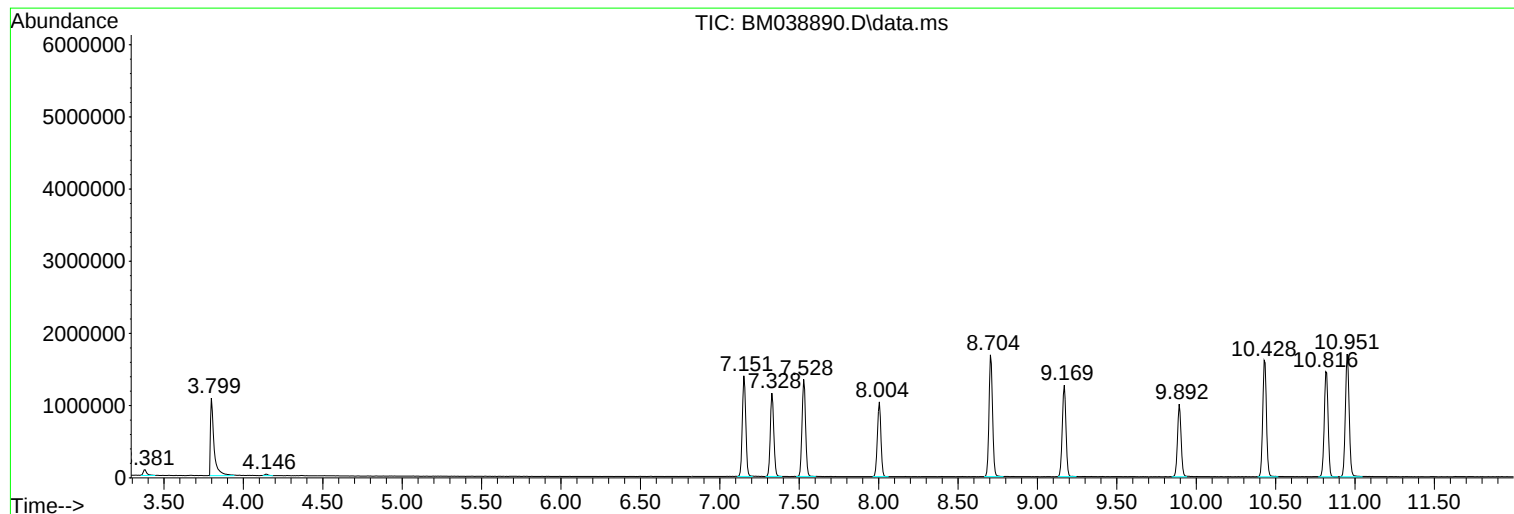

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM030723\  
Data File : BM038890.D  
Acq On : 07 Mar 2023 11:04  
Operator : CG/JU  
Sample : PB151234BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
SBLK234

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM022823.M  
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM030723\  
Data File : BM038890.D  
Acq On : 07 Mar 2023 11:04  
Operator : CG/JU  
Sample : PB151234BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
SBLK234

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\SFAM-EPA-BM022823.M  
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |