

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
 Data File : BM038891.D
 Acq On : 07 Mar 2023 11:42
 Operator : CG/JU
 Sample : PB151199BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK199

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038891.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	12	15	26	rVB	74249	113390	1.53%	0.156%
2	3.799	85	87	107	rBV	986232	1544319	20.77%	2.127%
3	4.146	142	146	151	rVB	17083	23582	0.32%	0.032%
4	7.151	649	657	673	rBV	1206729	1843561	24.80%	2.539%
5	7.328	680	687	696	rBV	1041325	1569169	21.11%	2.161%
6	7.528	713	721	734	rBV	1205695	1865428	25.09%	2.569%
7	8.004	795	802	810	rBV	967152	1492817	20.08%	2.056%
8	8.704	914	921	935	rBV	1460269	2287591	30.77%	3.151%
9	9.169	993	1000	1010	rBV	1157906	1806175	24.29%	2.488%
10	9.892	1116	1123	1133	rBV	854242	1369416	18.42%	1.886%
11	10.428	1208	1214	1228	rBV	1370841	2266231	30.48%	3.121%
12	10.816	1272	1280	1289	rBV	1372860	2274332	30.59%	3.132%
13	10.951	1296	1303	1313	rBV	1551482	2509784	33.76%	3.457%
14	12.398	1543	1549	1555	rBV	24068	37686	0.51%	0.052%
15	14.051	1823	1830	1841	rBV	2556412	3468613	46.65%	4.777%
16	14.333	1871	1878	1886	rBV	2950250	4192089	56.38%	5.773%
17	14.639	1923	1930	1938	rBV	2135832	3057005	41.12%	4.210%
18	14.816	1953	1960	1979	rBV	1236985	1796182	24.16%	2.474%
19	15.045	1996	1999	2004	rVB6	7387	9124	0.12%	0.013%
20	15.627	2091	2098	2106	rBV	3778492	5252659	70.65%	7.234%
21	15.739	2110	2117	2129	rBV	962126	1315881	17.70%	1.812%
22	15.869	2135	2139	2146	rVB2	17972	25039	0.34%	0.034%
23	17.163	2354	2359	2365	rBV3	6158	11662	0.16%	0.016%
24	17.380	2389	2396	2403	rBV	2598211	3611655	48.58%	4.974%
25	17.480	2407	2413	2428	rVV	4217327	5714699	76.86%	7.870%
26	19.333	2724	2728	2733	rBV2	41111	55754	0.75%	0.077%
27	19.404	2736	2740	2745	rVV	41273	55914	0.75%	0.077%
28	19.768	2796	2802	2812	rBV	5063305	6770881	91.07%	9.325%
29	21.562	3101	3107	3118	rBV	3047025	4116371	55.37%	5.669%
30	23.856	3490	3497	3507	rBV2	3833969	7434837	100.00%	10.239%
31	24.015	3517	3524	3536	rVB2	2359804	4718097	63.46%	6.498%




Sum of corrected areas: 72609943

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038891.D
Acq On : 07 Mar 2023 11:42
Operator : CG/JU
Sample : PB151199BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK199

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

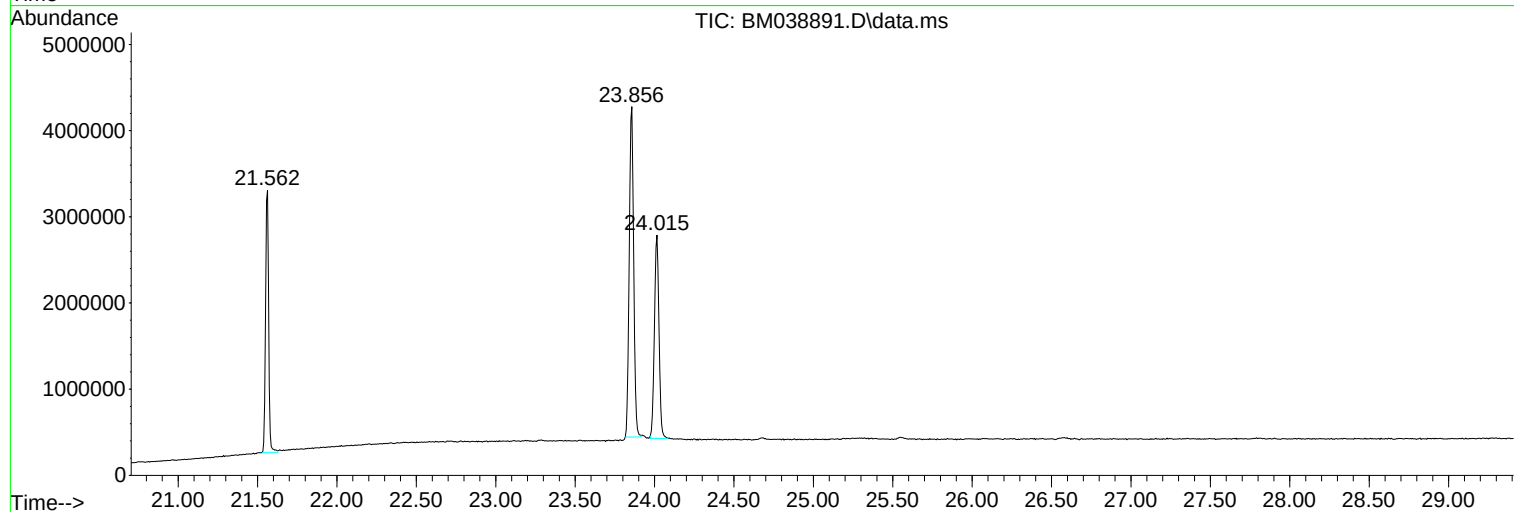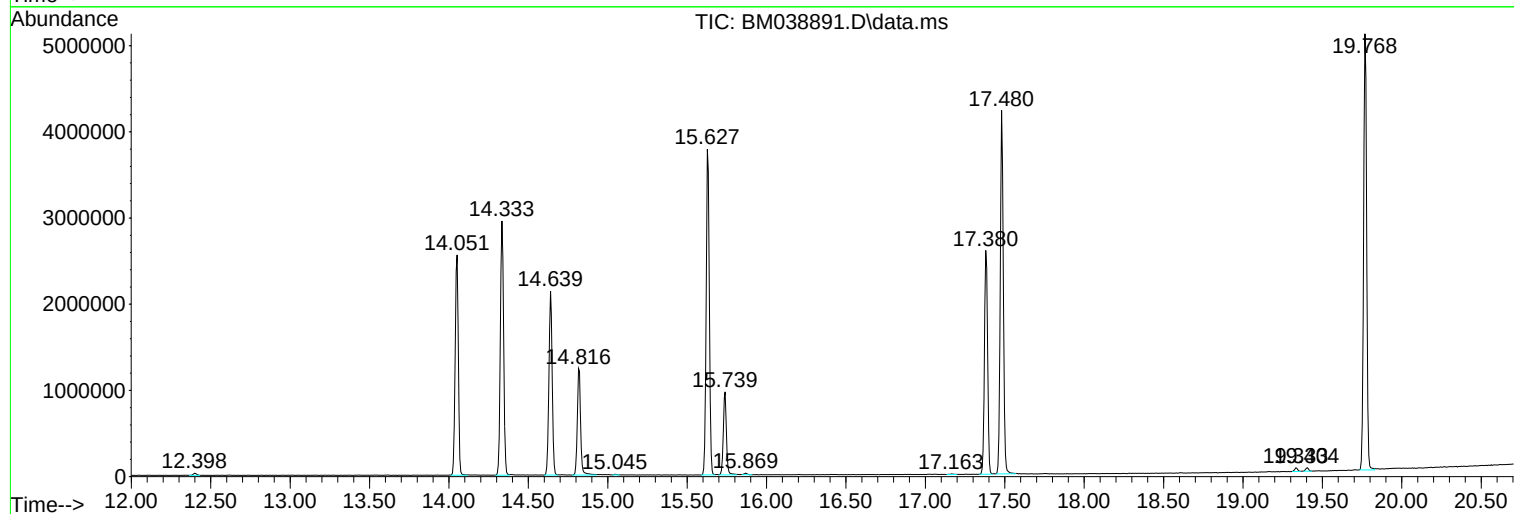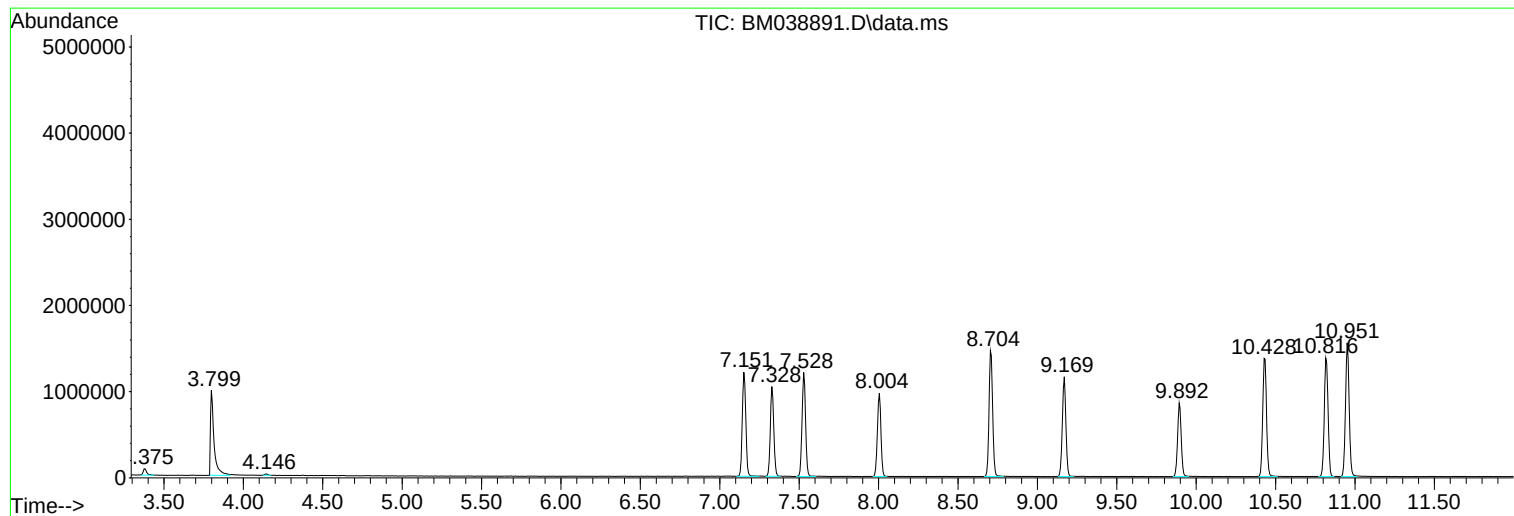

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038891.D
Acq On : 07 Mar 2023 11:42
Operator : CG/JU
Sample : PB151199BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK199

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038891.D
Acq On : 07 Mar 2023 11:42
Operator : CG/JU
Sample : PB151199BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK199

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------