

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
 Data File : BM038902.D
 Acq On : 07 Mar 2023 19:09
 Operator : CG/JU
 Sample : 01745-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COLE9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038902.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	12	15	21	rBV	52665	74682	0.71%	0.090%
2	3.805	86	88	106	rBV	197040	336093	3.19%	0.403%
3	4.046	124	129	136	rVB	28645	45451	0.43%	0.054%
4	4.146	141	146	150	rBV	17562	25641	0.24%	0.031%
5	4.246	160	163	169	rVB3	16976	22676	0.22%	0.027%
6	5.075	300	304	313	rVB2	27792	49961	0.47%	0.060%
7	6.381	518	526	533	rVB2	17040	30284	0.29%	0.036%
8	7.152	650	657	665	rVB	289068	444553	4.22%	0.533%
9	7.328	680	687	696	rBV	1149433	1750031	16.62%	2.098%
10	7.528	714	721	730	rBV	1038317	1605328	15.25%	1.925%
11	7.628	734	738	746	rVB10	6635	13629	0.13%	0.016%
12	7.893	776	783	789	rVB7	8460	16240	0.15%	0.019%
13	8.004	794	802	811	rVV	1052248	1662955	15.80%	1.994%
14	8.604	898	904	908	rVB5	11920	18080	0.17%	0.022%
15	8.704	914	921	930	rBV	832364	1314350	12.48%	1.576%
16	9.169	992	1000	1012	rBV	1295581	2089053	19.84%	2.505%
17	9.598	1069	1073	1075	rBV2	10729	14929	0.14%	0.018%
18	9.893	1115	1123	1135	rBV	980145	1548282	14.71%	1.856%
19	10.428	1206	1214	1224	rBV	1490532	2399879	22.80%	2.877%
20	10.675	1253	1256	1261	rVB6	8983	13492	0.13%	0.016%
21	10.816	1272	1280	1293	rVB	1545011	2566873	24.38%	3.078%
22	10.951	1296	1303	1319	rBV	1044613	1707801	16.22%	2.048%
23	11.369	1367	1374	1378	rBV7	6126	13324	0.13%	0.016%
24	11.416	1378	1382	1387	rVB8	10490	14733	0.14%	0.018%
25	12.098	1491	1498	1504	rBV2	20004	31121	0.30%	0.037%
26	12.398	1544	1549	1556	rVB2	29458	44114	0.42%	0.053%
27	12.628	1582	1588	1592	rBV7	5357	10905	0.10%	0.013%
28	12.775	1610	1613	1619	rBV6	12565	19512	0.19%	0.023%
29	13.269	1689	1697	1703	rVB	24353	40909	0.39%	0.049%
30	13.451	1722	1728	1736	rBV8	48069	88329	0.84%	0.106%
31	13.534	1736	1742	1747	rVB8	9759	21673	0.21%	0.026%
32	13.651	1757	1762	1768	rVB	25338	39880	0.38%	0.048%
33	14.051	1823	1830	1841	rBV	3134843	4333998	41.17%	5.196%
34	14.333	1871	1878	1885	rBV	3589952	4988198	47.38%	5.981%
35	14.639	1923	1930	1939	rBV	2452321	3496655	33.21%	4.192%
36	14.698	1939	1940	1947	rVB7	8996	16150	0.15%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
 Data File : BM038902.D
 Acq On : 07 Mar 2023 19:09
 Operator : CG/JU
 Sample : 01745-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COLE9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Title : SVOA CALIBRATION

37	14.816	1954	1960	1973	rBV	306216	451226	4.29%	0.541%
38	15.045	1994	1999	2005	rVB6	14507	22925	0.22%	0.027%
39	15.375	2050	2055	2061	rBV2	37649	51788	0.49%	0.062%
40	15.439	2061	2066	2070	rBV	26123	37314	0.35%	0.045%
41	15.628	2091	2098	2110	rBV	4938732	6816630	64.75%	8.173%
42	15.739	2110	2117	2132	rVV	1431743	1959769	18.62%	2.350%
43	15.869	2135	2139	2144	rVB2	22994	34910	0.33%	0.042%
44	15.992	2154	2160	2168	rVB	31934	44021	0.42%	0.053%
45	16.198	2189	2195	2199	rBV9	6541	13204	0.13%	0.016%
46	17.174	2357	2361	2368	rVB7	7677	16259	0.15%	0.019%
47	17.380	2389	2396	2403	rBV	3009336	4154354	39.46%	4.981%
48	17.480	2406	2413	2426	rBV	5929218	8197721	77.87%	9.829%
49	18.274	2545	2548	2554	rBV4	21350	31657	0.30%	0.038%
50	18.751	2624	2629	2634	rVB2	219945	281143	2.67%	0.337%
51	18.874	2648	2650	2653	rBV3	10422	11496	0.11%	0.014%
52	19.127	2691	2693	2698	rBV6	11325	19187	0.18%	0.023%
53	19.333	2724	2728	2734	rBV	68989	90876	0.86%	0.109%
54	19.404	2736	2740	2746	rVV	64409	84263	0.80%	0.101%
55	19.768	2796	2802	2810	rBV	7508477	9706218	92.20%	11.638%
56	21.557	3101	3106	3118	rBV	3622459	4672570	44.38%	5.602%
57	23.851	3489	3496	3506	rBV2	5313717	10527818	100.00%	12.623%
58	24.009	3516	3523	3539	rVB2	2612177	5268105	50.04%	6.316%




Sum of corrected areas: 83403218

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM038902\
Data File : BM038902.D
Acq On : 07 Mar 2023 19:09
Operator : CG/JU
Sample : 01745-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COLE9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

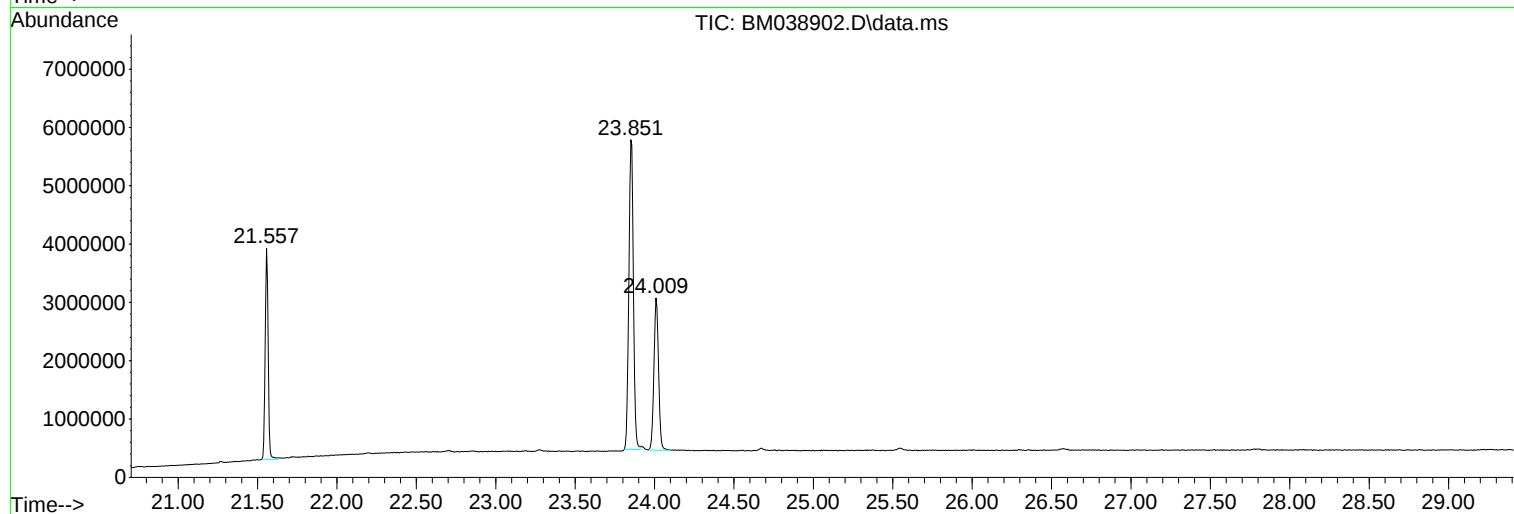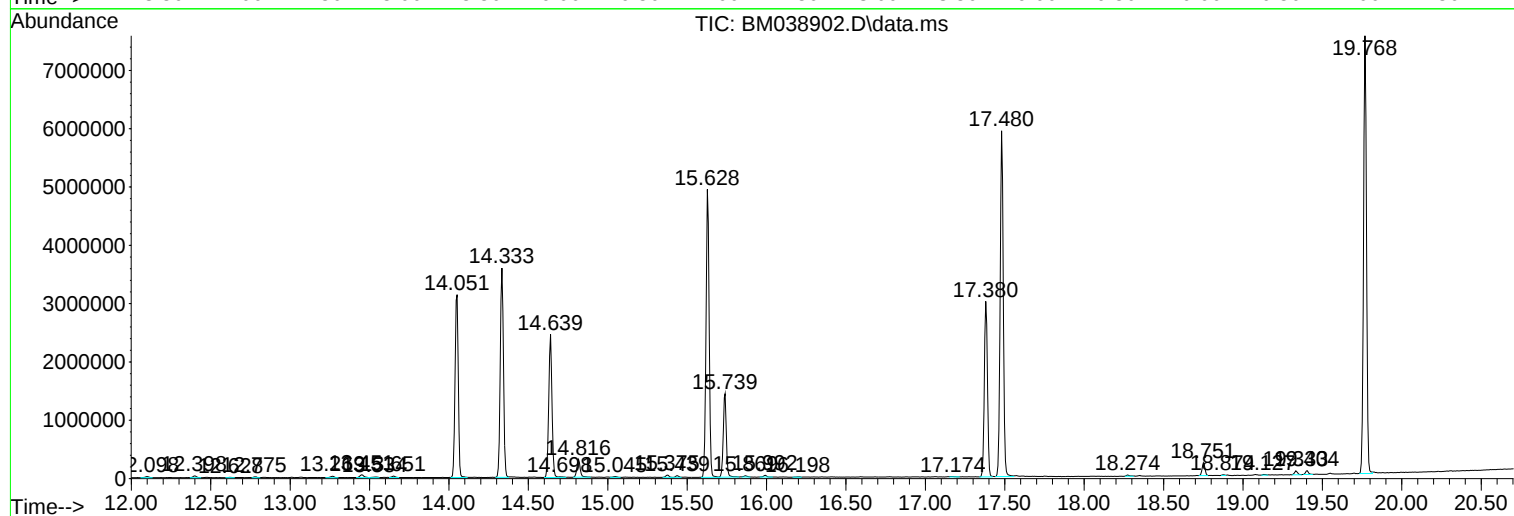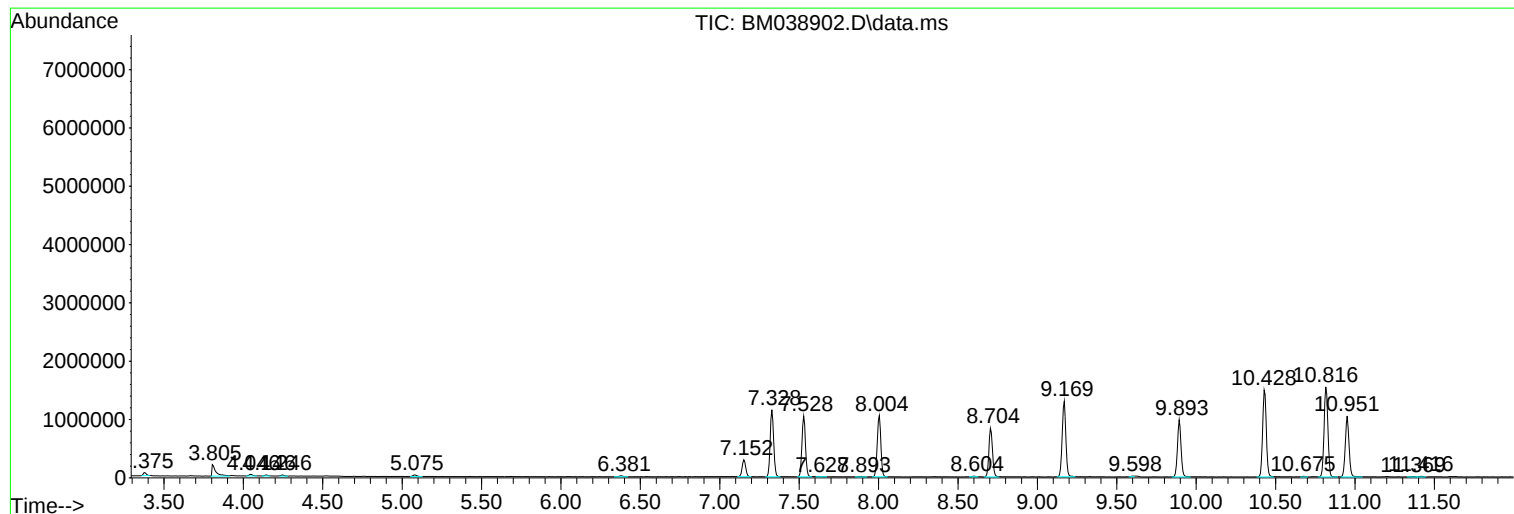

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038902.D
Acq On : 07 Mar 2023 19:09
Operator : CG/JU
Sample : 01745-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0LE9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038902.D
Acq On : 07 Mar 2023 19:09
Operator : CG/JU
Sample : 01745-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0LE9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc