

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
 Data File : BM038904.D
 Acq On : 07 Mar 2023 20:23
 Operator : CG/JU
 Sample : 01745-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COLF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038904.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	11	16	26	rVB	66269	103142	1.10%	0.128%
2	3.804	85	88	105	rBV	289030	497325	5.31%	0.619%
3	4.046	124	129	137	rVV	31294	50518	0.54%	0.063%
4	4.146	141	146	153	rVB	20151	32078	0.34%	0.040%
5	4.245	159	163	168	rVB4	17224	24468	0.26%	0.030%
6	5.081	300	305	311	rVB2	28203	46900	0.50%	0.058%
7	6.375	522	525	530	rVB2	17424	24699	0.26%	0.031%
8	7.151	651	657	668	rVB	298551	463102	4.95%	0.577%
9	7.328	680	687	696	rBV	1215121	1839795	19.65%	2.291%
10	7.528	714	721	729	rBV	1095481	1674143	17.88%	2.085%
11	8.004	795	802	811	rBV	1123263	1798011	19.21%	2.239%
12	8.598	899	903	910	rBV5	16499	29920	0.32%	0.037%
13	8.704	914	921	933	rBV	866563	1341183	14.33%	1.670%
14	9.169	992	1000	1009	rBV	1343346	2153705	23.01%	2.682%
15	9.598	1067	1073	1078	rBV	22042	33977	0.36%	0.042%
16	9.892	1115	1123	1133	rBV	955282	1538955	16.44%	1.917%
17	10.427	1207	1214	1228	rBV	1510491	2421843	25.87%	3.016%
18	10.816	1272	1280	1288	rBV	1650373	2729510	29.16%	3.400%
19	10.951	1296	1303	1317	rBV	1085305	1778594	19.00%	2.215%
20	12.098	1491	1498	1503	rBV	32442	50656	0.54%	0.063%
21	12.398	1544	1549	1557	rVB2	31071	47019	0.50%	0.059%
22	13.268	1690	1697	1702	rBV	31473	51173	0.55%	0.064%
23	13.539	1739	1743	1749	rVB6	8423	12508	0.13%	0.016%
24	13.610	1749	1755	1762	rBV7	4849	9776	0.10%	0.012%
25	14.051	1823	1830	1840	rBV	3027700	4068286	43.46%	5.067%
26	14.333	1871	1878	1888	rBV	3540458	4965943	53.05%	6.185%
27	14.639	1923	1930	1939	rBV	2607239	3681903	39.33%	4.586%
28	14.815	1953	1960	1968	rBV	238987	354740	3.79%	0.442%
29	15.045	1995	1999	2003	rVB7	12949	17218	0.18%	0.021%
30	15.439	2060	2066	2071	rBV	24088	31955	0.34%	0.040%
31	15.627	2091	2098	2109	rBV	4600920	6439216	68.79%	8.020%
32	15.739	2110	2117	2128	rBV	1106483	1538772	16.44%	1.917%
33	15.868	2135	2139	2145	rVB3	22598	32971	0.35%	0.041%
34	17.380	2390	2396	2404	rBV	3207684	4329642	46.25%	5.393%
35	17.480	2406	2413	2424	rVV	5550193	7631088	81.52%	9.504%
36	17.568	2425	2428	2432	rVB6	20604	29446	0.31%	0.037%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038904.D
Acq On : 07 Mar 2023 20:23
Operator : CG/JU
Sample : 01745-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COLF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Title : SVOA CALIBRATION

37	17.756	2454	2460	2463	rBV5	10076	18650	0.20%	0.023%
38	18.274	2545	2548	2553	rBV7	13580	18041	0.19%	0.022%
39	19.133	2690	2694	2698	rBV5	32713	43724	0.47%	0.054%
40	19.333	2724	2728	2733	rVB2	58794	73120	0.78%	0.091%
41	19.403	2736	2740	2744	rVV	54324	69607	0.74%	0.087%
42	19.768	2796	2802	2809	rBV	7052133	8876448	94.82%	11.055%
43	21.556	3101	3106	3115	rBV	3544832	4739974	50.63%	5.904%
44	23.856	3489	3497	3506	rBV2	4742280	9361068	100.00%	11.659%
45	24.009	3516	3523	3536	rVB2	2609300	5215192	55.71%	6.495%




Sum of corrected areas: 80290004

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038904.D
Acq On : 07 Mar 2023 20:23
Operator : CG/JU
Sample : 01745-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COLF1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

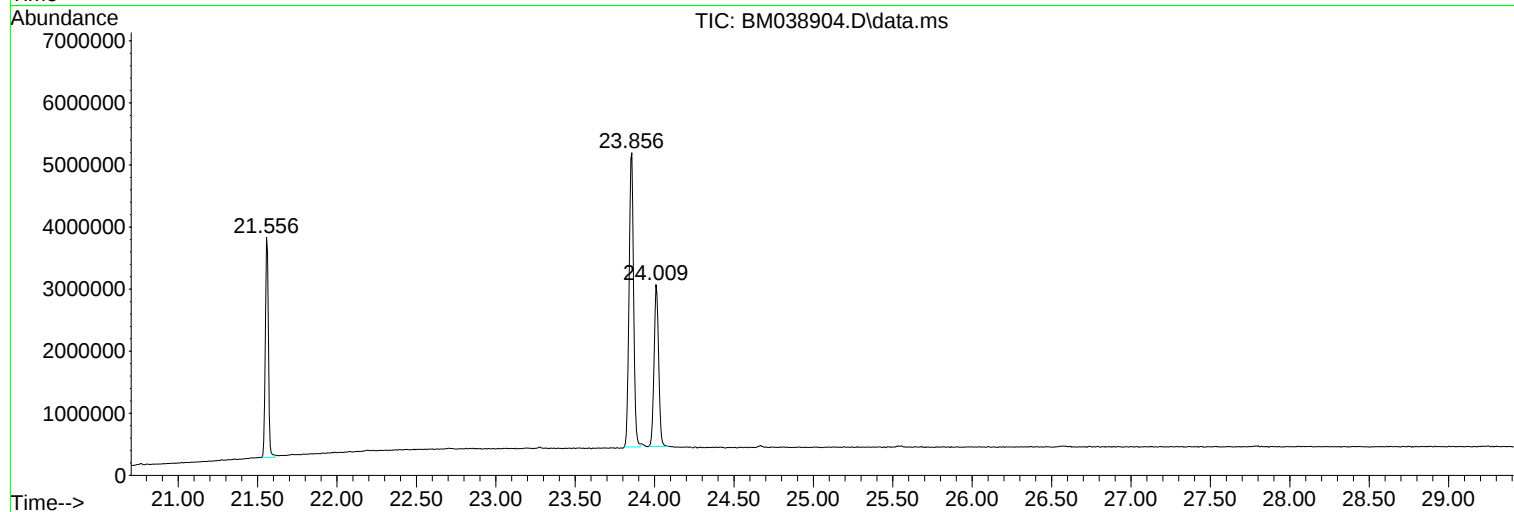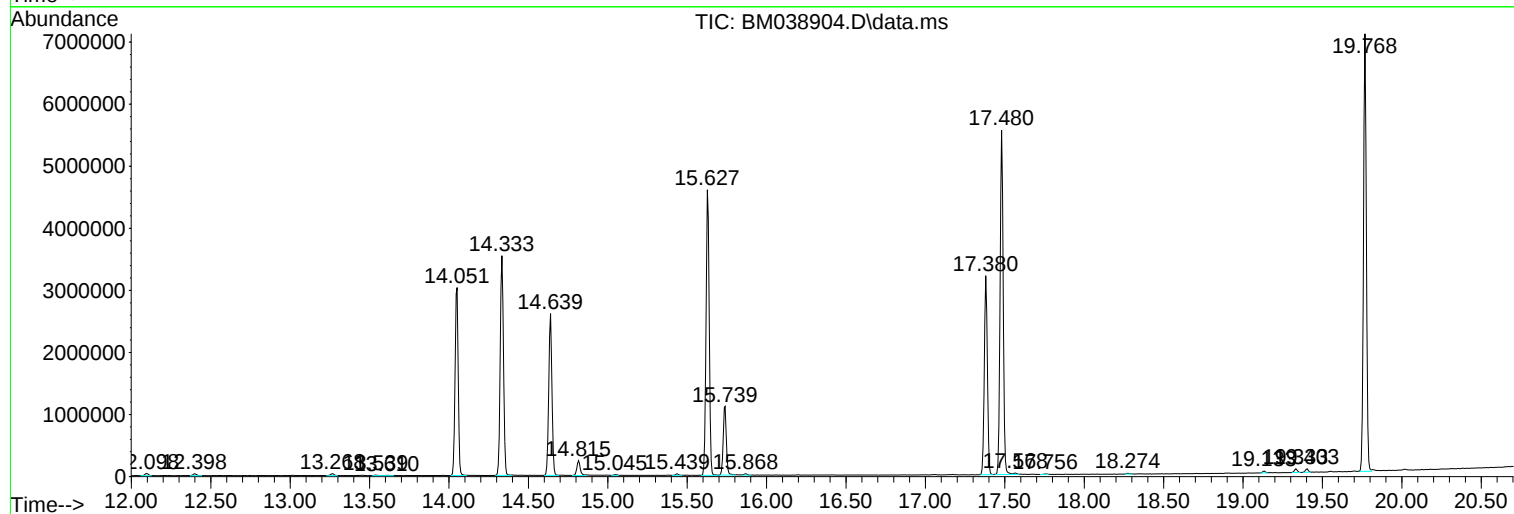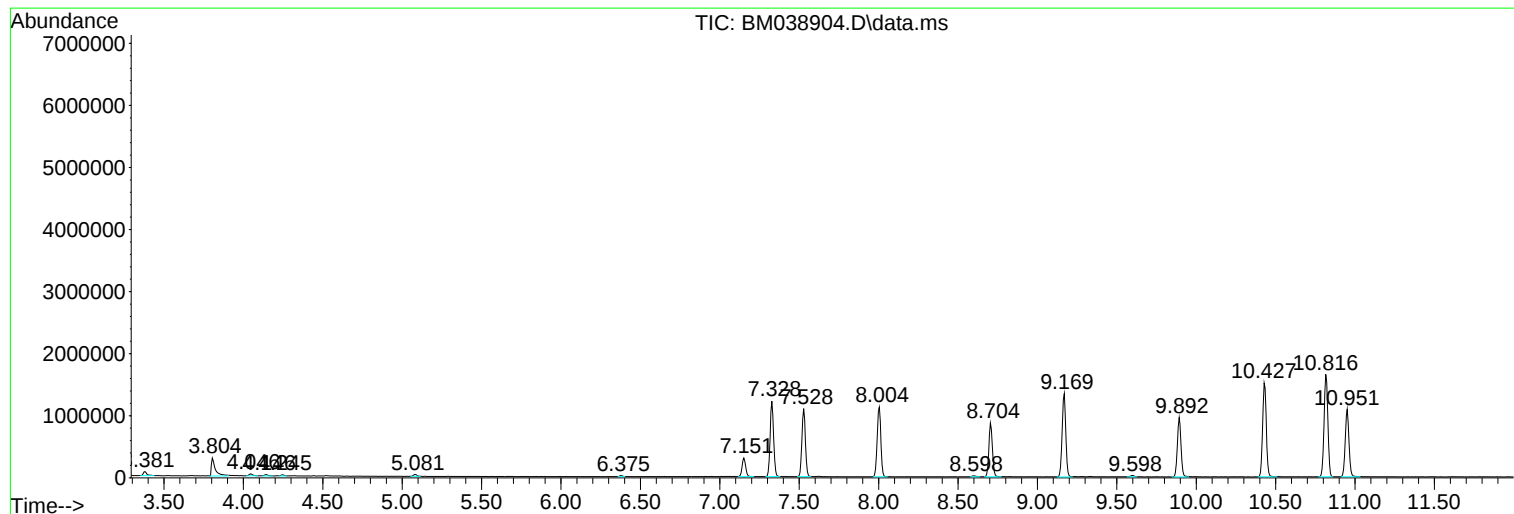

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038904.D
Acq On : 07 Mar 2023 20:23
Operator : CG/JU
Sample : 01745-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COLF1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038904.D
Acq On : 07 Mar 2023 20:23
Operator : CG/JU
Sample : 01745-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COLF1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc