

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
 Data File : BM038908.D
 Acq On : 07 Mar 2023 22:52
 Operator : CG/JU
 Sample : 01746-03DL 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCAC7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038908.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.840	92	94	103	rBV3	12998	28744	0.50%	0.060%
2	4.140	142	145	150	rVB	18585	26351	0.46%	0.055%
3	4.516	205	209	213	rBV4	14453	16683	0.29%	0.035%
4	5.992	456	460	467	rVB	19533	29264	0.51%	0.061%
5	7.151	650	657	663	rVB2	34659	55138	0.96%	0.115%
6	7.328	681	687	693	rBV	142604	224571	3.93%	0.469%
7	7.528	713	721	728	rVB	121804	195046	3.41%	0.408%
8	7.722	746	754	762	rBV	58780	99546	1.74%	0.208%
9	7.998	793	801	809	rBV	1133610	1825674	31.92%	3.815%
10	8.110	817	820	828	rVB4	10575	17968	0.31%	0.038%
11	8.545	888	894	898	rVB	28356	46705	0.82%	0.098%
12	8.704	915	921	928	rVV	91437	146970	2.57%	0.307%
13	8.851	940	946	951	rBV	92756	145608	2.55%	0.304%
14	9.163	994	999	1009	rVB	143036	253887	4.44%	0.531%
15	9.369	1030	1034	1038	rVB3	14961	22997	0.40%	0.048%
16	9.428	1038	1044	1048	rBV3	16140	27851	0.49%	0.058%
17	9.492	1048	1055	1061	rVV	35990	78910	1.38%	0.165%
18	9.551	1061	1065	1070	rVV3	14988	26393	0.46%	0.055%
19	9.892	1116	1123	1131	rBV	98005	170277	2.98%	0.356%
20	10.010	1137	1143	1148	rBV3	15206	27406	0.48%	0.057%
21	10.216	1172	1178	1186	rBV10	11786	27001	0.47%	0.056%
22	10.427	1208	1214	1221	rBV	172483	308973	5.40%	0.646%
23	10.816	1271	1280	1284	rVV	1708957	2839056	49.63%	5.933%
24	10.869	1284	1289	1297	rVV	3497161	5720010	100.00%	11.953%
25	10.951	1297	1303	1305	rVV	164925	280531	4.90%	0.586%
26	10.986	1305	1309	1318	rVB	353723	603132	10.54%	1.260%
27	11.833	1447	1453	1457	rBV2	18575	32049	0.56%	0.067%
28	11.927	1466	1469	1474	rVB5	12603	20574	0.36%	0.043%
29	12.369	1535	1544	1547	rBV	24963	42123	0.74%	0.088%
30	12.410	1547	1551	1555	rVV5	14104	21255	0.37%	0.044%
31	12.469	1555	1561	1570	rVV	358986	581971	10.17%	1.216%
32	12.586	1574	1581	1587	rVV4	13523	30906	0.54%	0.065%
33	12.686	1588	1598	1604	rVB	282930	458910	8.02%	0.959%
34	12.792	1611	1616	1618	rBV2	16771	22206	0.39%	0.046%
35	12.833	1618	1623	1629	rVB6	15143	27836	0.49%	0.058%
36	13.133	1665	1674	1678	rBV8	24351	61130	1.07%	0.128%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
 Data File : BM038908.D
 Acq On : 07 Mar 2023 22:52
 Operator : CG/JU
 Sample : 01746-03DL 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCAC7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Title : SVOA CALIBRATION

37	13.168	1678	1680	1686	rVB3	18762	25247	0.44%	0.053%
38	13.474	1727	1732	1737	rVV	192175	275708	4.82%	0.576%
39	13.668	1762	1765	1775	rVB5	13047	33231	0.58%	0.069%
40	13.804	1778	1788	1797	rBV10	32425	86580	1.51%	0.181%
41	13.957	1808	1814	1820	rBV3	36320	68200	1.19%	0.143%
42	14.045	1820	1829	1835	rBV	400812	558415	9.76%	1.167%
43	14.121	1839	1842	1847	rVB4	15210	22597	0.40%	0.047%
44	14.192	1851	1854	1858	rBV4	15587	21466	0.38%	0.045%
45	14.333	1871	1878	1887	rBV	380676	613453	10.72%	1.282%
46	14.463	1893	1900	1904	rBV8	15013	23081	0.40%	0.048%
47	14.639	1921	1930	1936	rBV	2709303	3856605	67.42%	8.059%
48	14.698	1936	1940	1946	rVV	494465	719586	12.58%	1.504%
49	14.762	1946	1951	1956	rVV	208616	295153	5.16%	0.617%
50	14.815	1956	1960	1971	rVB7	29627	61915	1.08%	0.129%
51	14.910	1971	1976	1980	rBV2	41440	61587	1.08%	0.129%
52	15.033	1991	1997	2003	rVB	433778	616795	10.78%	1.289%
53	15.174	2016	2021	2026	rBV	98775	156152	2.73%	0.326%
54	15.215	2026	2028	2031	rVV4	14305	19102	0.33%	0.040%
55	15.257	2031	2035	2039	rVB3	34019	50044	0.87%	0.105%
56	15.551	2082	2085	2092	rVV6	11203	19799	0.35%	0.041%
57	15.627	2092	2098	2103	rVV	562432	814660	14.24%	1.702%
58	15.680	2103	2107	2112	rVV	228220	309100	5.40%	0.646%
59	15.739	2112	2117	2123	rVV2	121759	214752	3.75%	0.449%
60	15.809	2124	2129	2137	rVV4	26352	64460	1.13%	0.135%
61	15.898	2141	2144	2148	rVB3	15882	19885	0.35%	0.042%
62	15.980	2153	2158	2163	rVV6	27747	64353	1.13%	0.134%
63	16.057	2166	2171	2176	rVV7	27798	54208	0.95%	0.113%
64	16.121	2178	2182	2189	rVB3	27535	50630	0.89%	0.106%
65	16.292	2208	2211	2215	rVV4	15642	26859	0.47%	0.056%
66	16.351	2215	2221	2231	rVB2	51410	104202	1.82%	0.218%
67	16.556	2247	2256	2262	rBV9	9549	26467	0.46%	0.055%
68	16.633	2262	2269	2275	rBV	152135	220999	3.86%	0.462%
69	17.027	2327	2336	2343	rVB2	213375	358996	6.28%	0.750%
70	17.156	2352	2358	2362	rBV8	17559	45634	0.80%	0.095%
71	17.198	2362	2365	2370	rVB	28848	40727	0.71%	0.085%
72	17.327	2384	2387	2390	rBV	26502	33644	0.59%	0.070%
73	17.380	2390	2396	2401	rVV	3424434	4702946	82.22%	9.827%
74	17.421	2401	2403	2408	rVV2	283134	367115	6.42%	0.767%
75	17.480	2408	2413	2424	rVB	632910	952672	16.66%	1.991%
76	17.692	2442	2449	2453	rVB8	18391	34271	0.60%	0.072%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
 Data File : BM038908.D
 Acq On : 07 Mar 2023 22:52
 Operator : CG/JU
 Sample : 01746-03DL 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCAC7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Title : SVOA CALIBRATION

77	17.780	2455	2464	2471	rBV	1194821	1628249	28.47%	3.402%
78	17.839	2471	2474	2477	rVV4	14793	19091	0.33%	0.040%
79	17.933	2485	2490	2497	rVB	157528	223449	3.91%	0.467%
80	18.215	2534	2538	2542	rVB2	21231	24909	0.44%	0.052%
81	18.268	2543	2547	2550	rBV	66861	96714	1.69%	0.202%
82	18.374	2562	2565	2572	rVB2	34559	50537	0.88%	0.106%
83	18.445	2573	2577	2578	rBV4	12902	17623	0.31%	0.037%
84	18.598	2600	2603	2606	rBV3	15095	20220	0.35%	0.042%
85	18.692	2615	2619	2624	rBV4	31350	53046	0.93%	0.111%
86	18.745	2624	2628	2633	rBV5	23985	35144	0.61%	0.073%
87	19.086	2683	2686	2689	rBV4	20215	23246	0.41%	0.049%
88	19.168	2698	2700	2704	rVB4	20484	21595	0.38%	0.045%
89	19.397	2737	2739	2742	rBV3	15616	19490	0.34%	0.041%
90	19.545	2761	2764	2769	rVB5	41213	45690	0.80%	0.095%
91	19.762	2796	2801	2807	rBV	830560	1148968	20.09%	2.401%
92	20.809	2976	2979	2982	rBV2	75410	83950	1.47%	0.175%
93	21.274	3054	3058	3063	rVB	235034	275434	4.82%	0.576%
94	21.556	3101	3106	3112	rBV	4127678	5173301	90.44%	10.810%
95	21.721	3130	3134	3139	rBV	313170	364424	6.37%	0.762%
96	22.191	3210	3214	3219	rVB	345520	437000	7.64%	0.913%
97	22.703	3297	3301	3307	rVB	279711	405174	7.08%	0.847%
98	23.274	3394	3398	3404	rVB	221818	333460	5.83%	0.697%
99	23.844	3490	3495	3503	rVB2	543539	1030989	18.02%	2.154%
100	24.009	3515	3523	3535	rVB2	2777467	5688912	99.46%	11.888%




Sum of corrected areas: 47855563

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038908.D
Acq On : 07 Mar 2023 22:52
Operator : CG/JU
Sample : 01746-03DL 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCAC7DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

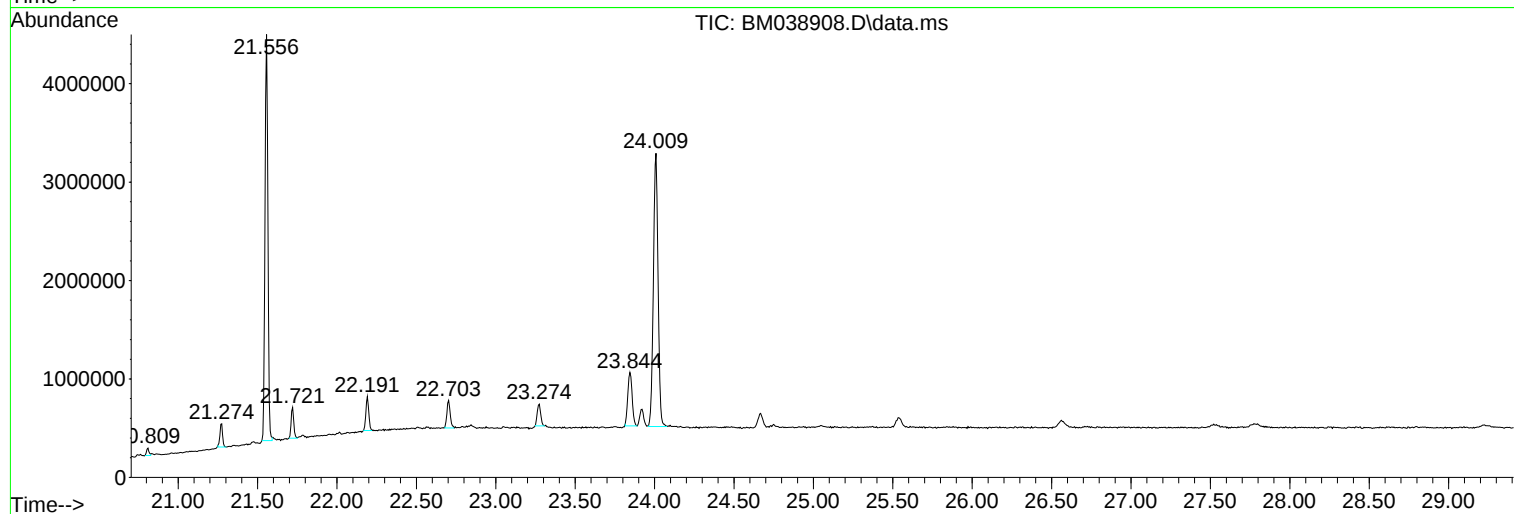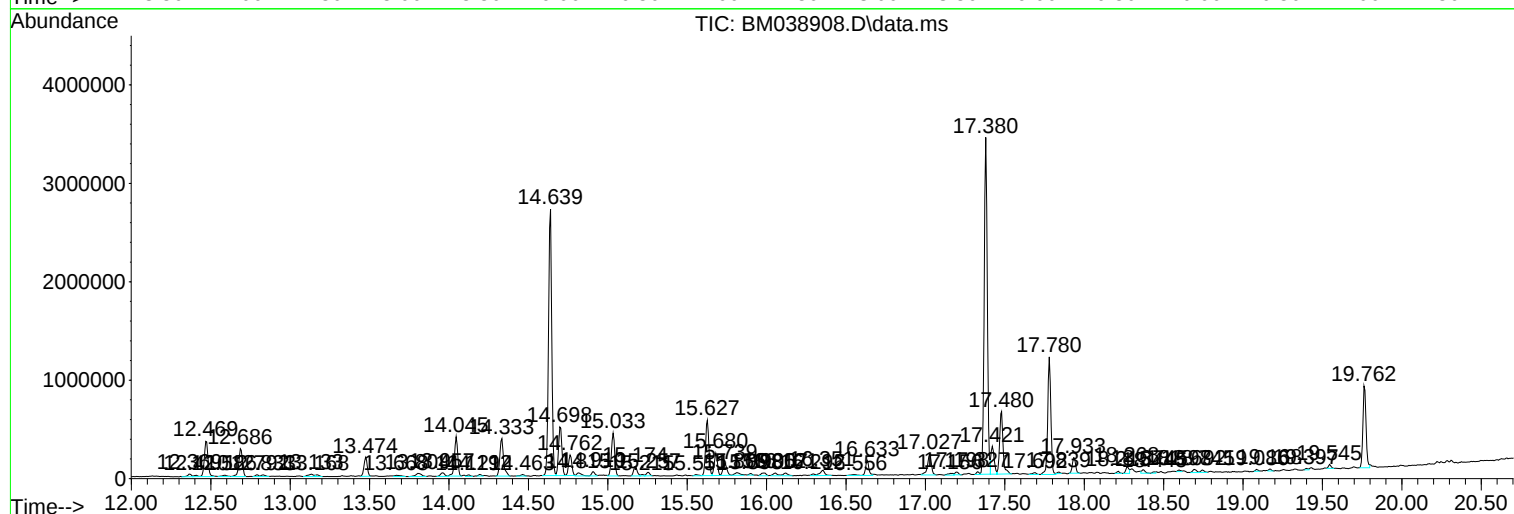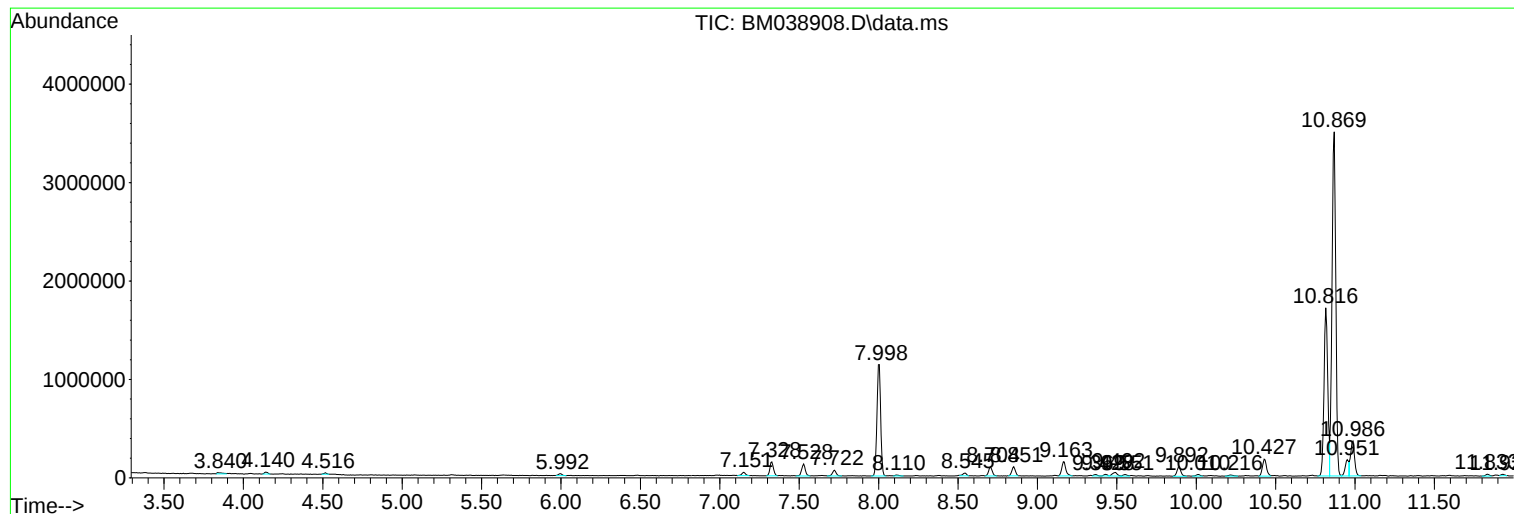

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038908.D
Acq On : 07 Mar 2023 22:52
Operator : CG/JU
Sample : 01746-03DL 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCAC7DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038908.D
Acq On : 07 Mar 2023 22:52
Operator : CG/JU
Sample : 01746-03DL 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCAC7DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc