

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
 Data File : BM038910.D
 Acq On : 08 Mar 2023 00:06
 Operator : CG/JU
 Sample : 01746-05DL 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCAD5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038910.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	12	16	23	rVB4	16560	28460	0.45%	0.054%
2	3.816	88	90	107	rBV	55691	106460	1.67%	0.202%
3	4.140	141	145	152	rVB2	21385	32718	0.51%	0.062%
4	5.340	346	349	356	rVB6	15404	27023	0.42%	0.051%
5	5.993	455	460	466	rVV	18578	33459	0.53%	0.064%
6	7.151	651	657	666	rVB	55804	97005	1.52%	0.184%
7	7.328	679	687	694	rBV	256217	411972	6.47%	0.783%
8	7.528	713	721	730	rVB	209466	344801	5.41%	0.655%
9	7.722	746	754	762	rBV	45333	78761	1.24%	0.150%
10	7.998	795	801	809	rBV	1062483	1697364	26.65%	3.225%
11	8.116	816	821	827	rVB4	11470	19929	0.31%	0.038%
12	8.540	884	893	899	rBV	34677	62625	0.98%	0.119%
13	8.704	915	921	930	rVB	161523	259106	4.07%	0.492%
14	8.851	939	946	954	rVB	58410	93842	1.47%	0.178%
15	9.163	993	999	1009	rVV	272885	478660	7.52%	0.909%
16	9.275	1013	1018	1024	rVV	40875	69415	1.09%	0.132%
17	9.363	1030	1033	1040	rVB3	20717	34738	0.55%	0.066%
18	9.487	1047	1054	1061	rVV3	38666	89220	1.40%	0.170%
19	9.551	1061	1065	1070	rVV2	16731	29439	0.46%	0.056%
20	9.892	1115	1123	1131	rBV	186962	311627	4.89%	0.592%
21	10.222	1173	1179	1183	rBV5	10592	19089	0.30%	0.036%
22	10.428	1207	1214	1224	rBV	318268	525641	8.25%	0.999%
23	10.816	1270	1280	1284	rBV	1550500	2648804	41.59%	5.033%
24	10.869	1284	1289	1297	rVV	3947778	6368250	100.00%	12.099%
25	10.951	1297	1303	1305	rVV	283941	476710	7.49%	0.906%
26	10.986	1305	1309	1319	rVB	337245	590346	9.27%	1.122%
27	11.928	1464	1469	1475	rVB4	20791	39234	0.62%	0.075%
28	12.128	1499	1503	1511	rVV8	9443	22030	0.35%	0.042%
29	12.363	1538	1543	1548	rVV	36123	60938	0.96%	0.116%
30	12.469	1554	1561	1568	rVV	385599	595407	9.35%	1.131%
31	12.586	1576	1581	1588	rVV3	12696	26226	0.41%	0.050%
32	12.686	1588	1598	1605	rVV	252871	411489	6.46%	0.782%
33	12.828	1618	1622	1628	rVB3	16851	26755	0.42%	0.051%
34	13.110	1664	1670	1672	rBV6	14961	24135	0.38%	0.046%
35	13.133	1672	1674	1678	rVV5	18693	29373	0.46%	0.056%
36	13.169	1678	1680	1686	rVB5	13710	20027	0.31%	0.038%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
 Data File : BM038910.D
 Acq On : 08 Mar 2023 00:06
 Operator : CG/JU
 Sample : 01746-05DL 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCAD5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Title : SVOA CALIBRATION

37	13.328	1702	1707	1711	rBV5	13340	22670	0.36%	0.043%
38	13.475	1726	1732	1741	rVB	192423	284558	4.47%	0.541%
39	13.651	1757	1762	1764	rVV6	15975	30701	0.48%	0.058%
40	13.698	1768	1770	1777	rVB7	15230	20138	0.32%	0.038%
41	13.810	1782	1789	1795	rVV7	36550	77343	1.21%	0.147%
42	13.957	1807	1814	1819	rVV2	28860	56824	0.89%	0.108%
43	14.045	1819	1829	1834	rVV	740937	1003881	15.76%	1.907%
44	14.092	1834	1837	1840	rVV5	10403	19086	0.30%	0.036%
45	14.192	1850	1854	1858	rVV4	16494	26248	0.41%	0.050%
46	14.333	1871	1878	1889	rVB2	697577	1172582	18.41%	2.228%
47	14.463	1896	1900	1908	rVB2	19981	38339	0.60%	0.073%
48	14.639	1921	1930	1936	rVV	2397785	3549333	55.73%	6.744%
49	14.698	1936	1940	1946	rVV	397821	585542	9.19%	1.112%
50	14.763	1946	1951	1956	rVV	246669	354687	5.57%	0.674%
51	14.816	1956	1960	1971	rVV3	45980	85466	1.34%	0.162%
52	14.904	1971	1975	1979	rVV6	12598	20184	0.32%	0.038%
53	14.969	1984	1986	1991	rVV5	14178	24878	0.39%	0.047%
54	15.033	1991	1997	2006	rVB	660640	924606	14.52%	1.757%
55	15.169	2016	2020	2025	rBV	62589	95788	1.50%	0.182%
56	15.257	2031	2035	2040	rVB4	23415	34373	0.54%	0.065%
57	15.339	2045	2049	2057	rVB2	9747	21147	0.33%	0.040%
58	15.627	2091	2098	2102	rVV	1044560	1476736	23.19%	2.806%
59	15.680	2102	2107	2112	rVV	487481	707538	11.11%	1.344%
60	15.733	2112	2116	2124	rVV2	221371	342800	5.38%	0.651%
61	15.816	2124	2130	2137	rVV4	39437	102256	1.61%	0.194%
62	15.892	2138	2143	2147	rVV2	58116	100565	1.58%	0.191%
63	15.986	2152	2159	2165	rVV3	58882	120004	1.88%	0.228%
64	16.057	2166	2171	2176	rVV7	18575	38276	0.60%	0.073%
65	16.116	2177	2181	2192	rVB3	39257	75954	1.19%	0.144%
66	16.292	2207	2211	2214	rBV5	16832	19190	0.30%	0.036%
67	16.351	2216	2221	2228	rVB	66196	110456	1.73%	0.210%
68	16.557	2252	2256	2262	rVB	28489	43279	0.68%	0.082%
69	16.633	2264	2269	2275	rBV	84315	133631	2.10%	0.254%
70	16.998	2323	2331	2332	rVV5	37519	65021	1.02%	0.124%
71	17.027	2332	2336	2345	rVB	138557	217564	3.42%	0.413%
72	17.157	2352	2358	2362	rBV6	22957	52382	0.82%	0.100%
73	17.198	2362	2365	2369	rVB	42996	56797	0.89%	0.108%
74	17.327	2384	2387	2390	rBV3	21137	28226	0.44%	0.054%
75	17.380	2390	2396	2401	rVV	3065403	4248415	66.71%	8.072%
76	17.421	2401	2403	2407	rVV	199657	248614	3.90%	0.472%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
 Data File : BM038910.D
 Acq On : 08 Mar 2023 00:06
 Operator : CG/JU
 Sample : 01746-05DL 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCAD5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Title : SVOA CALIBRATION

77	17.480	2407	2413	2422	rVB	1134338	1649453	25.90%	3.134%
78	17.615	2433	2436	2442	rVB8	13430	26934	0.42%	0.051%
79	17.692	2445	2449	2453	rVB5	16629	22393	0.35%	0.043%
80	17.780	2454	2464	2470	rBV	1156329	1558621	24.47%	2.961%
81	17.933	2486	2490	2497	rBV	63984	92716	1.46%	0.176%
82	18.215	2535	2538	2542	rVB3	15734	20904	0.33%	0.040%
83	18.274	2543	2548	2557	rBV2	97836	208124	3.27%	0.395%
84	18.368	2562	2564	2568	rVB	23289	30915	0.49%	0.059%
85	18.533	2588	2592	2594	rBV3	15260	24951	0.39%	0.047%
86	18.704	2616	2621	2624	rVB4	37501	52453	0.82%	0.100%
87	19.251	2711	2714	2720	rBV6	15986	28461	0.45%	0.054%
88	19.404	2737	2740	2741	rBV2	19014	19193	0.30%	0.036%
89	19.427	2742	2744	2752	rVB	36066	48149	0.76%	0.091%
90	19.545	2761	2764	2768	rBV4	48840	58909	0.93%	0.112%
91	19.762	2796	2801	2811	rBV	1465549	2031211	31.90%	3.859%
92	20.809	2976	2979	2981	rBV2	67328	70914	1.11%	0.135%
93	21.274	3054	3058	3062	rVB	236080	294142	4.62%	0.559%
94	21.556	3101	3106	3112	rBV	3648605	4732222	74.31%	8.991%
95	21.721	3130	3134	3138	rBV	296032	346050	5.43%	0.657%
96	22.192	3210	3214	3220	rVB	322895	410021	6.44%	0.779%
97	22.703	3297	3301	3308	rVB	252489	353270	5.55%	0.671%
98	23.274	3394	3398	3409	rVB	212292	389749	6.12%	0.741%
99	23.844	3489	3495	3503	rBV2	1054744	2035762	31.97%	3.868%
100	24.009	3516	3523	3535	rVB2	2621918	5300421	83.23%	10.071%




Sum of corrected areas: 52633094

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038910.D
Acq On : 08 Mar 2023 00:06
Operator : CG/JU
Sample : 01746-05DL 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCAD5DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

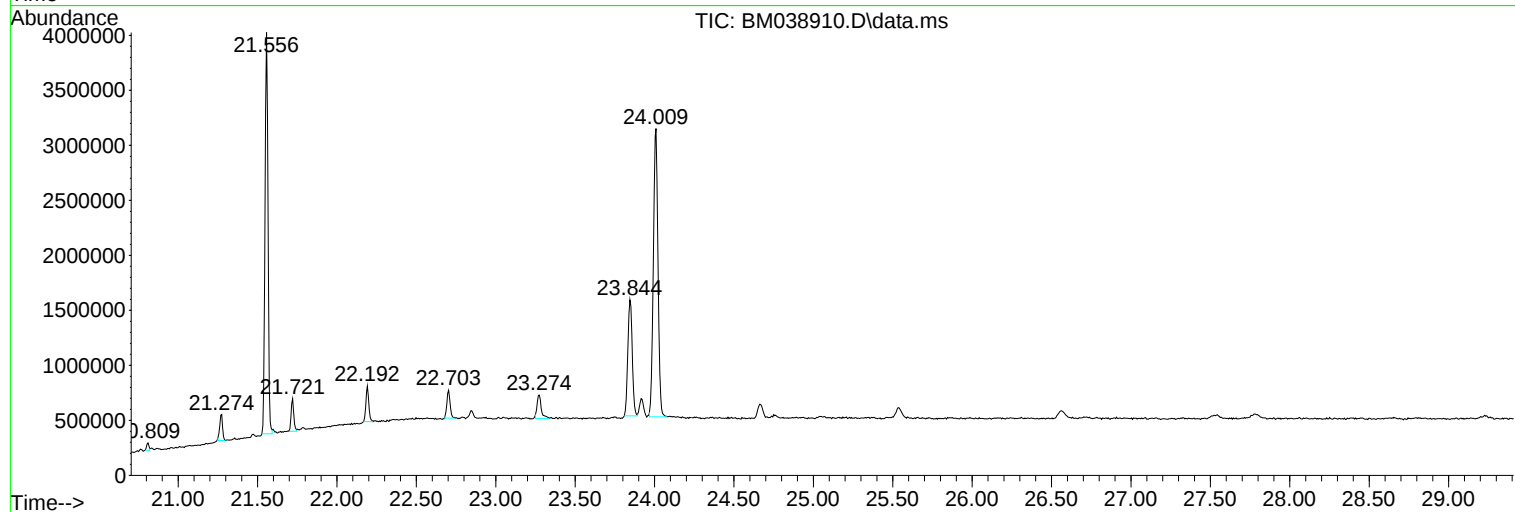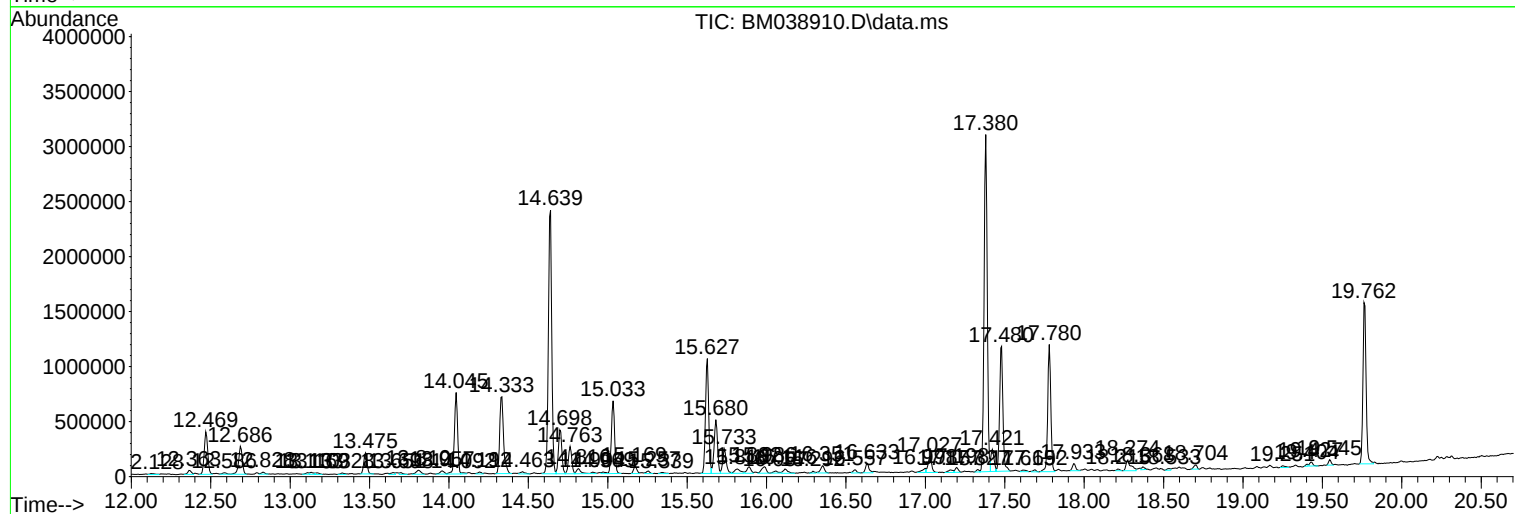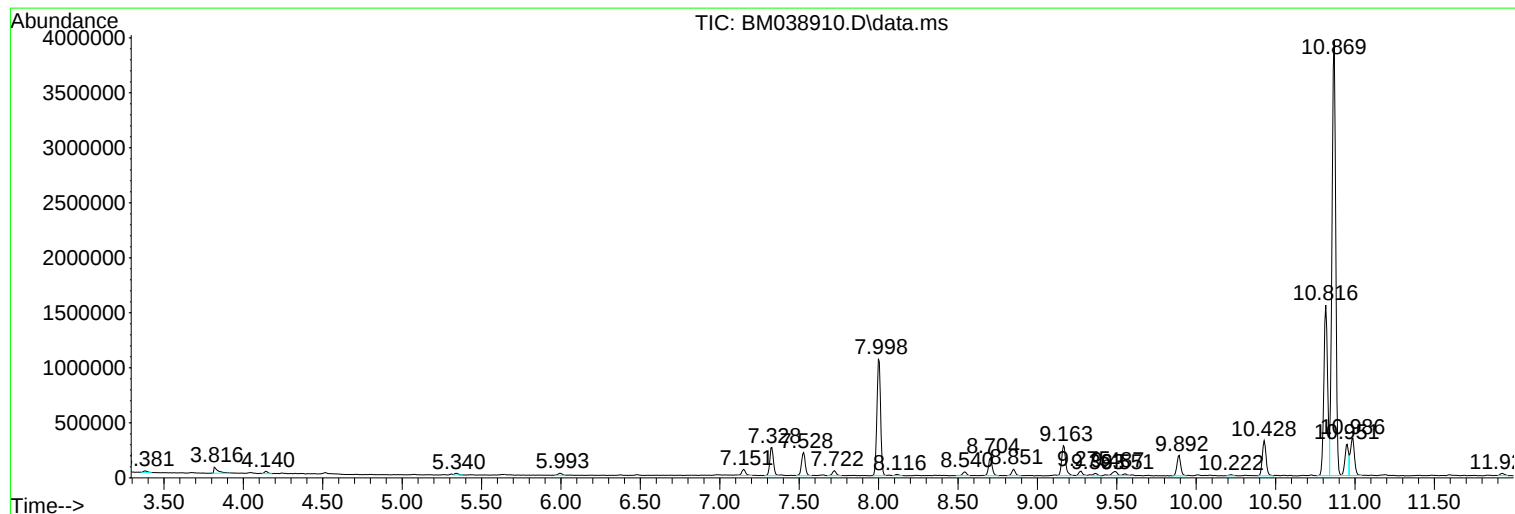

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038910.D
Acq On : 08 Mar 2023 00:06
Operator : CG/JU
Sample : 01746-05DL 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCAD5DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038910.D
Acq On : 08 Mar 2023 00:06
Operator : CG/JU
Sample : 01746-05DL 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCAD5DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc