

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
 Data File : BM038912.D
 Acq On : 08 Mar 2023 01:20
 Operator : CG/JU
 Sample : 01746-08DL 10X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCAE2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038912.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.846	93	95	100	rBV4	8496	16168	0.32%	0.039%
2	4.146	141	146	153	rVB	18721	32835	0.66%	0.079%
3	4.510	205	208	213	rVV5	10773	19096	0.38%	0.046%
4	5.993	456	460	466	rBV2	16079	25432	0.51%	0.061%
5	7.151	651	657	666	rVB	26838	48772	0.98%	0.117%
6	7.328	681	687	694	rBV	120977	191201	3.83%	0.460%
7	7.528	715	721	728	rVB	97890	156717	3.14%	0.377%
8	7.722	748	754	760	rVB	54397	89642	1.79%	0.215%
9	7.998	794	801	808	rBV	1018964	1598529	32.00%	3.843%
10	8.116	815	821	831	rVB3	9492	18280	0.37%	0.044%
11	8.539	887	893	900	rBV	32719	52009	1.04%	0.125%
12	8.704	915	921	933	rVB	75262	128847	2.58%	0.310%
13	8.851	937	946	951	rBV	99588	159466	3.19%	0.383%
14	9.163	994	999	1009	rVV	124076	222415	4.45%	0.535%
15	9.363	1030	1033	1038	rVB2	14509	21912	0.44%	0.053%
16	9.428	1038	1044	1048	rBV2	26036	41076	0.82%	0.099%
17	9.486	1048	1054	1060	rVV	32192	70641	1.41%	0.170%
18	9.551	1060	1065	1071	rVV2	15016	28866	0.58%	0.069%
19	9.892	1115	1123	1132	rBV	82941	151783	3.04%	0.365%
20	10.016	1138	1144	1149	rBV4	12738	21777	0.44%	0.052%
21	10.216	1172	1178	1187	rBV8	12525	25201	0.50%	0.061%
22	10.428	1207	1214	1222	rBV	151559	269704	5.40%	0.648%
23	10.728	1260	1265	1270	rBV9	9069	17216	0.34%	0.041%
24	10.816	1272	1280	1284	rVV	1500240	2527822	50.61%	6.077%
25	10.863	1284	1288	1296	rVV	2402670	3950627	79.10%	9.497%
26	10.951	1296	1303	1305	rVV	139440	255263	5.11%	0.614%
27	10.981	1305	1308	1319	rVV	320436	540303	10.82%	1.299%
28	11.833	1447	1453	1457	rBV4	12682	24690	0.49%	0.059%
29	11.886	1457	1462	1465	rVV5	9926	18462	0.37%	0.044%
30	11.927	1465	1469	1477	rVB3	25306	44772	0.90%	0.108%
31	12.369	1538	1544	1547	rBV2	23954	41116	0.82%	0.099%
32	12.410	1547	1551	1555	rVV6	13343	21301	0.43%	0.051%
33	12.469	1555	1561	1573	rVV	253092	409038	8.19%	0.983%
34	12.586	1573	1581	1586	rVV3	14612	30880	0.62%	0.074%
35	12.686	1589	1598	1605	rVB	232872	388128	7.77%	0.933%
36	12.786	1610	1615	1618	rBV2	19630	25745	0.52%	0.062%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
 Data File : BM038912.D
 Acq On : 08 Mar 2023 01:20
 Operator : CG/JU
 Sample : 01746-08DL 10X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCAE2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Title : SVOA CALIBRATION

37	12.827	1618	1622	1628	rVB4	15103	24373	0.49%	0.059%
38	13.133	1666	1674	1677	rBV6	24460	62754	1.26%	0.151%
39	13.169	1678	1680	1689	rVB2	20897	28142	0.56%	0.068%
40	13.474	1726	1732	1740	rVV	177754	267327	5.35%	0.643%
41	13.810	1779	1789	1795	rBV8	26366	73630	1.47%	0.177%
42	13.957	1809	1814	1820	rBV2	30769	56396	1.13%	0.136%
43	14.045	1820	1829	1834	rBV	358514	508270	10.18%	1.222%
44	14.121	1839	1842	1846	rVV3	14463	21674	0.43%	0.052%
45	14.192	1850	1854	1857	rVV3	13284	22608	0.45%	0.054%
46	14.327	1871	1877	1887	rBV2	335226	556414	11.14%	1.338%
47	14.463	1895	1900	1908	rVB10	15612	32627	0.65%	0.078%
48	14.639	1921	1930	1935	rVV	2253702	3401570	68.10%	8.177%
49	14.698	1935	1940	1946	rVV	468742	686444	13.74%	1.650%
50	14.763	1946	1951	1956	rVV	219414	312628	6.26%	0.752%
51	14.816	1956	1960	1964	rVB3	19514	29608	0.59%	0.071%
52	14.904	1971	1975	1980	rBV3	23535	33752	0.68%	0.081%
53	15.033	1992	1997	2004	rVB	415846	591270	11.84%	1.421%
54	15.174	2014	2021	2026	rBV	98445	160251	3.21%	0.385%
55	15.251	2031	2034	2039	rVB3	38882	56688	1.13%	0.136%
56	15.627	2092	2098	2102	rBV	507229	737346	14.76%	1.773%
57	15.680	2102	2107	2112	rVV	161669	235485	4.71%	0.566%
58	15.733	2112	2116	2124	rVB3	115333	197404	3.95%	0.475%
59	15.815	2124	2130	2135	rBV4	33861	70431	1.41%	0.169%
60	15.898	2140	2144	2148	rVV6	21937	40700	0.81%	0.098%
61	15.980	2152	2158	2165	rVV3	33776	77690	1.56%	0.187%
62	16.051	2165	2170	2176	rVV8	27495	60638	1.21%	0.146%
63	16.115	2178	2181	2188	rVB3	27620	50469	1.01%	0.121%
64	16.292	2207	2211	2213	rVV3	17671	19255	0.39%	0.046%
65	16.351	2215	2221	2226	rVB2	31980	64828	1.30%	0.156%
66	16.633	2263	2269	2276	rBV	161286	246486	4.93%	0.593%
67	17.027	2327	2336	2344	rVB2	234331	381747	7.64%	0.918%
68	17.162	2353	2359	2361	rBV7	11041	23390	0.47%	0.056%
69	17.198	2362	2365	2369	rVB	31178	36663	0.73%	0.088%
70	17.268	2375	2377	2382	rVB4	15212	20007	0.40%	0.048%
71	17.327	2383	2387	2390	rBV	30178	39495	0.79%	0.095%
72	17.380	2390	2396	2400	rBV	3017761	4057143	81.23%	9.753%
73	17.421	2400	2403	2408	rVB	264328	358434	7.18%	0.862%
74	17.474	2408	2412	2418	rBV	547781	761436	15.24%	1.830%
75	17.692	2445	2449	2453	rVB6	16837	22445	0.45%	0.054%
76	17.780	2454	2464	2470	rBV	1202699	1628604	32.61%	3.915%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
 Data File : BM038912.D
 Acq On : 08 Mar 2023 01:20
 Operator : CG/JU
 Sample : 01746-08DL 10X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCAE2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Title : SVOA CALIBRATION

77	17.839	2471	2474	2477	rVB4	16281	17407	0.35%	0.042%
78	17.933	2485	2490	2496	rVB	174927	234458	4.69%	0.564%
79	18.080	2513	2515	2519	rVB2	17240	18996	0.38%	0.046%
80	18.127	2519	2523	2526	rBV6	13247	22092	0.44%	0.053%
81	18.209	2535	2537	2543	rVB2	18330	26327	0.53%	0.063%
82	18.268	2543	2547	2550	rBV2	75350	111046	2.22%	0.267%
83	18.368	2561	2564	2570	rVB2	26863	40923	0.82%	0.098%
84	18.445	2573	2577	2581	rBV4	12555	23871	0.48%	0.057%
85	18.533	2588	2592	2594	rBV3	16150	25763	0.52%	0.062%
86	18.592	2600	2602	2606	rBV	15076	18449	0.37%	0.044%
87	18.692	2615	2619	2624	rVB5	33300	50185	1.00%	0.121%
88	18.745	2624	2628	2633	rBV3	26499	36761	0.74%	0.088%
89	19.168	2698	2700	2705	rVB4	27883	29213	0.58%	0.070%
90	19.545	2761	2764	2768	rVB4	40834	49394	0.99%	0.119%
91	19.762	2796	2801	2811	rBV	772023	1087791	21.78%	2.615%
92	20.803	2976	2978	2981	rBV2	59393	63430	1.27%	0.152%
93	21.268	3054	3057	3062	rVB	218483	241611	4.84%	0.581%
94	21.556	3100	3106	3111	rBV	3368668	4537868	90.85%	10.909%
95	21.715	3130	3133	3137	rBV	267440	300571	6.02%	0.723%
96	22.186	3210	3213	3218	rVB	298819	375030	7.51%	0.902%
97	22.697	3297	3300	3308	rVB	246345	342841	6.86%	0.824%
98	23.268	3394	3397	3404	rVB	210723	307865	6.16%	0.740%
99	23.844	3490	3495	3502	rVB2	484720	899693	18.01%	2.163%
100	24.003	3515	3522	3536	rVB2	2465754	4994727	100.00%	12.007%




Sum of corrected areas: 41598566

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038912.D
Acq On : 08 Mar 2023 01:20
Operator : CG/JU
Sample : 01746-08DL 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCAE2DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

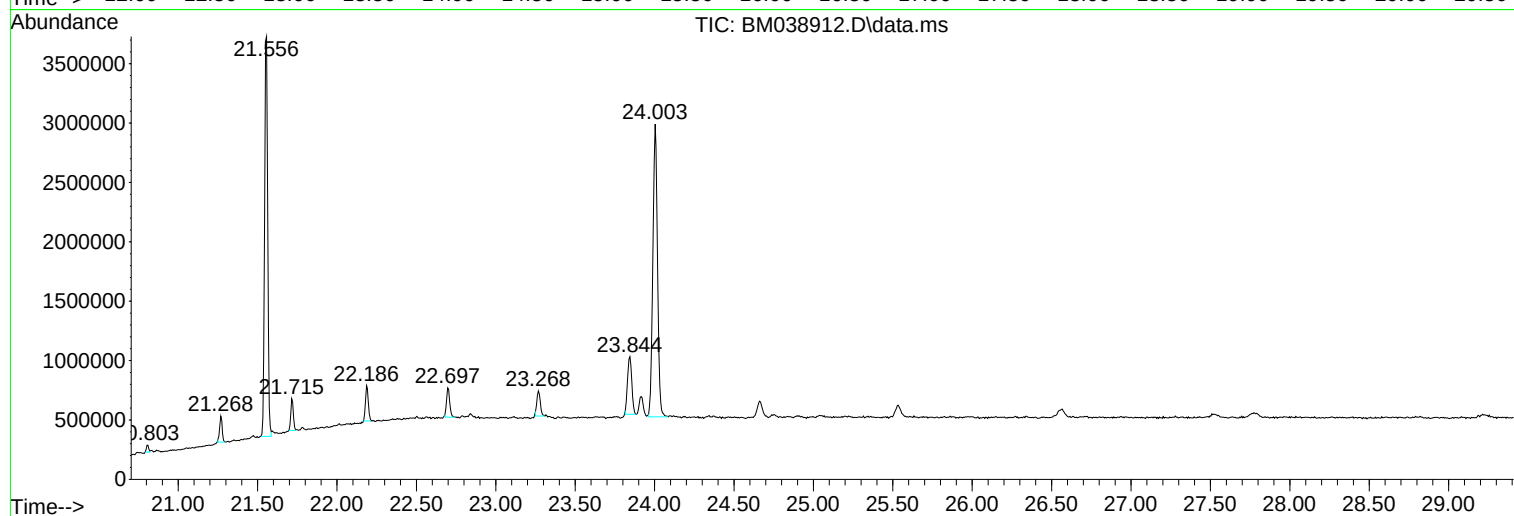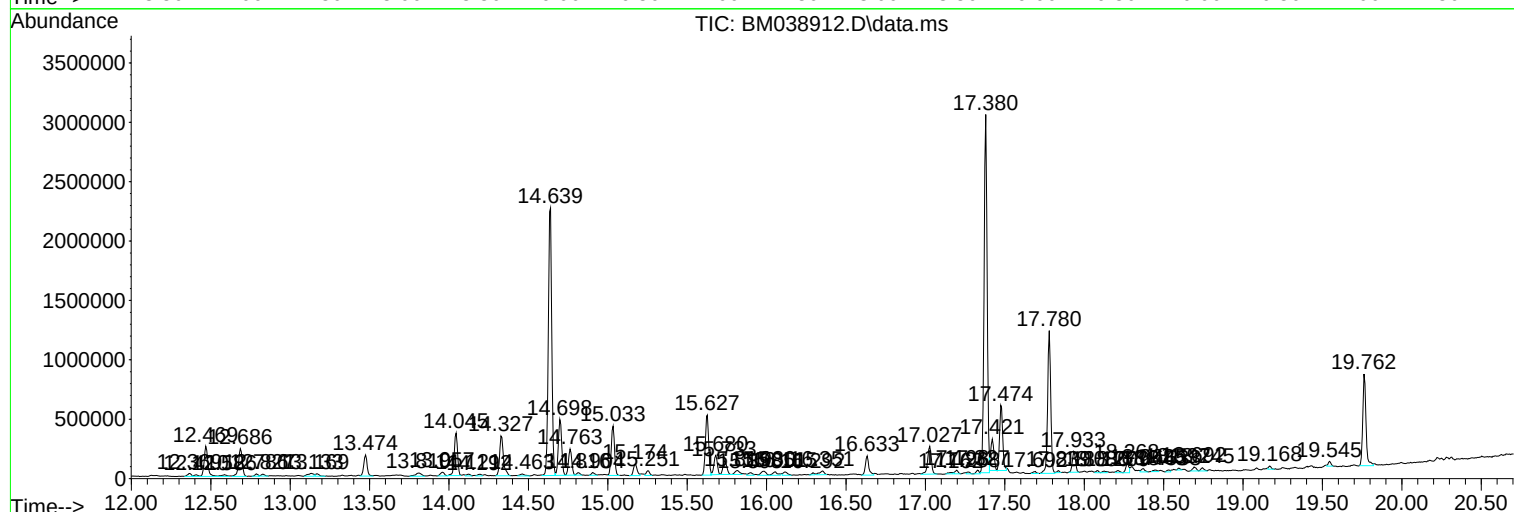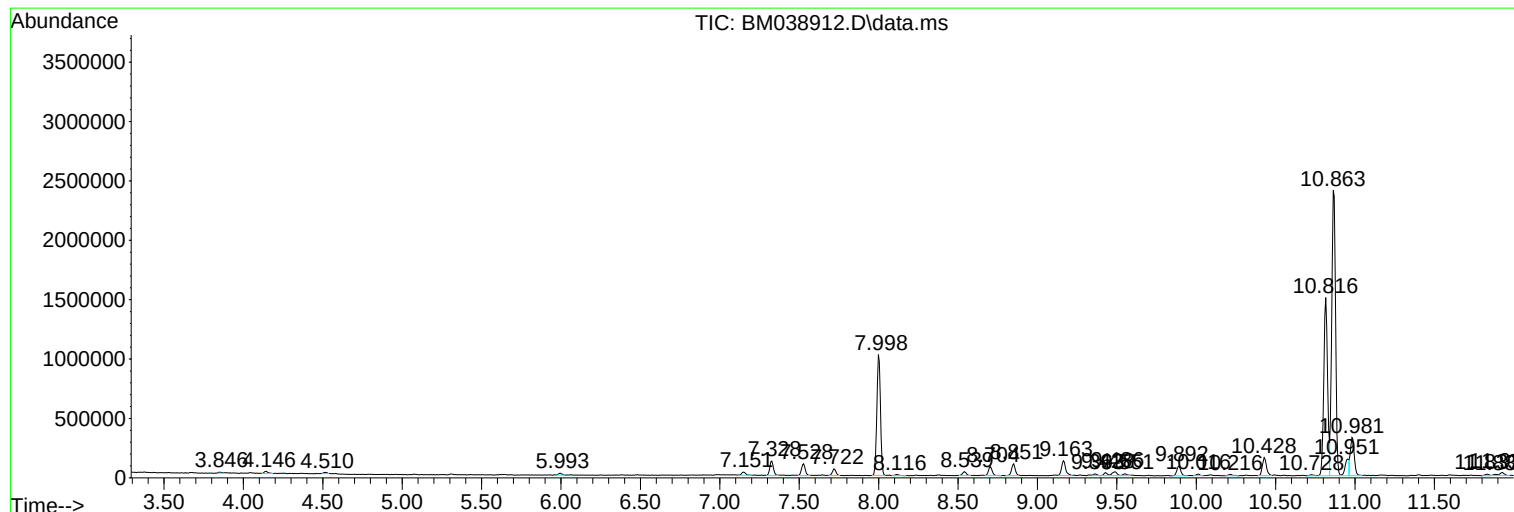

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038912.D
Acq On : 08 Mar 2023 01:20
Operator : CG/JU
Sample : 01746-08DL 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCAE2DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038912.D
Acq On : 08 Mar 2023 01:20
Operator : CG/JU
Sample : 01746-08DL 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCAE2DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc