

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
 Data File : BM038914.D
 Acq On : 08 Mar 2023 02:34
 Operator : CG/JU
 Sample : 01746-10DL 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCAE4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038914.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.846	91	95	98	rBV3	12300	22058	0.28%	0.049%
2	4.140	142	145	149	rVB2	17001	22381	0.29%	0.050%
3	5.993	454	460	466	rBV2	20078	33372	0.43%	0.074%
4	7.146	652	656	664	rVB	27583	47972	0.62%	0.107%
5	7.328	681	687	694	rBV	117497	189820	2.45%	0.423%
6	7.528	714	721	727	rBV	97772	160723	2.07%	0.358%
7	7.722	747	754	760	rVB	64795	107754	1.39%	0.240%
8	7.998	793	801	811	rBV	1074855	1691352	21.81%	3.770%
9	8.116	817	821	824	rBV	10124	14271	0.18%	0.032%
10	8.540	889	893	899	rVB	19895	35959	0.46%	0.080%
11	8.704	915	921	929	rBV2	78011	132814	1.71%	0.296%
12	8.845	940	945	953	rVB	85756	141550	1.83%	0.315%
13	9.163	993	999	1009	rVB	126349	228158	2.94%	0.509%
14	9.363	1028	1033	1039	rVB3	16551	26624	0.34%	0.059%
15	9.428	1039	1044	1047	rBV5	15571	24303	0.31%	0.054%
16	9.487	1048	1054	1060	rVV3	36110	75162	0.97%	0.168%
17	9.551	1060	1065	1070	rVB2	11981	20458	0.26%	0.046%
18	9.892	1116	1123	1129	rBV	82103	144608	1.86%	0.322%
19	10.010	1137	1143	1148	rBV4	15930	28603	0.37%	0.064%
20	10.216	1173	1178	1185	rVB10	8268	19011	0.25%	0.042%
21	10.428	1207	1214	1223	rBV	150944	267807	3.45%	0.597%
22	10.722	1259	1264	1268	rBV6	6893	11757	0.15%	0.026%
23	10.816	1272	1280	1284	rVV	1537404	2686345	34.64%	5.987%
24	10.869	1284	1289	1297	rVV	4732826	7754717	100.00%	17.283%
25	10.951	1297	1303	1304	rVV	133543	198169	2.56%	0.442%
26	10.981	1304	1308	1318	rVB	346319	623284	8.04%	1.389%
27	11.157	1334	1338	1341	rBV5	8009	12662	0.16%	0.028%
28	11.828	1447	1452	1458	rBV5	17743	32690	0.42%	0.073%
29	11.886	1458	1462	1466	rVV5	17967	28453	0.37%	0.063%
30	11.928	1466	1469	1476	rVB7	9968	19771	0.25%	0.044%
31	12.363	1537	1543	1548	rBV2	22012	40382	0.52%	0.090%
32	12.404	1548	1550	1555	rVB4	10298	11841	0.15%	0.026%
33	12.469	1555	1561	1568	rBV	537329	812166	10.47%	1.810%
34	12.586	1575	1581	1585	rBV	14974	25425	0.33%	0.057%
35	12.686	1589	1598	1608	rVB	320447	504486	6.51%	1.124%
36	12.792	1610	1616	1618	rBV2	13782	19521	0.25%	0.044%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
 Data File : BM038914.D
 Acq On : 08 Mar 2023 02:34
 Operator : CG/JU
 Sample : 01746-10DL 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCAE4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Title : SVOA CALIBRATION

37	12.827	1618	1622	1629	rVB6	13066	21610	0.28%	0.048%
38	13.057	1658	1661	1665	rVB5	8116	11205	0.14%	0.025%
39	13.127	1665	1673	1677	rVV8	19992	52537	0.68%	0.117%
40	13.169	1677	1680	1686	rVB5	14083	21314	0.27%	0.048%

41	13.333	1702	1708	1713	rBV4	14735	29413	0.38%	0.066%
42	13.475	1726	1732	1740	rVB	146597	218635	2.82%	0.487%
43	13.669	1762	1765	1768	rVV3	10174	10262	0.13%	0.023%
44	13.810	1779	1789	1796	rBV5	43272	96941	1.25%	0.216%
45	13.874	1796	1800	1806	rBV6	7475	12961	0.17%	0.029%

46	13.957	1808	1814	1819	rBV2	45923	85063	1.10%	0.190%
47	14.010	1819	1823	1824	rVV2	24725	24643	0.32%	0.055%
48	14.045	1824	1829	1835	rVB	361278	492504	6.35%	1.098%
49	14.122	1838	1842	1848	rVB7	7170	12597	0.16%	0.028%
50	14.192	1850	1854	1859	rBV3	19269	33946	0.44%	0.076%

51	14.327	1871	1877	1887	rVB	335284	567152	7.31%	1.264%
52	14.633	1917	1929	1935	rVV	2299036	3527358	45.49%	7.862%
53	14.698	1935	1940	1946	rVV	458428	644297	8.31%	1.436%
54	14.763	1946	1951	1956	rVV	202709	282300	3.64%	0.629%
55	14.827	1956	1962	1969	rVV2	56146	124701	1.61%	0.278%

56	14.904	1971	1975	1981	rBV2	60119	89339	1.15%	0.199%
57	15.033	1991	1997	2003	rVB	424862	596638	7.69%	1.330%
58	15.169	2015	2020	2026	rBV	85731	138129	1.78%	0.308%
59	15.251	2030	2034	2039	rVB3	35324	52075	0.67%	0.116%
60	15.557	2082	2086	2092	rBV	17319	30521	0.39%	0.068%

61	15.621	2092	2097	2102	rVV	496407	729271	9.40%	1.625%
62	15.680	2102	2107	2112	rVV	281745	411541	5.31%	0.917%
63	15.733	2112	2116	2124	rVB2	107505	178411	2.30%	0.398%
64	15.798	2124	2127	2130	rBV4	14310	17854	0.23%	0.040%
65	15.898	2140	2144	2147	rBV3	19465	25648	0.33%	0.057%

66	15.980	2153	2158	2163	rVB4	30558	60703	0.78%	0.135%
67	16.051	2164	2170	2173	rBV7	9755	16072	0.21%	0.036%
68	16.116	2178	2181	2189	rVB3	26106	47439	0.61%	0.106%
69	16.351	2214	2221	2233	rVB3	37917	76477	0.99%	0.170%
70	16.557	2252	2256	2260	rVB2	15673	22080	0.28%	0.049%

71	16.633	2263	2269	2276	rBV	119417	178267	2.30%	0.397%
72	16.845	2300	2305	2308	rBV7	7759	12101	0.16%	0.027%
73	17.027	2330	2336	2343	rVB2	169651	259894	3.35%	0.579%
74	17.163	2355	2359	2361	rBV4	6846	10435	0.13%	0.023%
75	17.198	2361	2365	2370	rVB2	29407	41442	0.53%	0.092%

76	17.268	2375	2377	2383	rVB4	11369	12587	0.16%	0.028%
----	--------	------	------	------	------	-------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
 Data File : BM038914.D
 Acq On : 08 Mar 2023 02:34
 Operator : CG/JU
 Sample : 01746-10DL 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCAE4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Title : SVOA CALIBRATION

77	17.327	2383	2387	2390	rBV2	22937	30921	0.40%	0.069%
78	17.380	2390	2396	2400	rBV	3005103	4214852	54.35%	9.394%
79	17.421	2400	2403	2408	rVB	307079	408868	5.27%	0.911%
80	17.474	2408	2412	2417	rBV	561790	744653	9.60%	1.660%
81	17.780	2455	2464	2471	rBV	985891	1352411	17.44%	3.014%
82	17.933	2485	2490	2495	rBV	130877	180015	2.32%	0.401%
83	18.080	2513	2515	2519	rVB5	15936	17646	0.23%	0.039%
84	18.127	2519	2523	2526	rVB6	9737	15405	0.20%	0.034%
85	18.215	2534	2538	2542	rBV3	11939	15493	0.20%	0.035%
86	18.274	2544	2548	2549	rBV2	25134	32839	0.42%	0.073%
87	18.298	2549	2552	2556	rVB2	25247	34712	0.45%	0.077%
88	18.368	2561	2564	2571	rVB	36034	54790	0.71%	0.122%
89	18.598	2598	2603	2607	rBV	65139	104531	1.35%	0.233%
90	18.692	2615	2619	2624	rVB5	24023	38307	0.49%	0.085%
91	18.745	2624	2628	2632	rBV3	16455	25502	0.33%	0.057%
92	18.792	2633	2636	2640	rVB6	13343	15252	0.20%	0.034%
93	19.251	2712	2714	2719	rBV4	15591	15691	0.20%	0.035%
94	19.398	2737	2739	2742	rBV4	14023	20751	0.27%	0.046%
95	19.427	2742	2744	2748	rVB3	18831	21830	0.28%	0.049%
96	19.545	2761	2764	2770	rVB5	32447	38780	0.50%	0.086%
97	19.762	2796	2801	2811	rBV	764678	1040484	13.42%	2.319%
98	21.556	3100	3106	3113	rBV	3608364	4765439	61.45%	10.621%
99	23.839	3489	3494	3503	rVB2	511833	961676	12.40%	2.143%
100	24.003	3515	3522	3533	rVB2	2602952	5224225	67.37%	11.644%




Sum of corrected areas: 44867865

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038914.D
Acq On : 08 Mar 2023 02:34
Operator : CG/JU
Sample : 01746-10DL 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCAE4DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

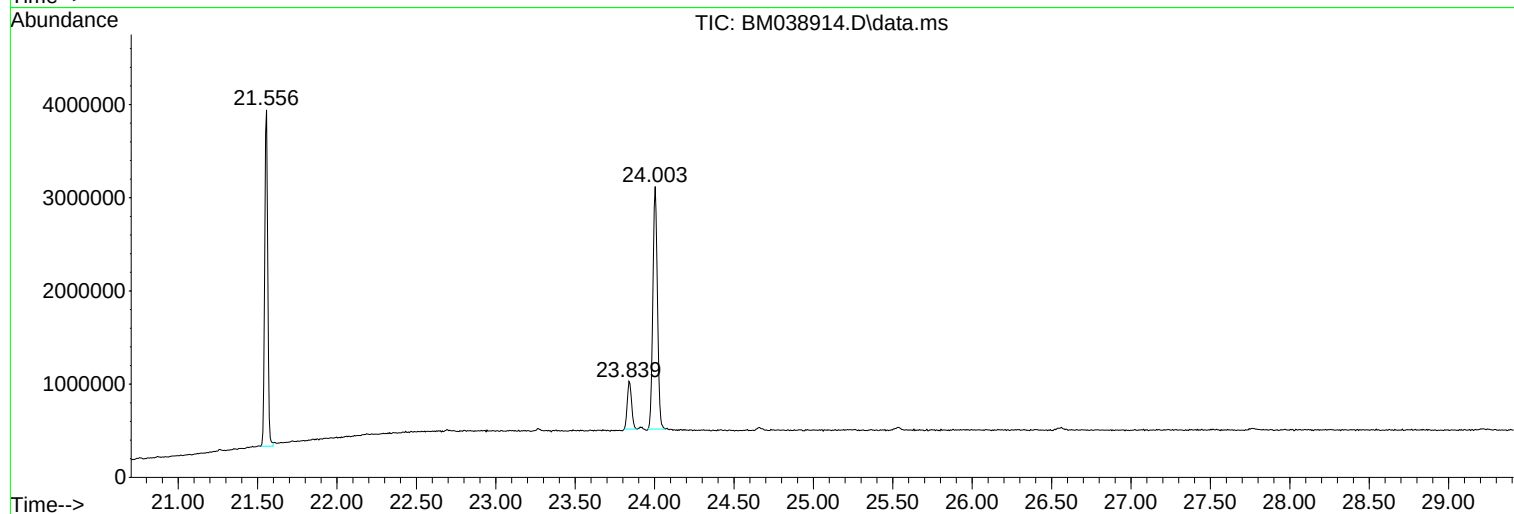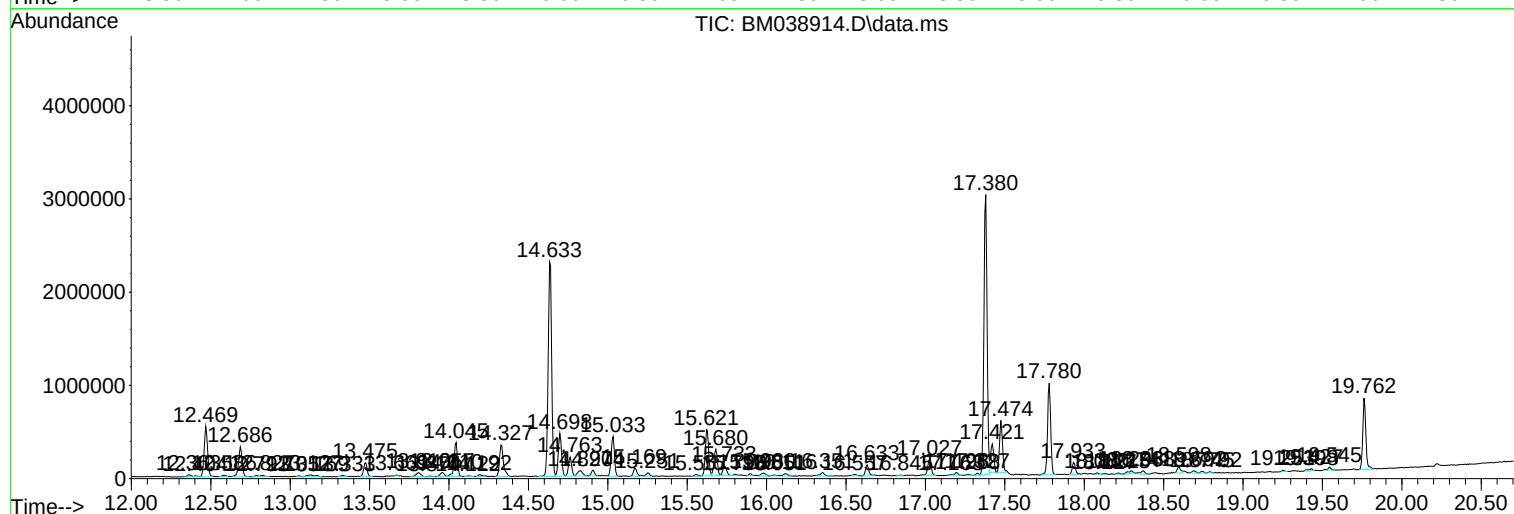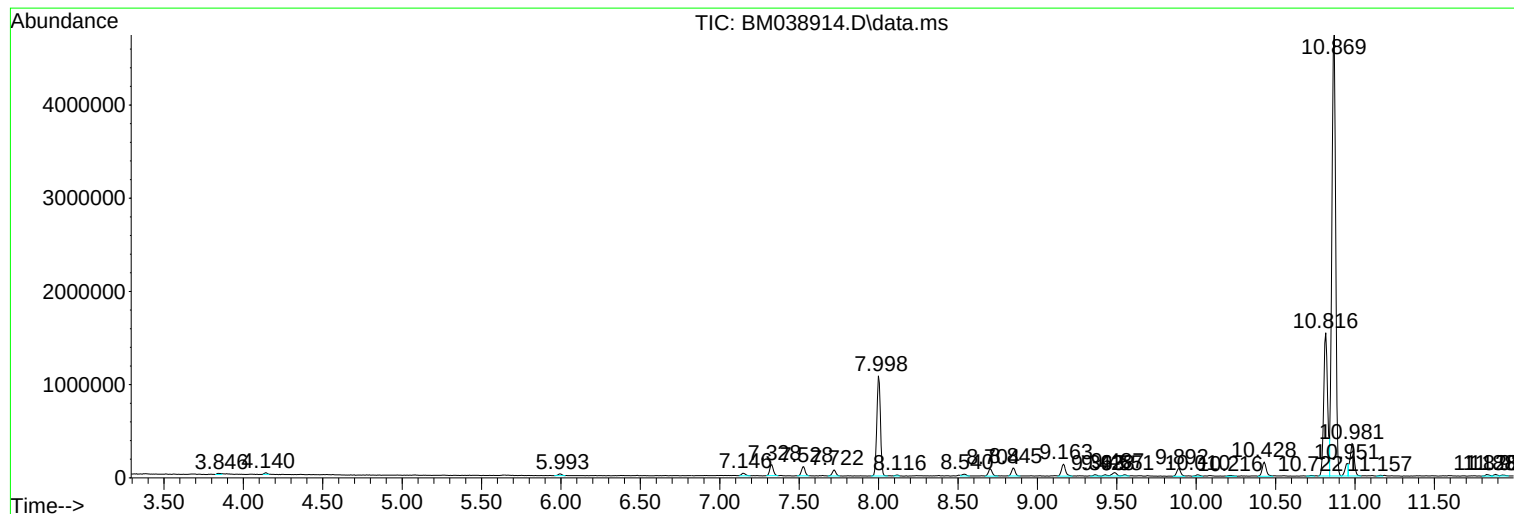

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038914.D
Acq On : 08 Mar 2023 02:34
Operator : CG/JU
Sample : 01746-10DL 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCAE4DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038914.D
Acq On : 08 Mar 2023 02:34
Operator : CG/JU
Sample : 01746-10DL 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCAE4DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
